

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053122\
 Data File : FB027324.D
 Signal(s) : FID2B.CH
 Acq On : 31 May 2022 10:41
 Operator : AJ/MA
 Sample : BSF0531S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0531S1

Integration File: Calibration.e
 Quant Time: Jun 01 03:54:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
 Quant Title :
 QLast Update : Tue May 10 13:42:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	236884	22.566 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	433645	27.250 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	495388	30.705 ng/ml
3) t n-Heptane	7.752	143720	8.795 ng/ml
4) t Benzene	7.889	202651	10.928 ng/ml
6) t Toluene	10.621	556349	31.336 ng/ml
7) t Ethylbenzene	13.057	176590	10.694 ng/ml
8) t m-Xylene	13.189	347398	21.113 ng/ml
9) t O-Xylene	13.916	342295	20.868 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	352902	21.138 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053122\
Data File : FB027324.D
Signal(s) : FID2B.CH
Acq On : 31 May 2022 10:41
Operator : AJ/MA
Sample : BSF0531S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0531S1

Integration File: Calibration.e
Quant Time: Jun 01 03:54:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

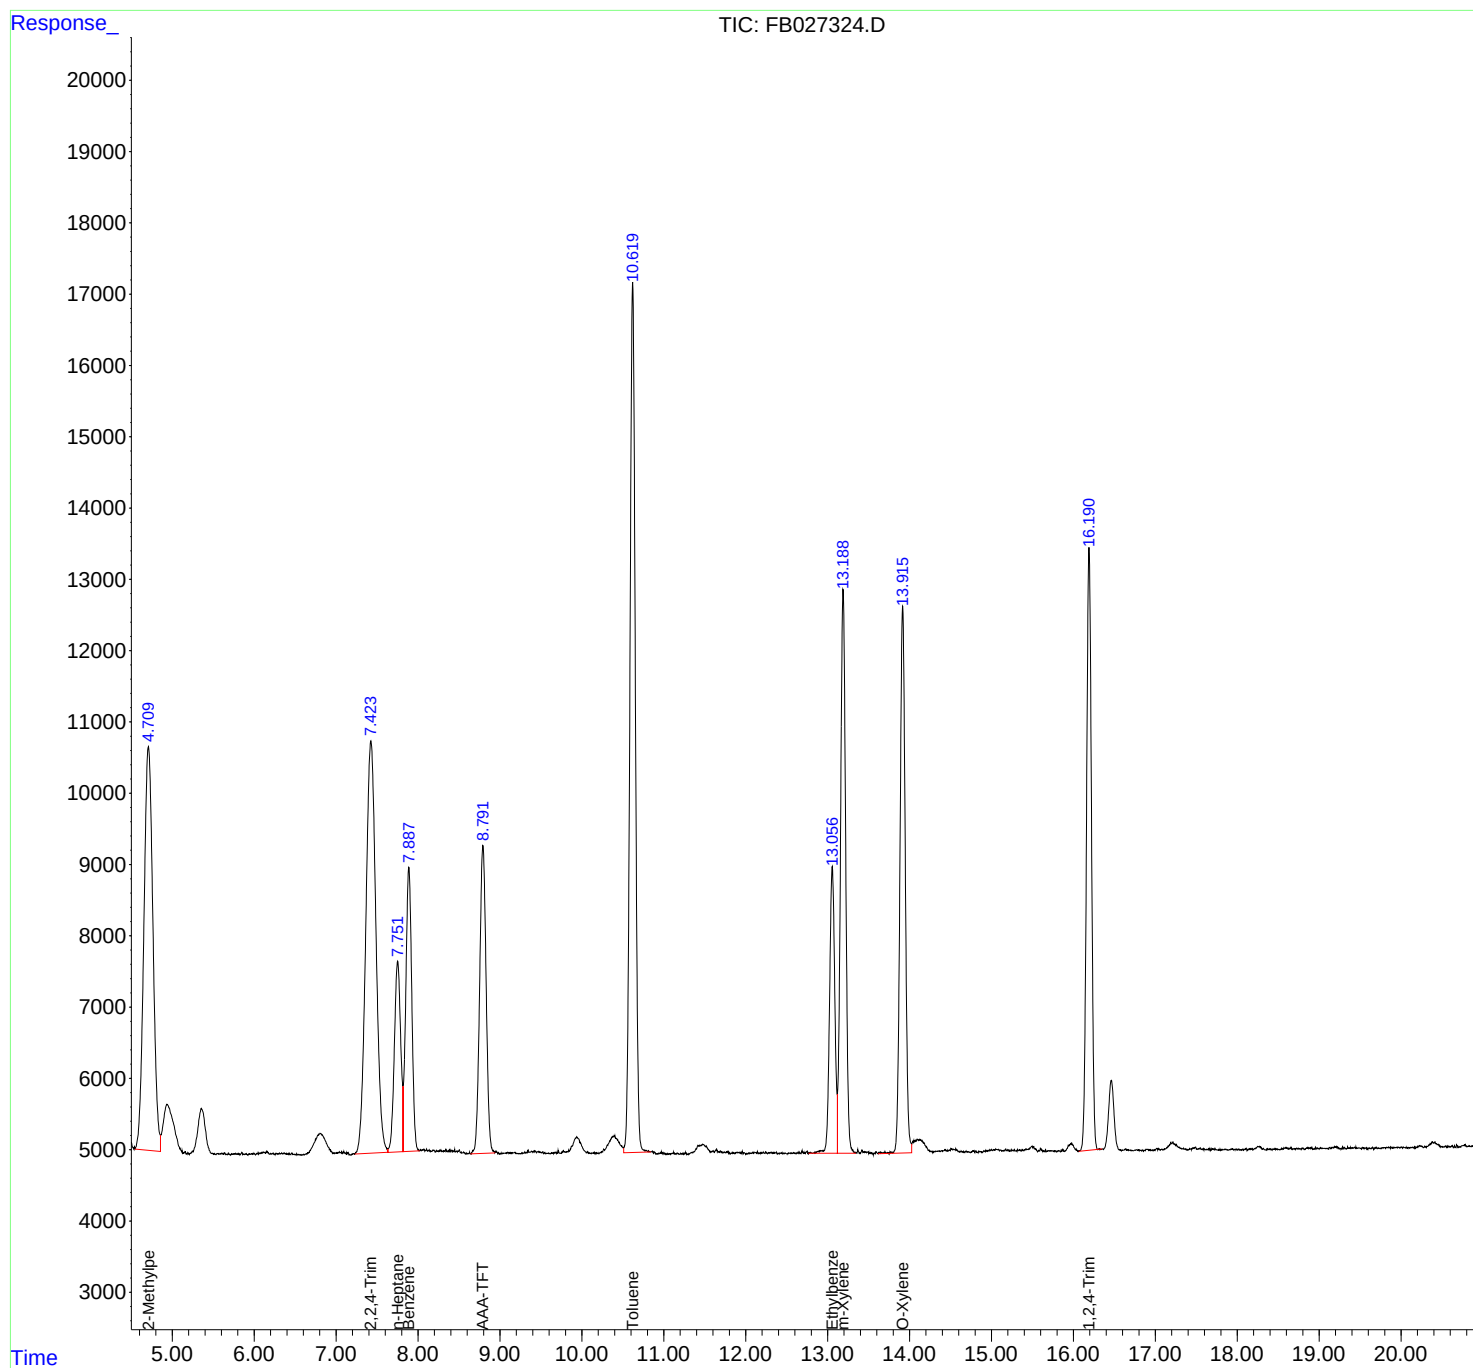


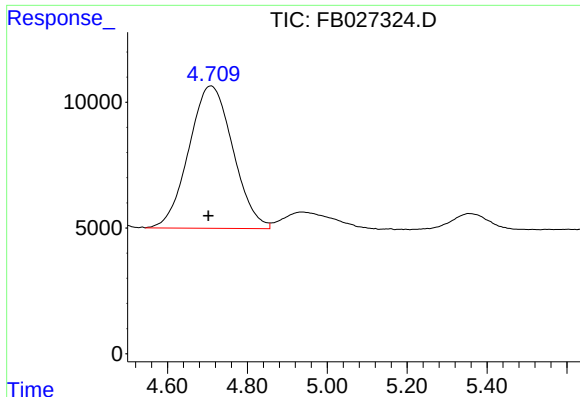

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.008 min
Response: 433645
Conc: 27.25 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0531S1

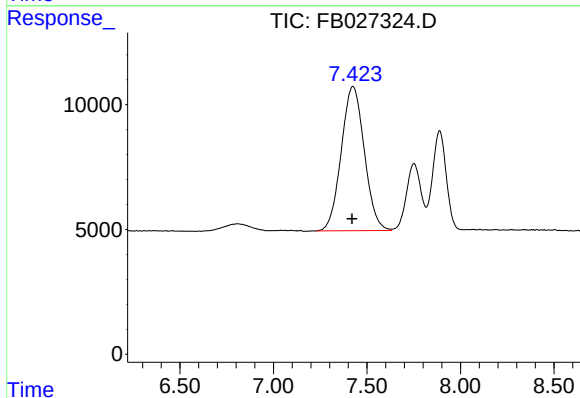


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: 0.005 min
Response: 495388
Conc: 30.70 ng/ml

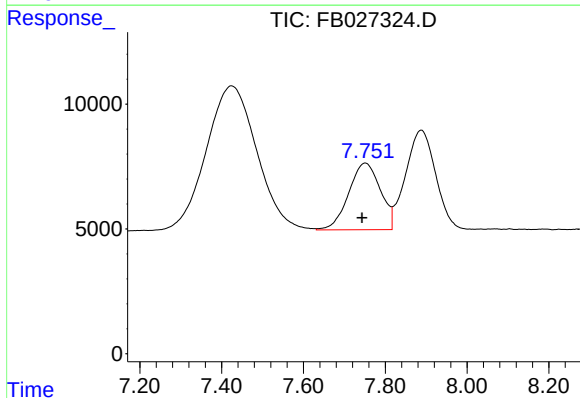


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.008 min
Response: 143720
Conc: 8.80 ng/ml

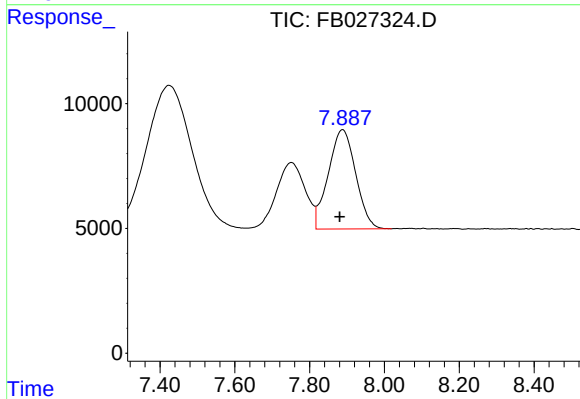

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.008 min
Response: 202651
Conc: 10.93 ng/ml

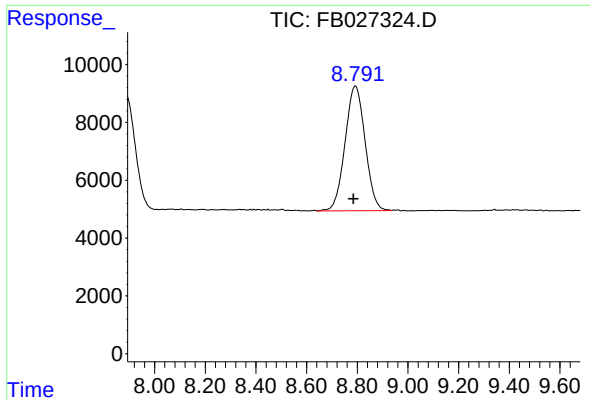

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.008 min
Response: 236884
Conc: 22.57 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0531S1

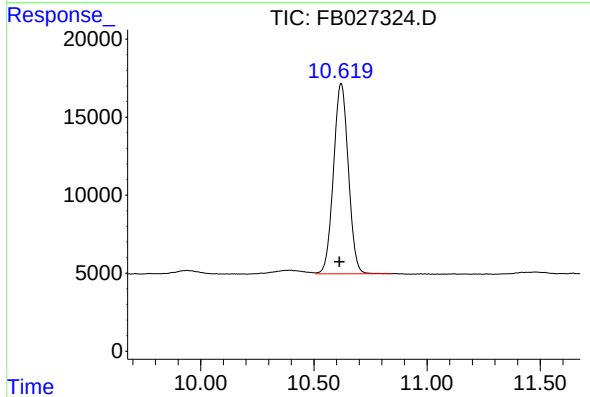


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.007 min
Response: 556349
Conc: 31.34 ng/ml

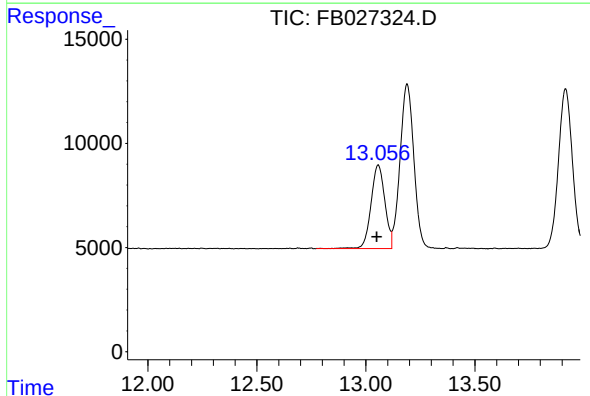


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.007 min
Response: 176590
Conc: 10.69 ng/ml

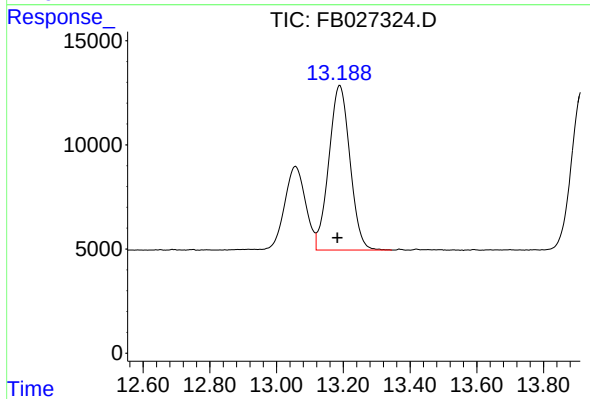

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.007 min
Response: 347398
Conc: 21.11 ng/ml

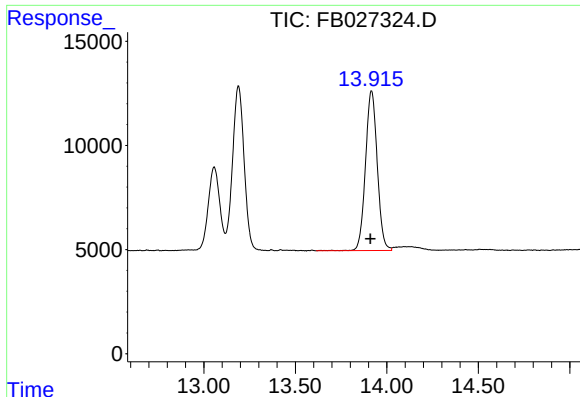

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.006 min
Response: 342295
Conc: 20.87 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0531S1

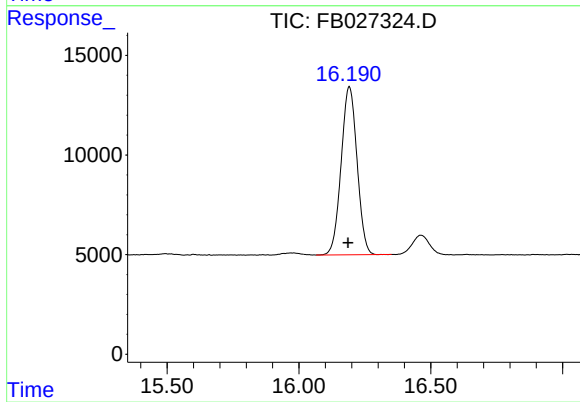

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.006 min
Response: 352902
Conc: 21.14 ng/ml