

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053122\
 Data File : FB027331.D
 Signal(s) : FID2B.CH
 Acq On : 31 May 2022 15:00
 Operator : AJ/MA
 Sample : BSF0531S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0531S2

Integration File: Calibration.e
 Quant Time: Jun 01 03:55:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
 Quant Title :
 QLast Update : Tue May 10 13:42:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	226216	21.550 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	389760	24.492 ng/ml
2) t 2,2,4-Trimethylpentane	7.434	466815	28.934 ng/ml
3) t n-Heptane	7.754	133894	8.194 ng/ml
4) t Benzene	7.892	186047	10.033 ng/ml
6) t Toluene	10.626	714567	40.248 ng/ml
7) t Ethylbenzene	13.063	214668	12.999 ng/ml
8) t m-Xylene	13.194	512834	31.167 ng/ml
9) t O-Xylene	13.922	397653	24.243 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	425436	25.483 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB053122\
Data File : FB027331.D
Signal(s) : FID2B.CH
Acq On : 31 May 2022 15:00
Operator : AJ/MA
Sample : BSF0531S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0531S2

Integration File: Calibration.e
Quant Time: Jun 01 03:55:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

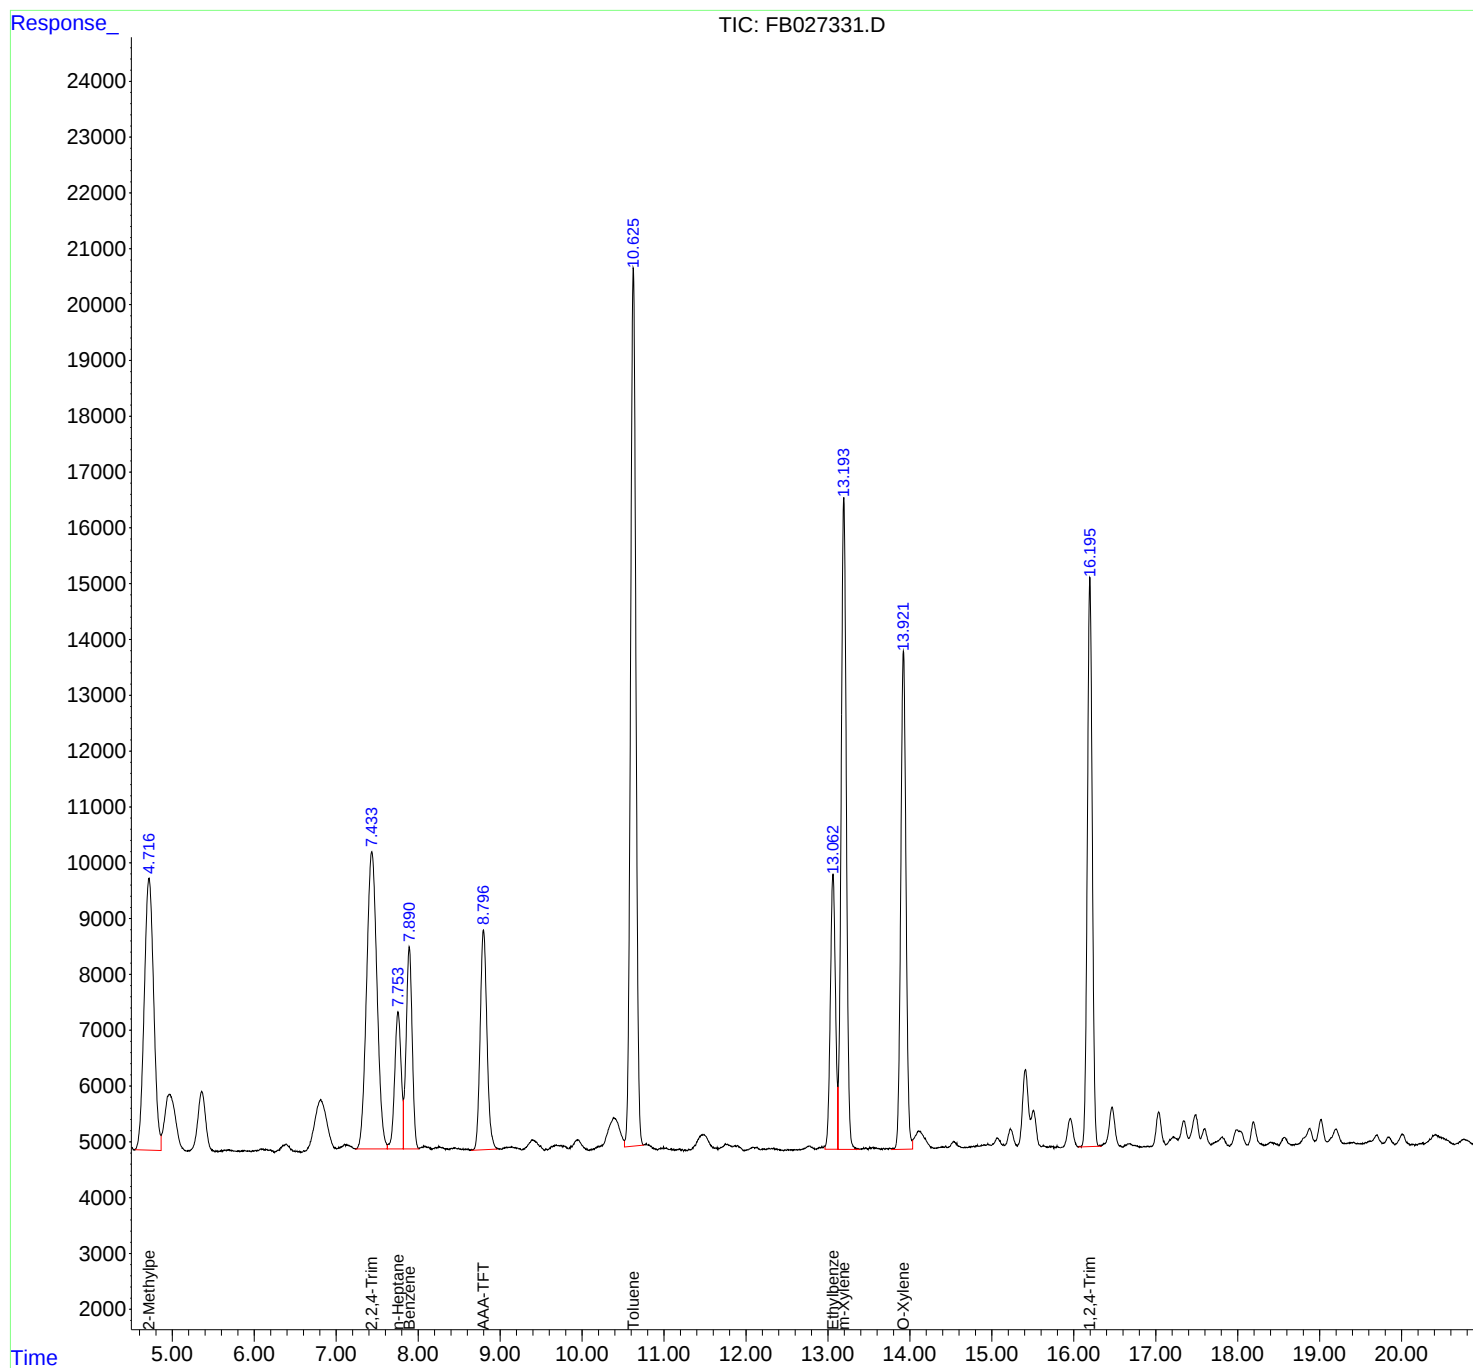


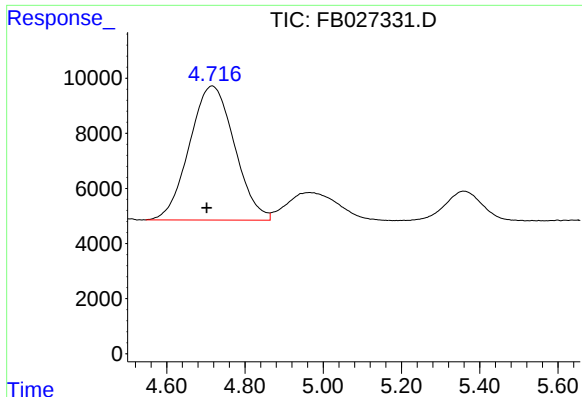

#1 2-Methylpentane


R.T.: 4.717 min
Delta R.T.: 0.015 min
Response: 389760
Conc: 24.49 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0531S2

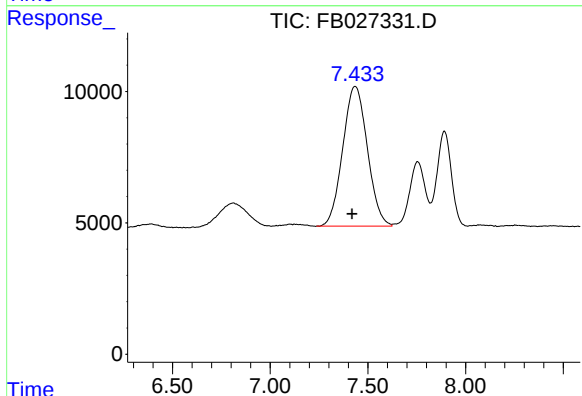


#2 2,2,4-Trimethylpentane

R.T.: 7.434 min
Delta R.T.: 0.015 min
Response: 466815
Conc: 28.93 ng/ml

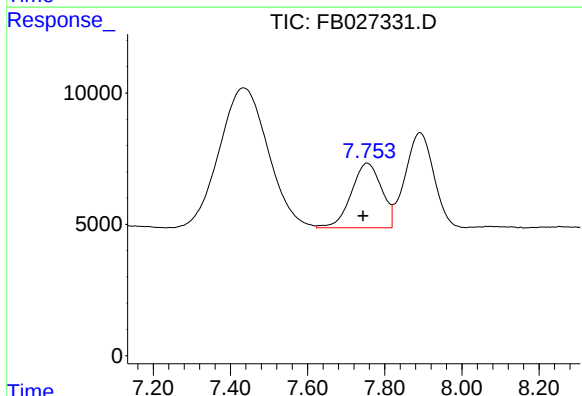


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.011 min
Response: 133894
Conc: 8.19 ng/ml

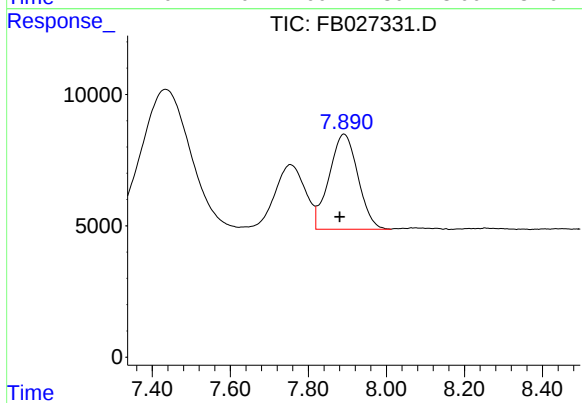

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.012 min
Response: 186047
Conc: 10.03 ng/ml

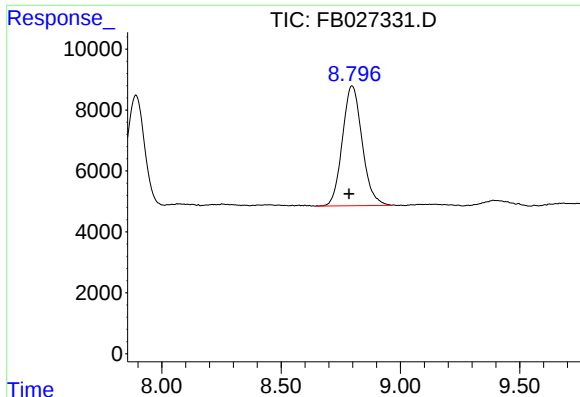

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.012 min
Response: 226216
Conc: 21.55 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0531S2

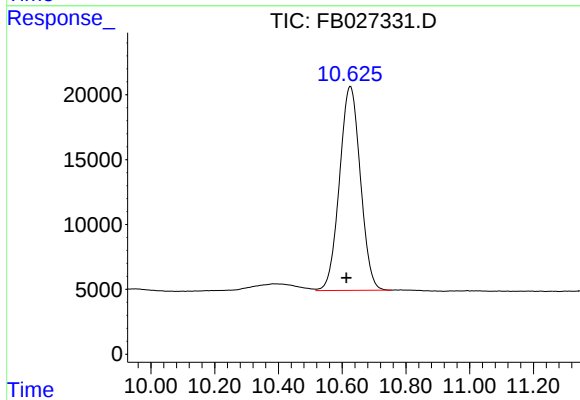


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.013 min
Response: 714567
Conc: 40.25 ng/ml

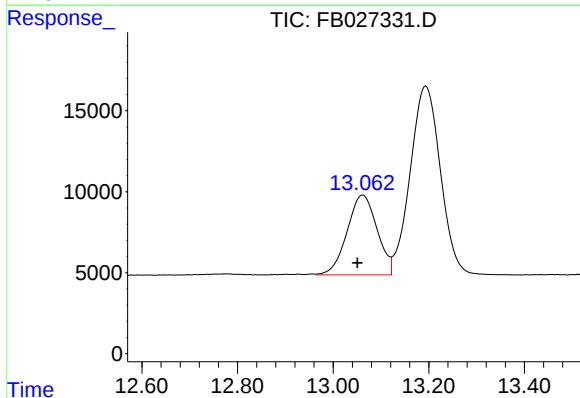


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.012 min
Response: 214668
Conc: 13.00 ng/ml

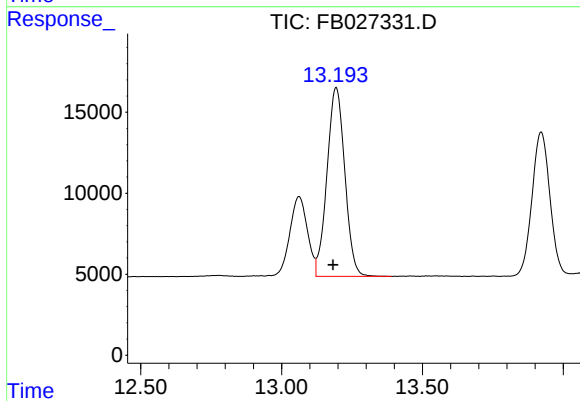

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: 0.011 min
Response: 512834
Conc: 31.17 ng/ml

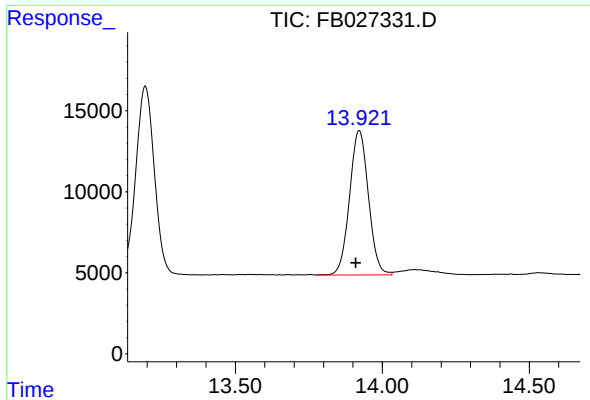

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.012 min
Response: 397653
Conc: 24.24 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0531S2

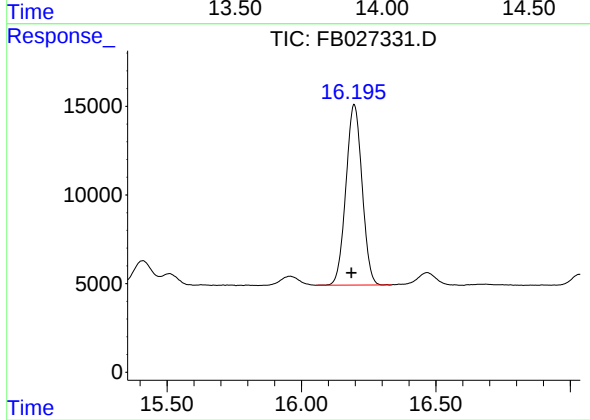

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.011 min
Response: 425436
Conc: 25.48 ng/ml