

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060120\
 Data File : FB024411.D
 Signal(s) : FID2B.CH
 Acq On : 1 Jun 2020 12:08
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 02 00:52:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	501651	22.718 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	968629	32.824 ng/ml
2) t 2,2,4-Trimethylpentane	7.409	1031803	33.775 ng/ml
3) t n-Heptane	7.750	345042	11.389 ng/ml
4) t Benzene	7.885	430377	11.384 ng/ml
6) t Toluene	10.623	1226424	33.845 ng/ml
7) t Ethylbenzene	13.063	366789	10.819 ng/ml
8) t m-Xylene	13.196	715522	21.683 ng/ml
9) t O-Xylene	13.923	702942	21.783 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	574957	21.319 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060120\
Data File : FB024411.D
Signal(s) : FID2B.CH
Acq On : 1 Jun 2020 12:08
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 02 00:52:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

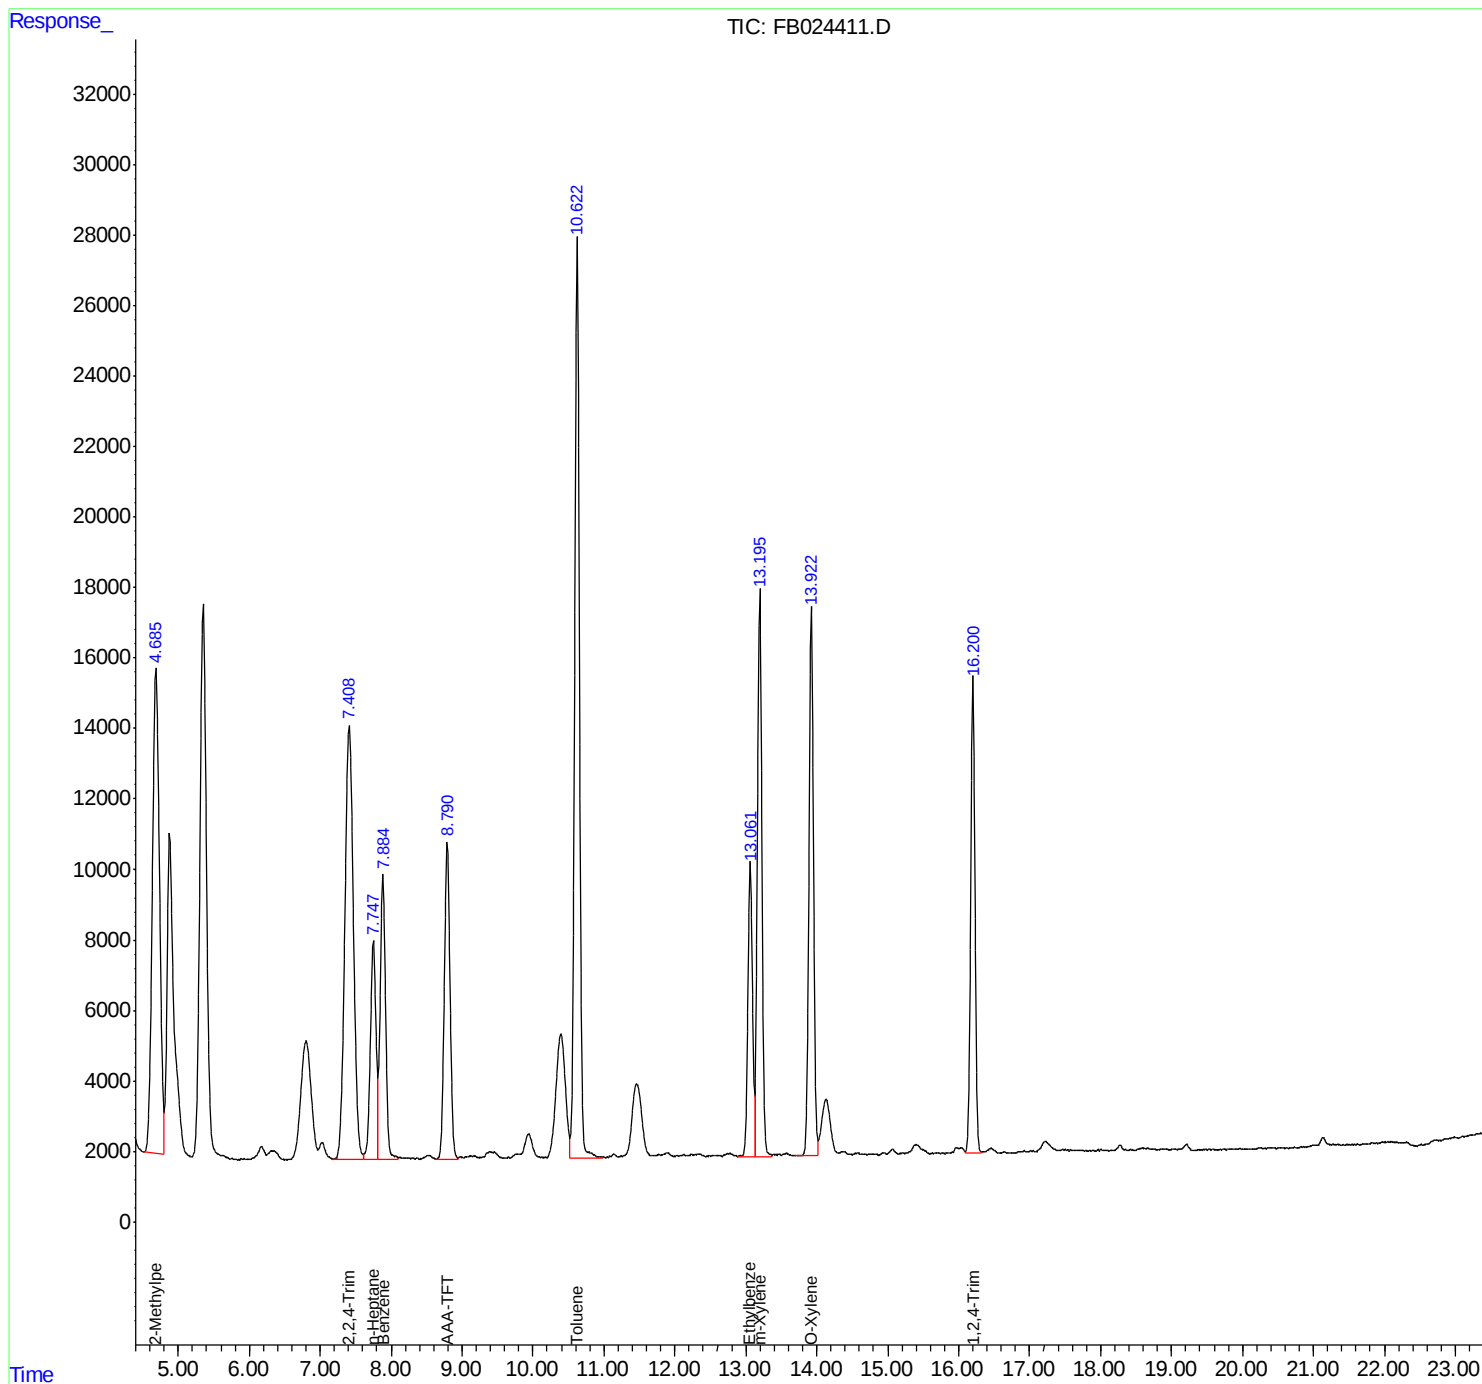

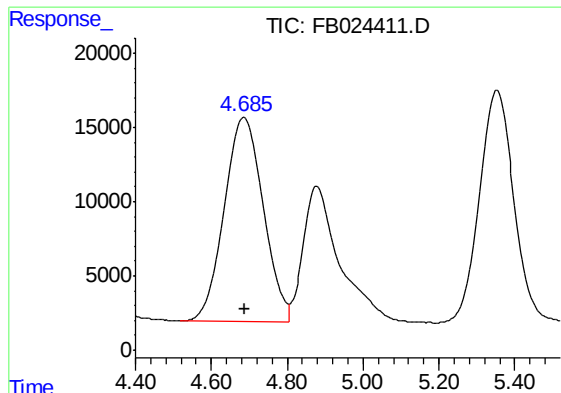


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: -0.003 min
Response: 968629
Conc: 32.82 ng/ml

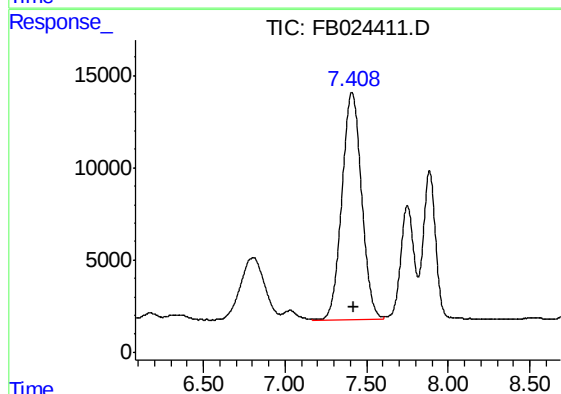


#2 2,2,4-Trimethylpentane

R.T.: 7.409 min
Delta R.T.: -0.008 min
Response: 1031803
Conc: 33.77 ng/ml

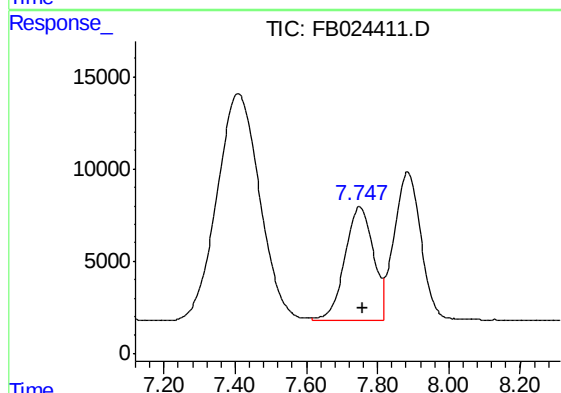


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.008 min
Response: 345042
Conc: 11.39 ng/ml

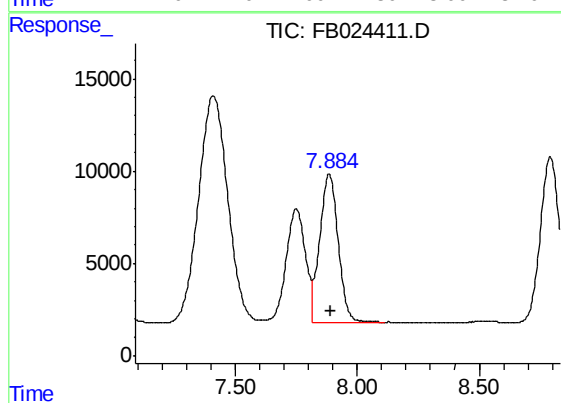


#4 Benzene

R.T.: 7.885 min
Delta R.T.: -0.008 min
Response: 430377
Conc: 11.38 ng/ml

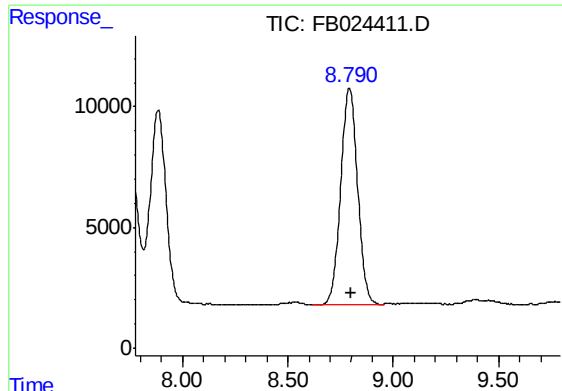


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: -0.008 min
Response: 501651
Conc: 22.72 ng/ml

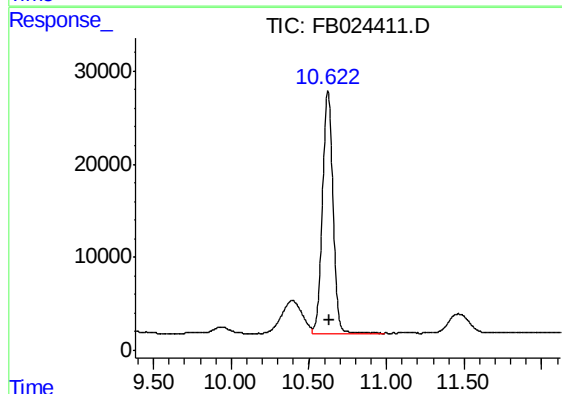


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.008 min
Response: 1226424
Conc: 33.84 ng/ml

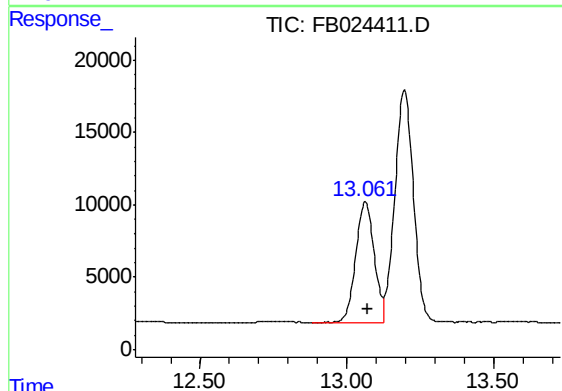


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: -0.009 min
Response: 366789
Conc: 10.82 ng/ml

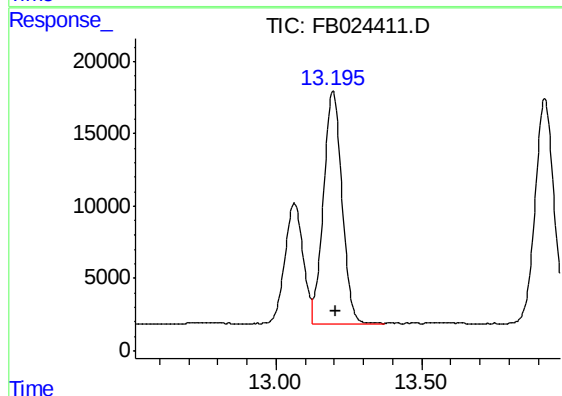


#8 m-Xylene

R.T.: 13.196 min
Delta R.T.: -0.008 min
Response: 715522
Conc: 21.68 ng/ml

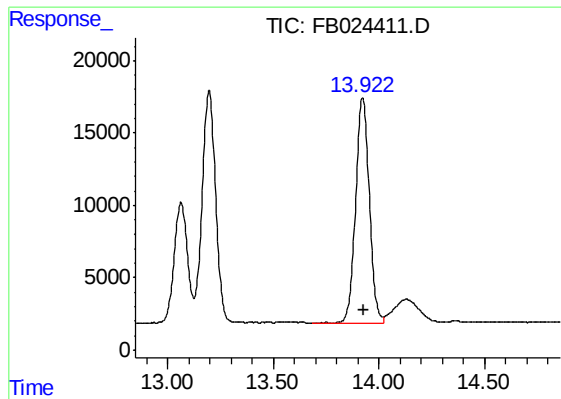

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: -0.009 min
Response: 702942
Conc: 21.78 ng/ml

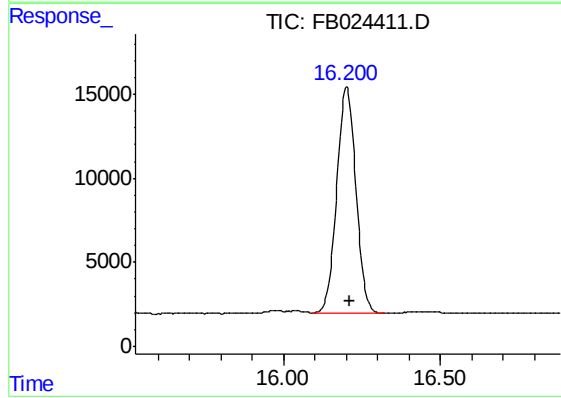

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: -0.009 min
Response: 574957
Conc: 21.32 ng/ml