

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060120\
 Data File : FB024417.D
 Signal(s) : FID2B.CH
 Acq On : 1 Jun 2020 15:10
 Operator : DD/AJ
 Sample : L2813-02MSD
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 02 00:53:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	450860	20.418 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	724045	24.535 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	704073	23.047 ng/ml
3) t n-Heptane	7.756	80778	2.666 ng/ml
4) t Benzene	7.890	346886	9.176 ng/ml
6) t Toluene	10.628	1007731	27.810 ng/ml
7) t Ethylbenzene	13.064	488588	14.412 ng/ml
8) t m-Xylene	13.201	510424	15.468 ng/ml
9) t O-Xylene	13.929	689775	21.375 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	726493	26.937 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060120\
Data File : FB024417.D
Signal(s) : FID2B.CH
Acq On : 1 Jun 2020 15:10
Operator : DD/AJ
Sample : L2813-02MSD
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 02 00:53:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

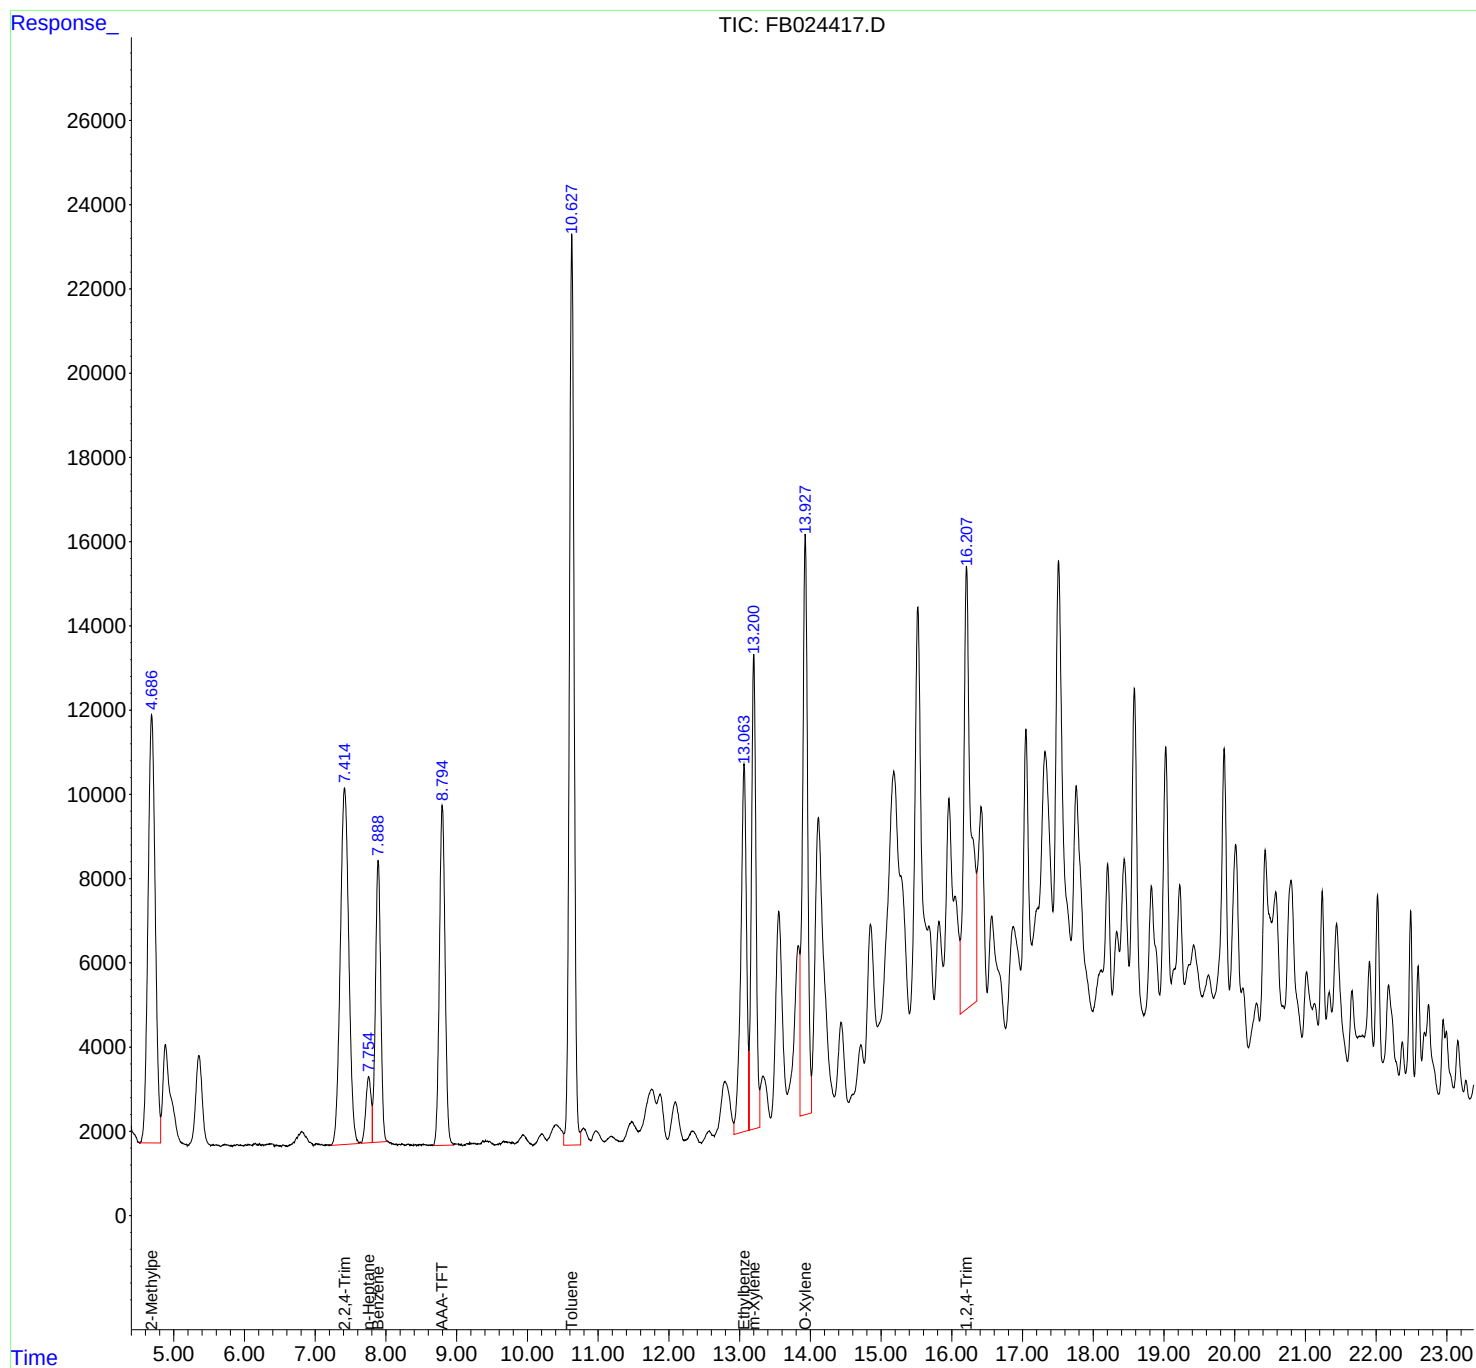

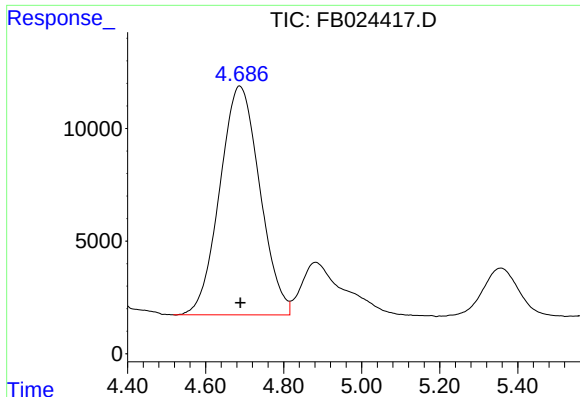


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: -0.002 min
Response: 724045
Conc: 24.54 ng/ml

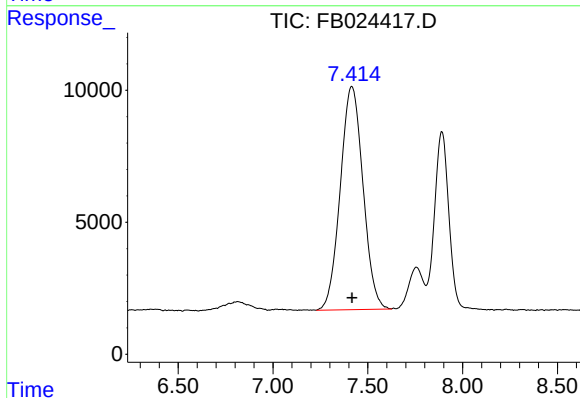


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.002 min
Response: 704073
Conc: 23.05 ng/ml

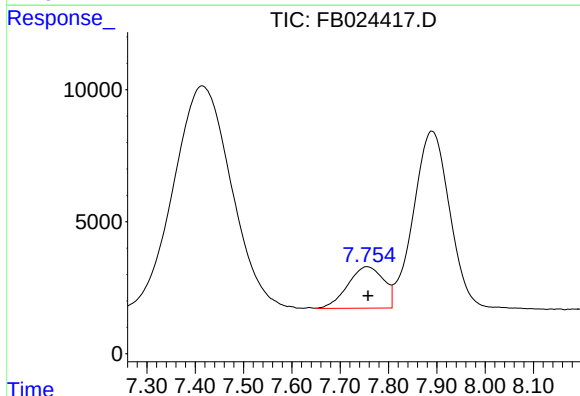


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 80778
Conc: 2.67 ng/ml

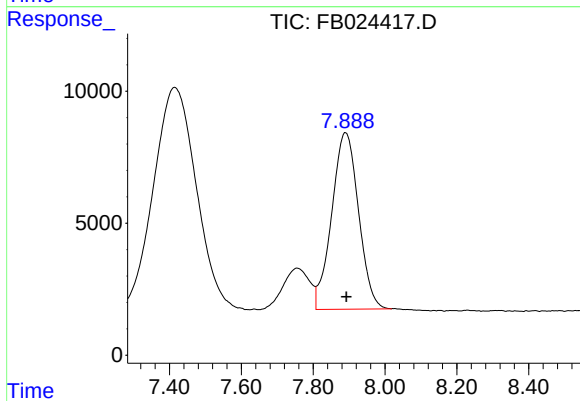


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 346886
Conc: 9.18 ng/ml

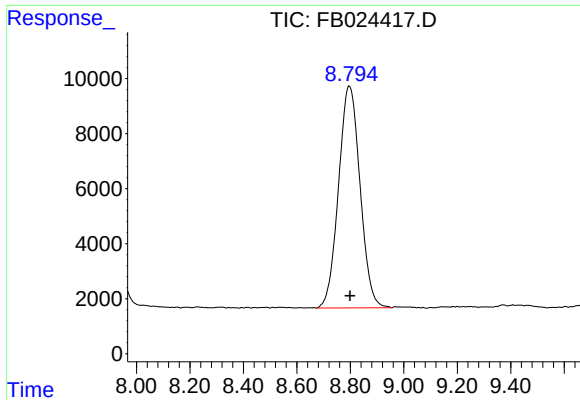


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 450860
Conc: 20.42 ng/ml

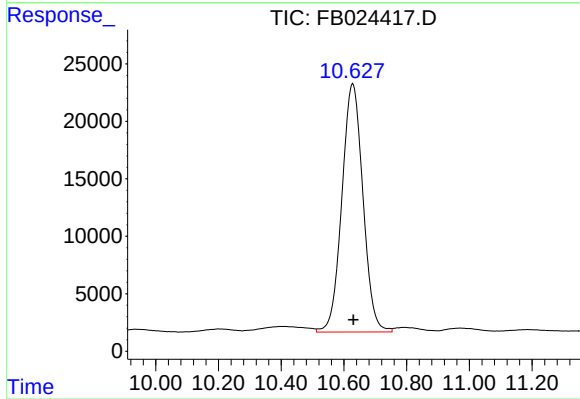


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.002 min
Response: 1007731
Conc: 27.81 ng/ml

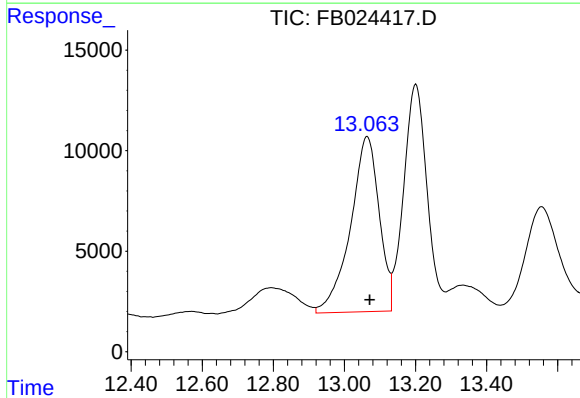


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: -0.007 min
Response: 488588
Conc: 14.41 ng/ml

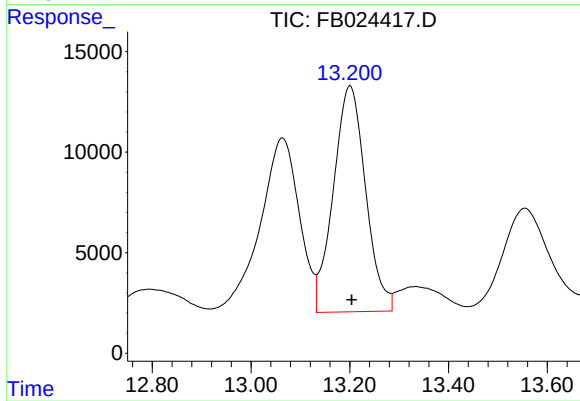


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.003 min
Response: 510424
Conc: 15.47 ng/ml

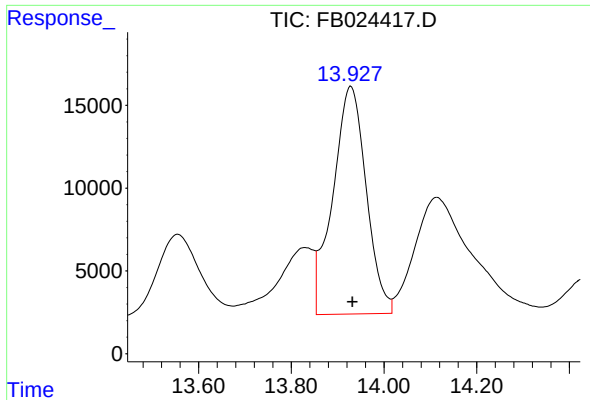

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.003 min
Response: 689775
Conc: 21.38 ng/ml

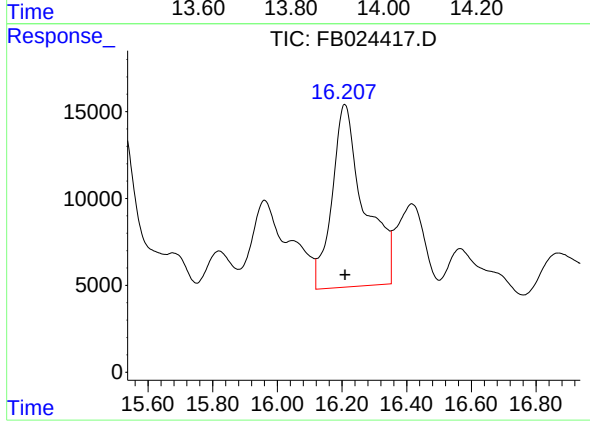

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 726493
Conc: 26.94 ng/ml