

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060221\
 Data File : FB025823.D
 Signal(s) : FID2B.CH
 Acq On : 2 Jun 2021 18:35
 Operator : DD/AJ
 Sample : M2578-01MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 03 01:59:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060221.M
 Quant Title :
 QLast Update : Wed Jun 02 14:44:25 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.215	378615	14.949 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.168	593574	21.282 ng/ml
2) t 2,2,4-Trimethylpentane	7.869	375097	15.936 ng/ml
3) t n-Heptane	8.189	186649	5.107 ng/ml
4) t Benzene	8.340	329321	7.571 ng/ml
6) t Toluene	11.035	905104	22.379 ng/ml
7) t Ethylbenzene	13.443	262569	6.791 ng/ml
8) t m-Xylene	13.574	469487	12.338 ng/ml
9) t O-Xylene	14.297	498739	13.950 ng/ml
10) t 1,2,4-Trimethylbenzene	16.549	252481	10.057 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060221\
Data File : FB025823.D
Signal(s) : FID2B.CH
Acq On : 2 Jun 2021 18:35
Operator : DD/AJ
Sample : M2578-01MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 03 01:59:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060221.M
Quant Title :
QLast Update : Wed Jun 02 14:44:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

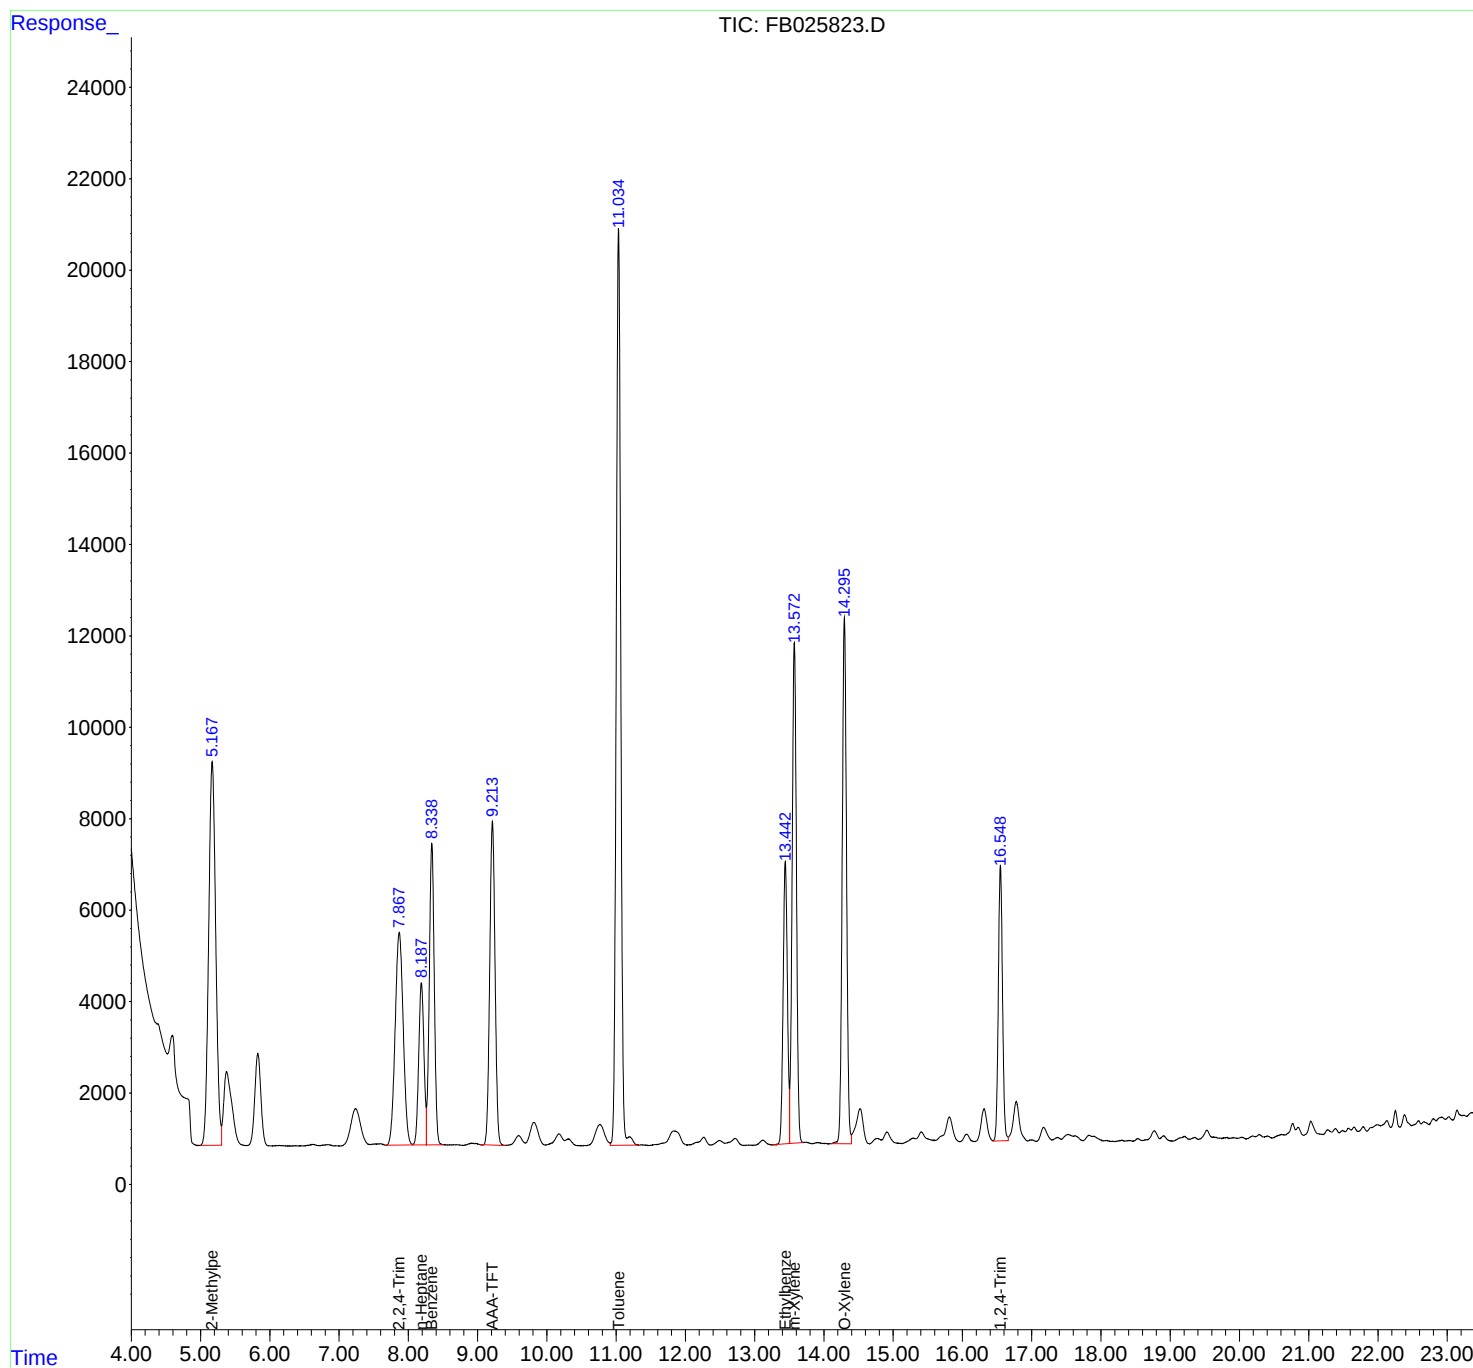


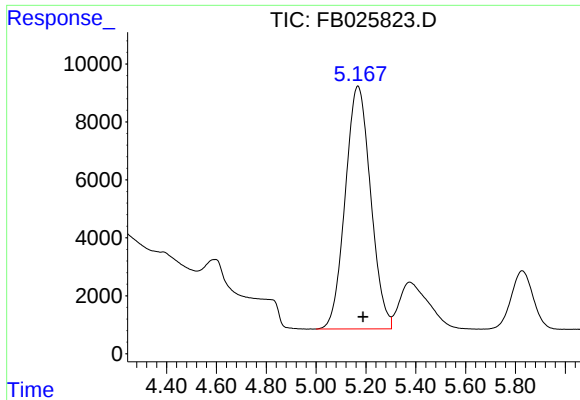

#1 2-Methylpentane


R.T.: 5.168 min
Delta R.T.: -0.021 min
Response: 593574
Conc: 21.28 ng/ml

Instrument :
FID_B
ClientSampleId :

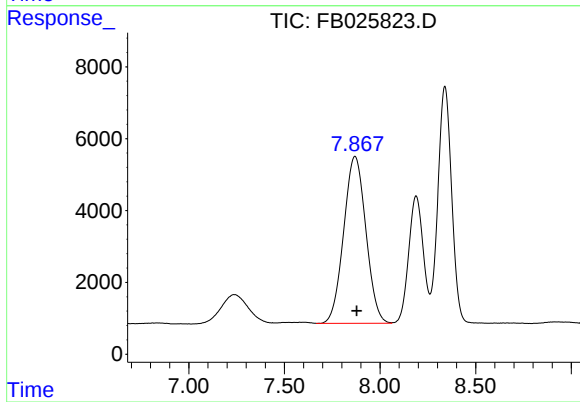


#2 2,2,4-Trimethylpentane

R.T.: 7.869 min
Delta R.T.: -0.009 min
Response: 375097
Conc: 15.94 ng/ml

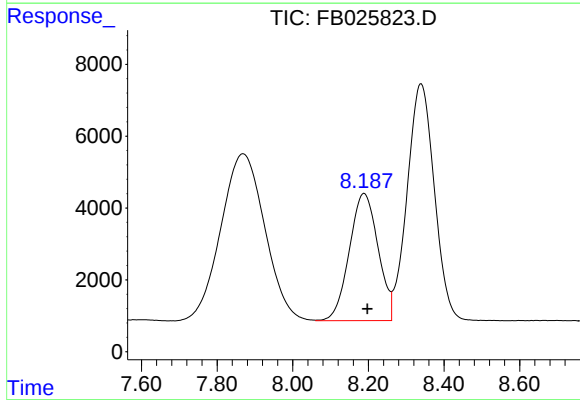


#3 n-Heptane

R.T.: 8.189 min
Delta R.T.: -0.008 min
Response: 186649
Conc: 5.11 ng/ml

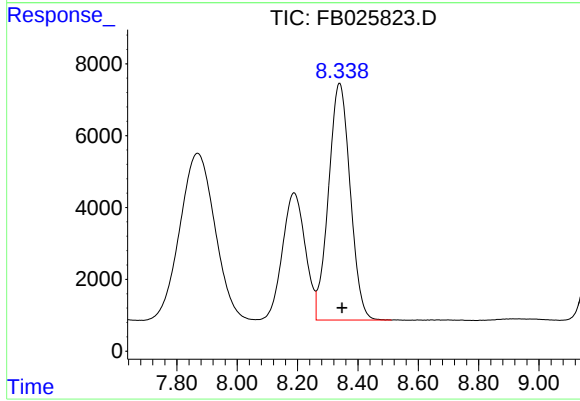


#4 Benzene

R.T.: 8.340 min
Delta R.T.: -0.008 min
Response: 329321
Conc: 7.57 ng/ml

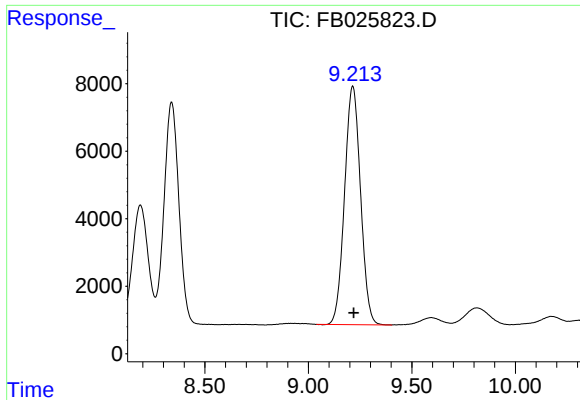


```
#5  AAA-TFT
      R.T.:    9.215 min
Delta R.T.:   -0.005 min
Response:     378615
Conc:         14.95 ng/ml
```


Instrument : FID_B
ClientSampleId :

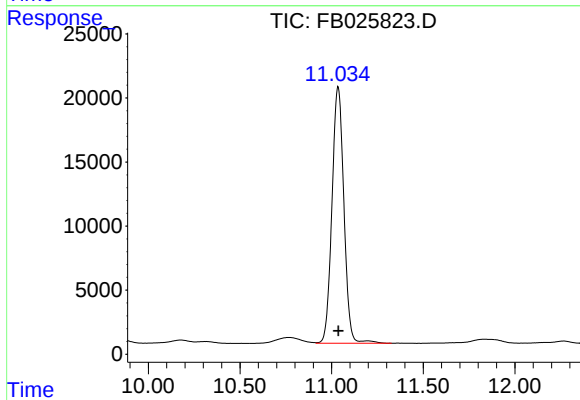


```
#6  Toluene
      R.T.:   11.035 min
Delta R.T.:  -0.002 min
  Response:   905104
      Conc:   22.38 ng/ml
```

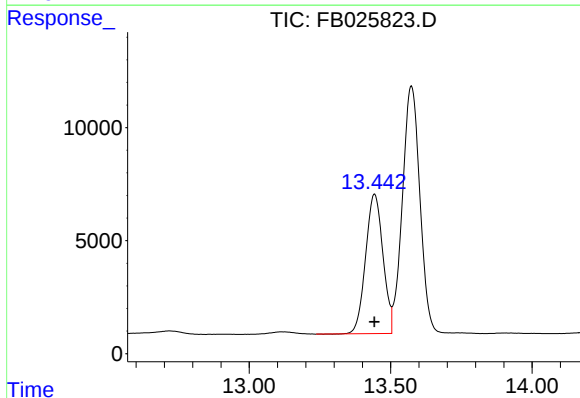

```
#7 Ethylbenzene
      R.T.:    13.443 min
Delta R.T.:    0.000 min
  Response:    262569
      Conc:    6.79 ng/ml
```

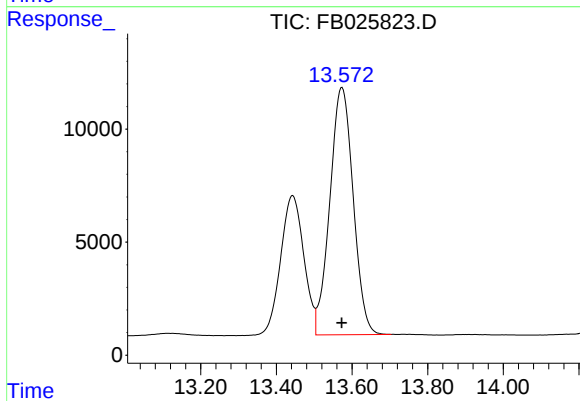


```
#8  m-Xylene
      R.T.:   13.574 min
Delta R.T.:   0.000 min
  Response:   469487
      Conc:   12.34 ng/ml
```

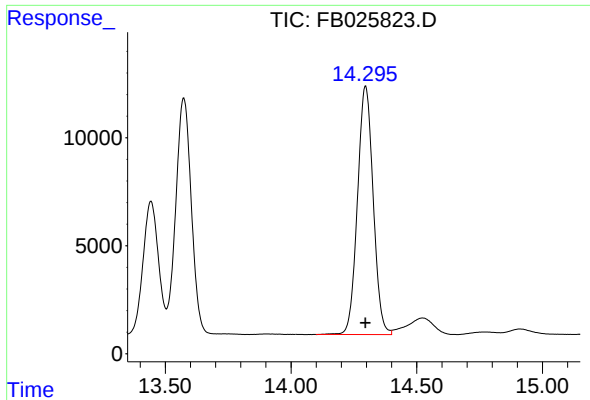

#9 O-Xylene

R.T.: 14.297 min
Delta R.T.: 0.000 min
Response: 498739
Conc: 13.95 ng/ml

Instrument :
FID_B
ClientSampleId :

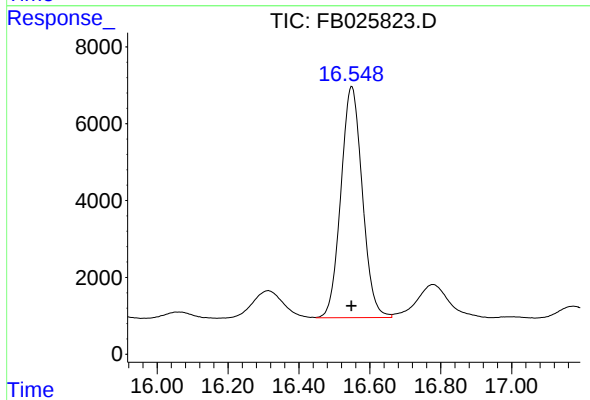

#10 1,2,4-Trimethylbenzene

R.T.: 16.549 min
Delta R.T.: 0.002 min
Response: 252481
Conc: 10.06 ng/ml