

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060223\
 Data File : FB029955.D
 Signal(s) : FID2B.CH
 Acq On : 2 Jun 2023 21:11
 Operator : YP/AJ
 Sample : 03016-05MSD 50X
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 05 02:19:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
 Quant Title :
 QLast Update : Thu May 11 11:33:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	278931	22.905 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	557255	32.524 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	596412	34.944 ng/ml
3) t n-Heptane	7.751	186491	10.502 ng/ml
4) t Benzene	7.886	218397	10.425 ng/ml
6) t Toluene	10.620	629389	30.910 ng/ml
7) t Ethylbenzene	13.056	202845	10.584 ng/ml
8) t m-Xylene	13.189	408637	21.208 ng/ml
9) t O-Xylene	13.915	401848	21.602 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	412222	22.161 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060223\
 Data File : FB029955.D
 Signal(s) : FID2B.CH
 Acq On : 2 Jun 2023 21:11
 Operator : YP/AJ
 Sample : 03016-05MSD 50X
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 05 02:19:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
 Quant Title :
 QLast Update : Thu May 11 11:33:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

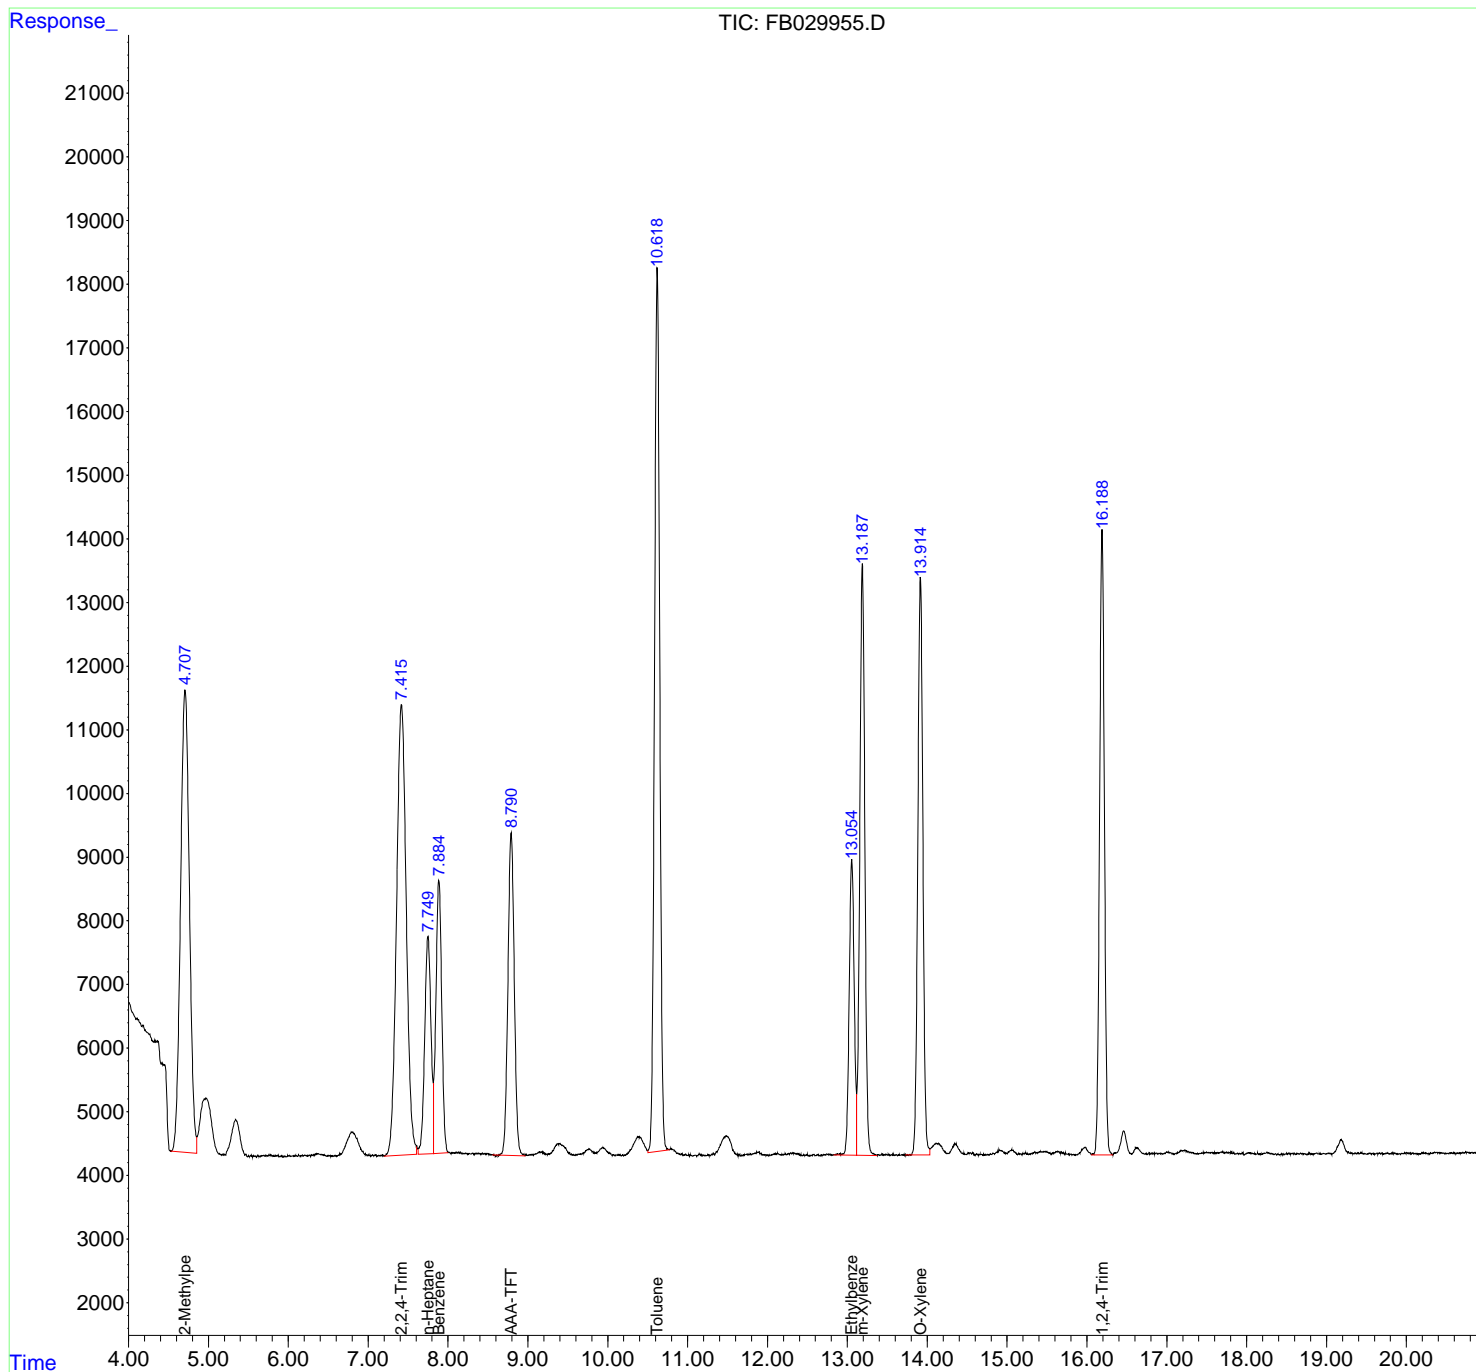


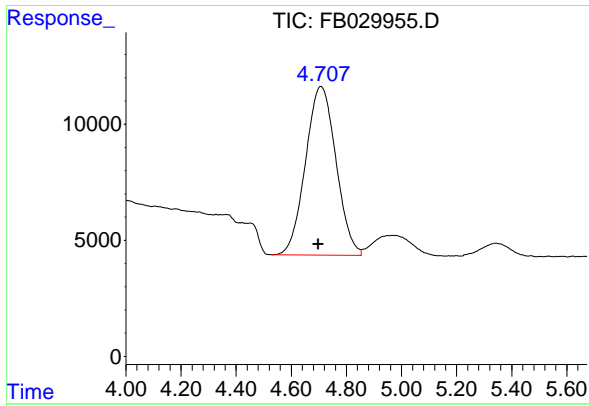

#1 2-Methylpentane


R.T.: 4.708 min
 Delta R.T.: 0.009 min
 Response: 557255
 Conc: 32.52 ng/ml

Instrument :
 FID_B
 ClientSampleId :

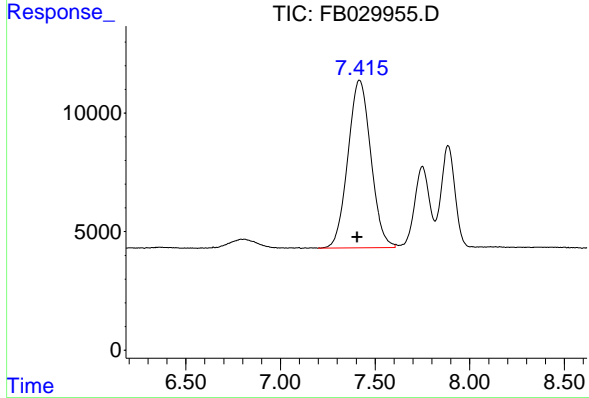


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
 Delta R.T.: 0.011 min
 Response: 596412
 Conc: 34.94 ng/ml

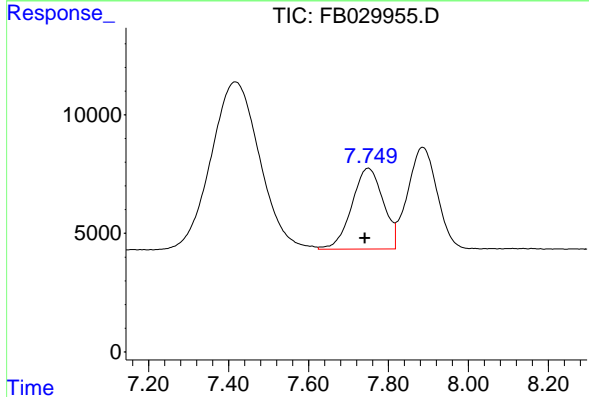


#3 n-Heptane

R.T.: 7.751 min
 Delta R.T.: 0.009 min
 Response: 186491
 Conc: 10.50 ng/ml

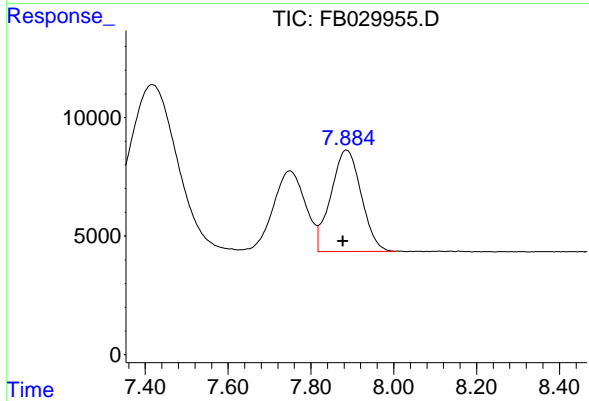

#4 Benzene


R.T.: 7.886 min
 Delta R.T.: 0.008 min
 Response: 218397
 Conc: 10.43 ng/ml

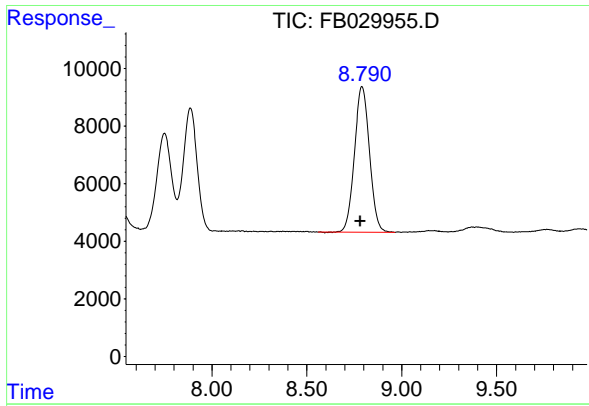

#5 AAA-TFT


R.T.: 8.791 min
 Delta R.T.: 0.009 min
 Response: 278931
 Conc: 22.91 ng/ml

Instrument :
 FID_B
 ClientSampleId :

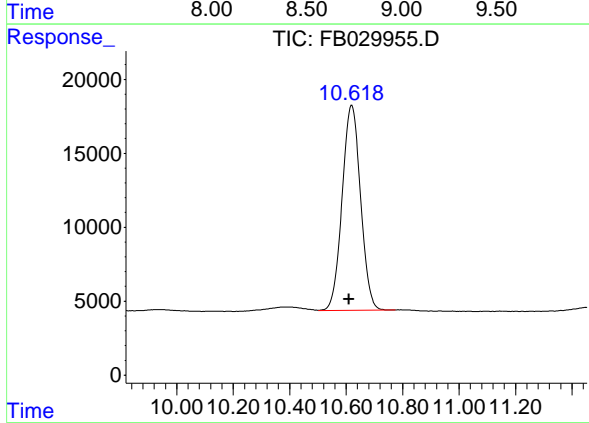


#6 Toluene

R.T.: 10.620 min
 Delta R.T.: 0.010 min
 Response: 629389
 Conc: 30.91 ng/ml

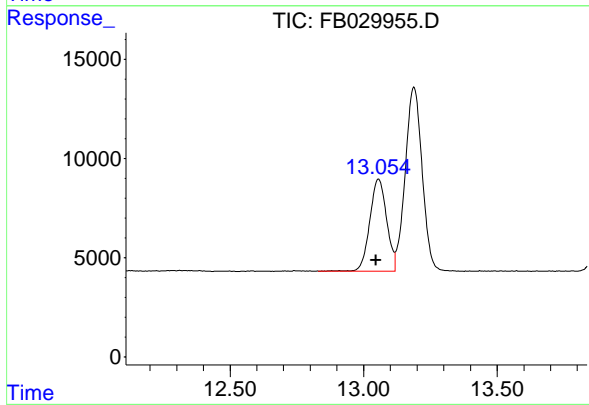


#7 Ethylbenzene

R.T.: 13.056 min
 Delta R.T.: 0.010 min
 Response: 202845
 Conc: 10.58 ng/ml

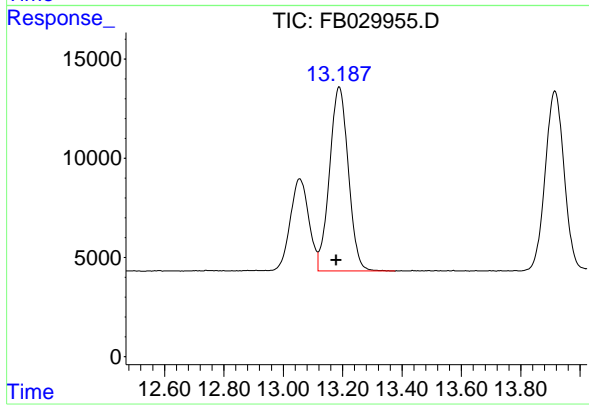

#8 m-Xylene


R.T.: 13.189 min
 Delta R.T.: 0.010 min
 Response: 408637
 Conc: 21.21 ng/ml

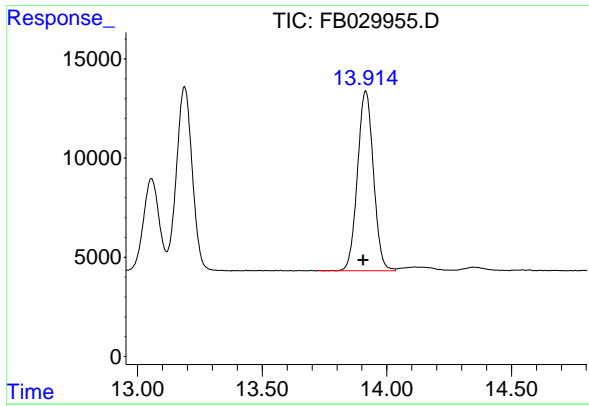

#9 O-Xylene

R.T.: 13.915 min
 Delta R.T.: 0.010 min
 Response: 401848
 Conc: 21.60 ng/ml

Instrument :
 FID_B
 ClientSampleId :

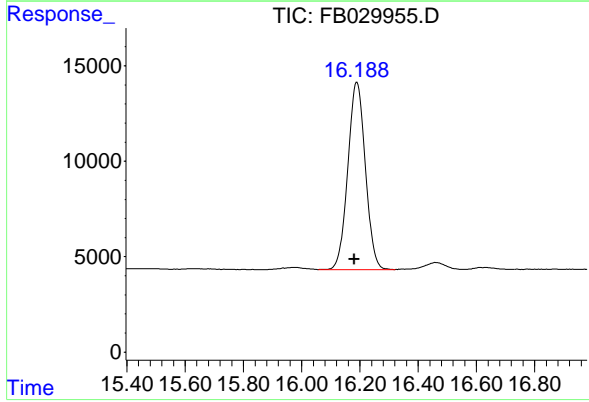

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
 Delta R.T.: 0.009 min
 Response: 412222
 Conc: 22.16 ng/ml