

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060223\
 Data File : FB029950.D
 Signal(s) : FID2B.CH
 Acq On : 2 Jun 2023 15:38
 Operator : YP/AJ
 Sample : BSF0602S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0602S2

Integration File: Calibration.e
 Quant Time: Jun 05 01:22:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
 Quant Title :
 QLast Update : Thu May 11 11:33:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	263593	21.646 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	578608	33.770 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	581989	34.099 ng/ml
3) t n-Heptane	7.751	202799	11.420 ng/ml
4) t Benzene	7.887	233385	11.141 ng/ml
6) t Toluene	10.621	666540	32.735 ng/ml
7) t Ethylbenzene	13.057	207313	10.817 ng/ml
8) t m-Xylene	13.189	417193	21.653 ng/ml
9) t O-Xylene	13.916	401610	21.589 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	380716	20.467 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060223\
Data File : FB029950.D
Signal(s) : FID2B.CH
Acq On : 2 Jun 2023 15:38
Operator : YP/AJ
Sample : BSF0602S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0602S2

Integration File: Calibration.e
Quant Time: Jun 05 01:22:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
Quant Title :
QLast Update : Thu May 11 11:33:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

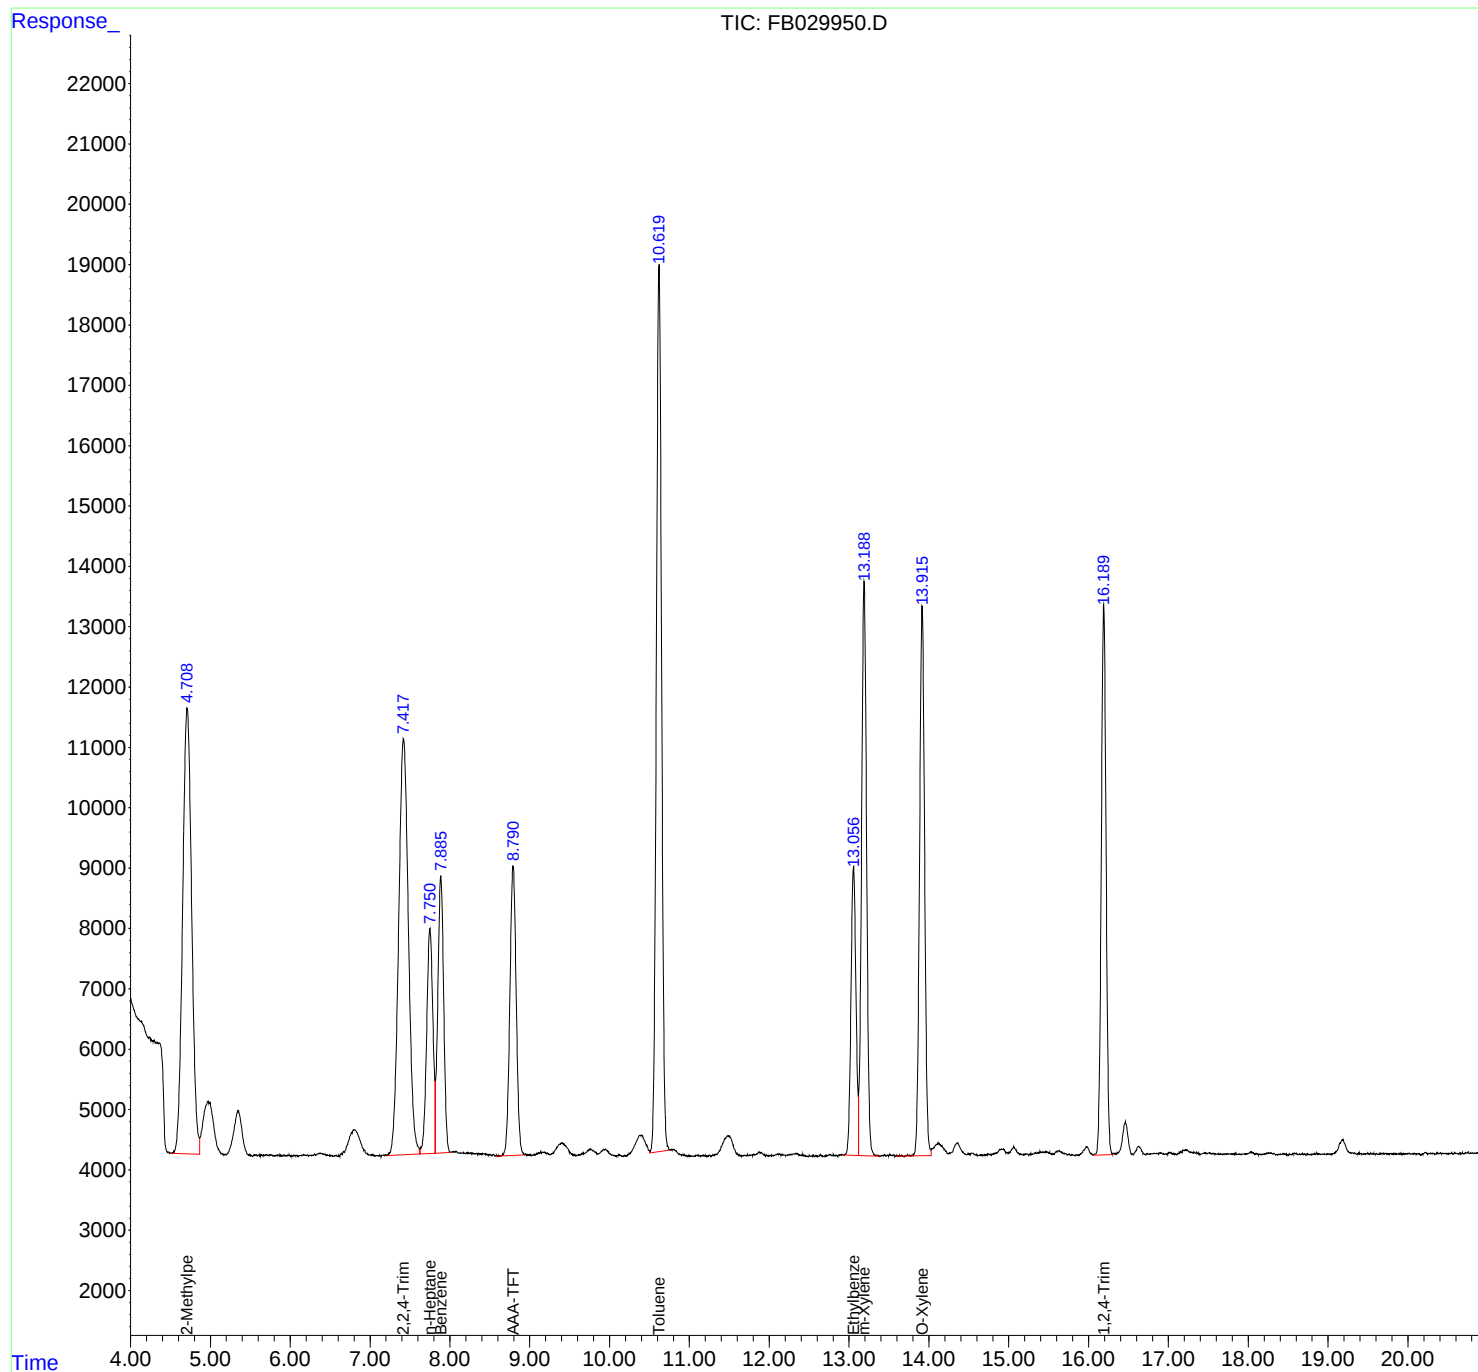


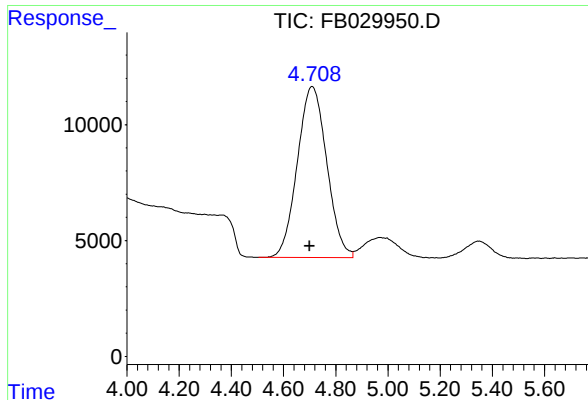

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.010 min
Response: 578608
Conc: 33.77 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0602S2

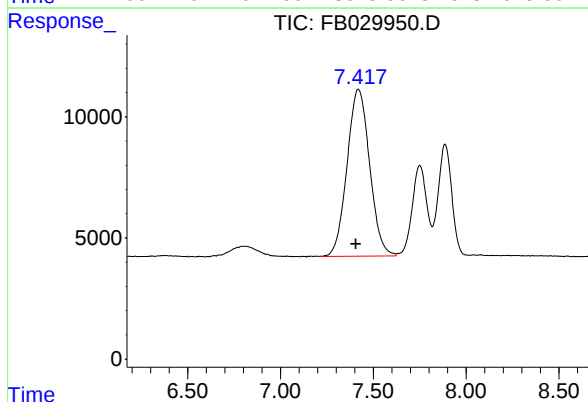


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.013 min
Response: 581989
Conc: 34.10 ng/ml

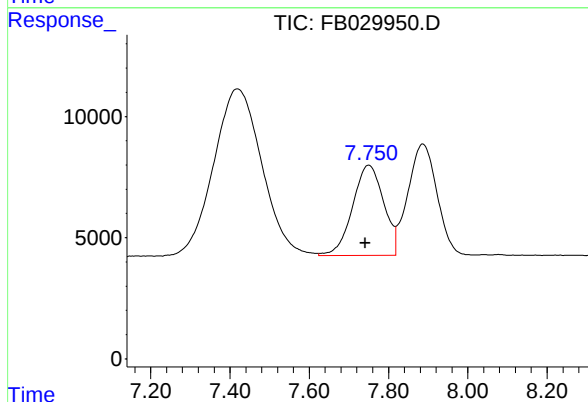


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.009 min
Response: 202799
Conc: 11.42 ng/ml

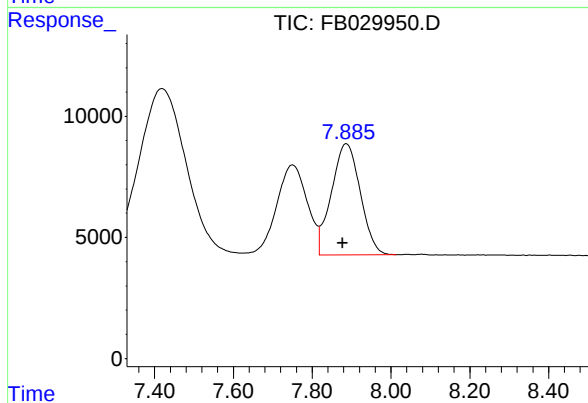

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.009 min
Response: 233385
Conc: 11.14 ng/ml

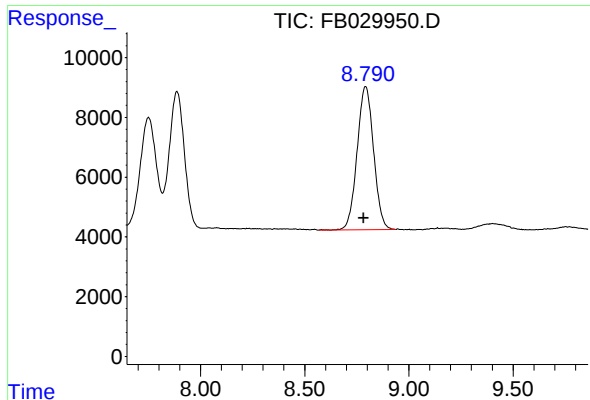

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.010 min
Response: 263593
Conc: 21.65 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0602S2

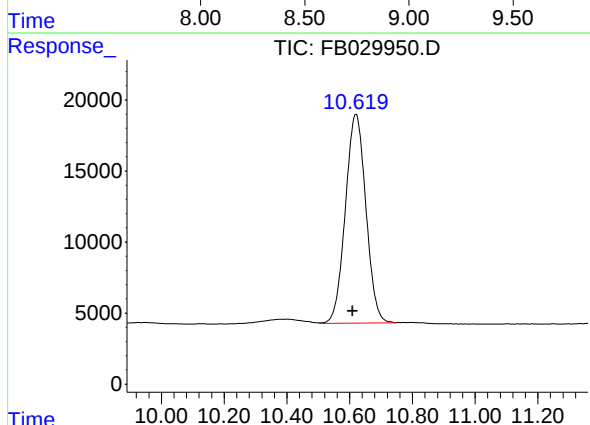


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.011 min
Response: 666540
Conc: 32.74 ng/ml

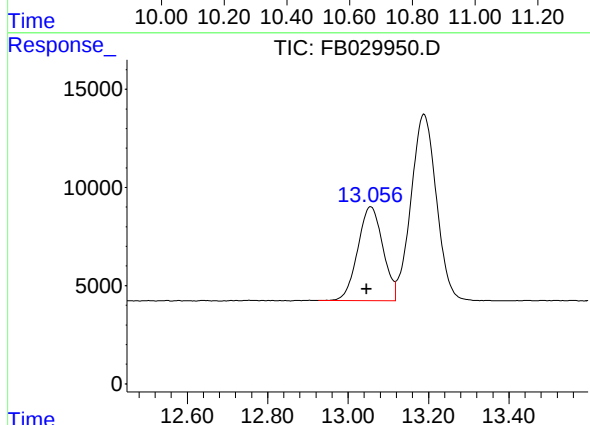


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.011 min
Response: 207313
Conc: 10.82 ng/ml

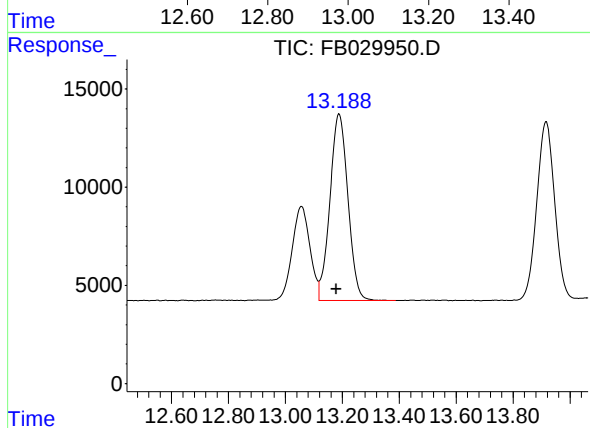

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.010 min
Response: 417193
Conc: 21.65 ng/ml

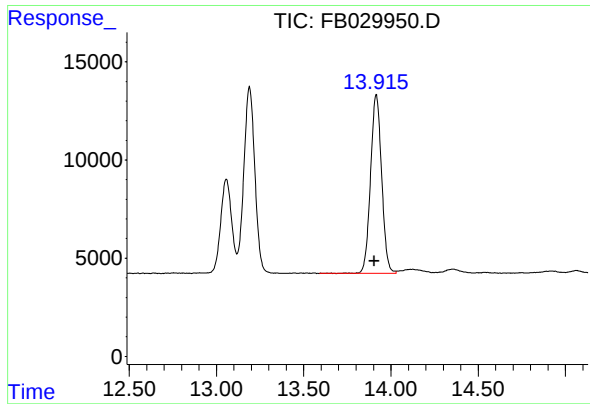

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.010 min
Response: 401610
Conc: 21.59 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0602S2

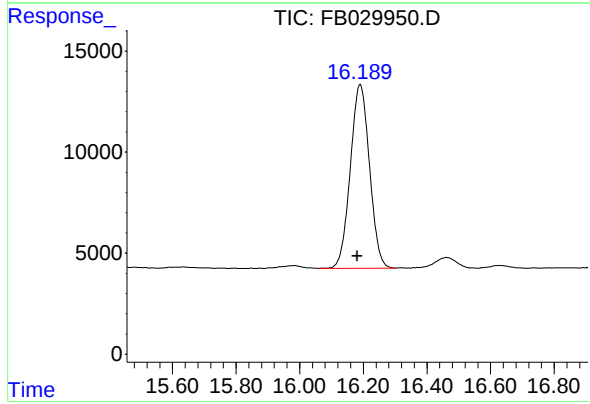

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.010 min
Response: 380716
Conc: 20.47 ng/ml