

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060225\
Data File : FB031848.D
Signal(s) : FID2B.CH
Acq On : 2 Jun 2025 18:23
Operator : YP/AJ
Sample : Q2150-07
Misc : 5.90G/5.00 ML DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-51

Integration File: Calibration.e
Quant Time: Jun 03 05:28:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB053025.M
Quant Title :
QLast Update : Fri May 30 15:30:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	222047	18.197 ng/ml
Target Compounds			
4) t Benzene	7.891	42570	2.141 ng/ml
8) t m-Xylene	13.187	12266	0.718 ng/ml
9) t O-Xylene	13.917	9647	0.608 ng/ml
10) t 1,2,4-Trimethylbenzene	16.204	7237	0.627 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060225\
Data File : FB031848.D
Signal(s) : FID2B.CH
Acq On : 2 Jun 2025 18:23
Operator : YP/AJ
Sample : Q2150-07
Misc : 5.90G/5.00 ML DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-51

Integration File: Calibration.e
Quant Time: Jun 03 05:28:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB053025.M
Quant Title :
QLast Update : Fri May 30 15:30:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

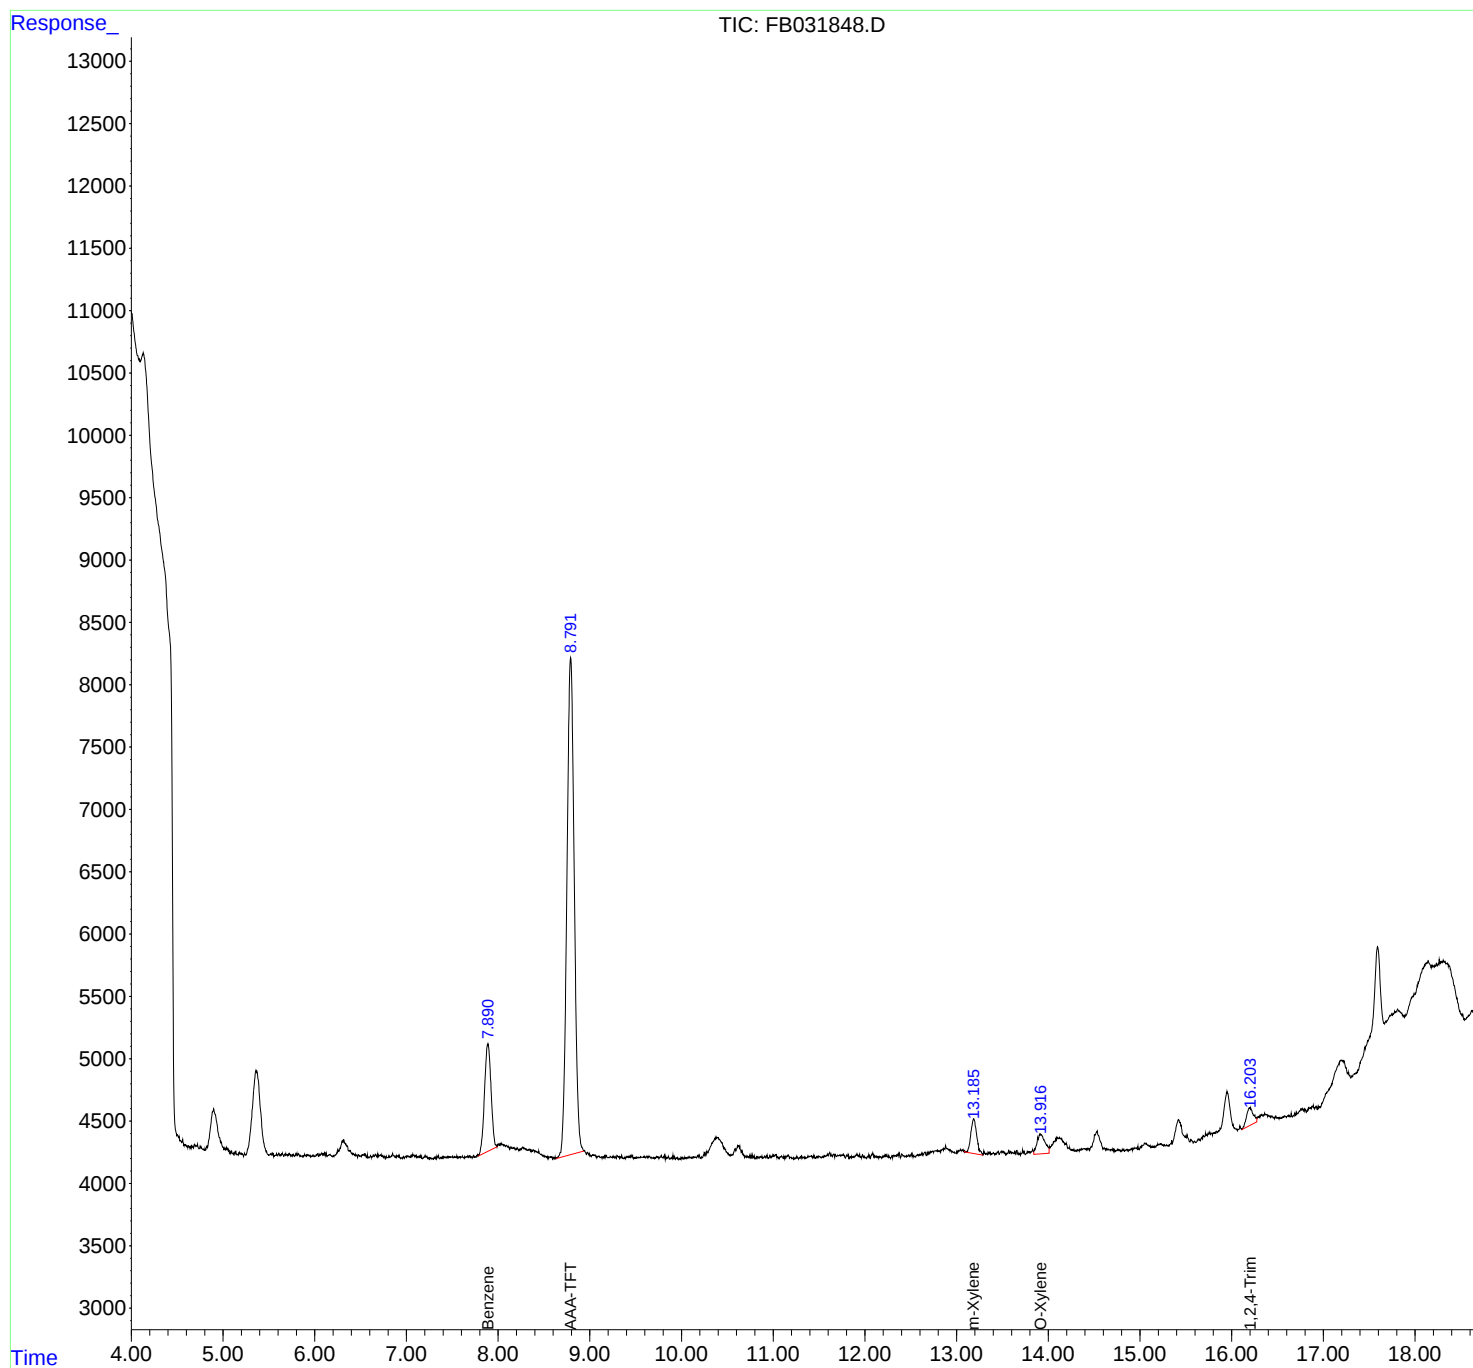


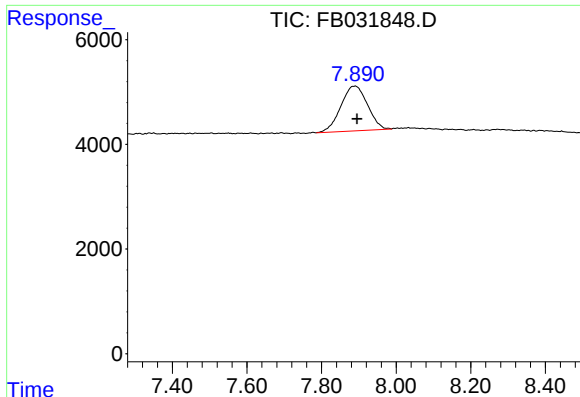

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.004 min
Response: 42570
Conc: 2.14 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-51

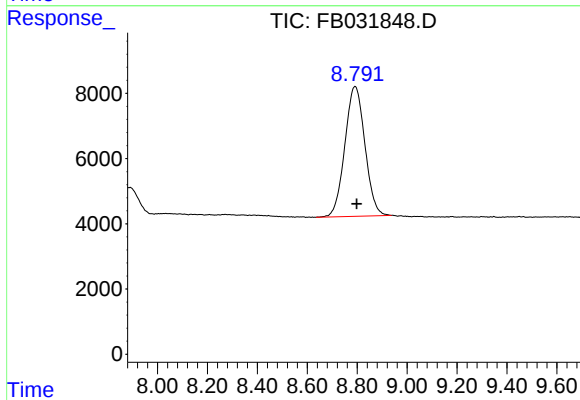


#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: -0.005 min
Response: 222047
Conc: 18.20 ng/ml

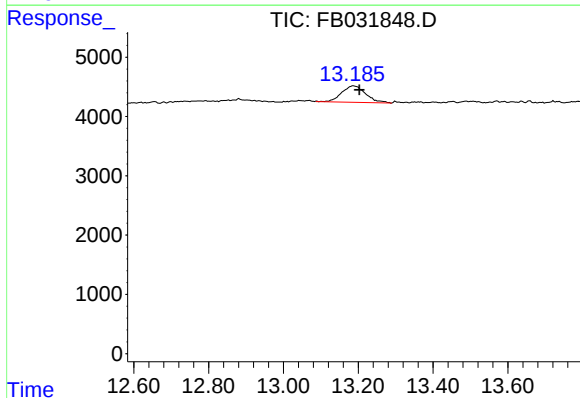


#8 m-Xylene

R.T.: 13.187 min
Delta R.T.: -0.016 min
Response: 12266
Conc: 0.72 ng/ml

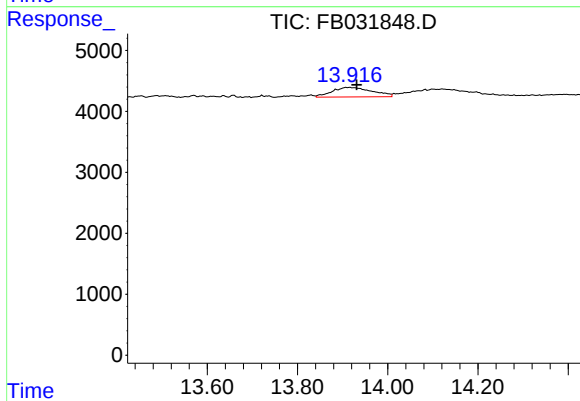

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.014 min
Response: 9647
Conc: 0.61 ng/ml

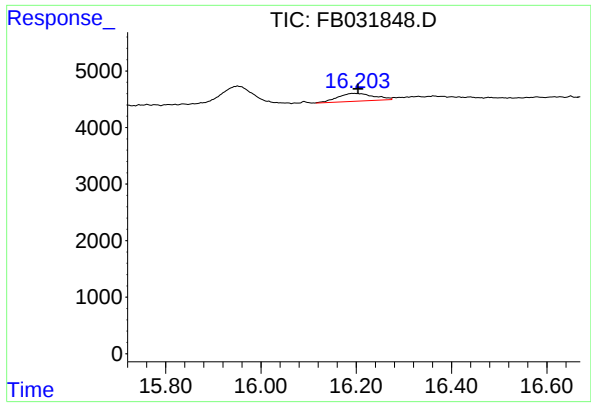

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min
Delta R.T.: 0.000 min
Response: 7237
Conc: 0.63 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-51