

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060319\
 Data File : FB021294.D
 Signal(s) : FID2B.CH
 Acq On : 3 Jun 2019 9:23
 Operator : MJ/SJ
 Sample : BSF0603S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 04 03:08:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.993	354078	24.015 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.855	1212485	32.252 ng/ml
2) t	2,2,4-Trimethylpentane	7.608	1168543	34.218 ng/ml
3) t	n-Heptane	7.950	368237	11.295 ng/ml
4) t	Benzene	8.085	395941	11.471 ng/ml
6) t	Toluene	10.837	789865	33.324 ng/ml
7) t	Ethylbenzene	13.287	254525	10.893 ng/ml
8) t	m-Xylene	13.421	550830	22.068 ng/ml
9) t	O-Xylene	14.151	564357	21.634 ng/ml
10) t	1,2,4-Trimethylbenzene	16.436	569335	21.200 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060319\
Data File : FB021294.D
Signal(s) : FID2B.CH
Acq On : 3 Jun 2019 9:23
Operator : MJ/SJ
Sample : BSF0603S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 04 03:08:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

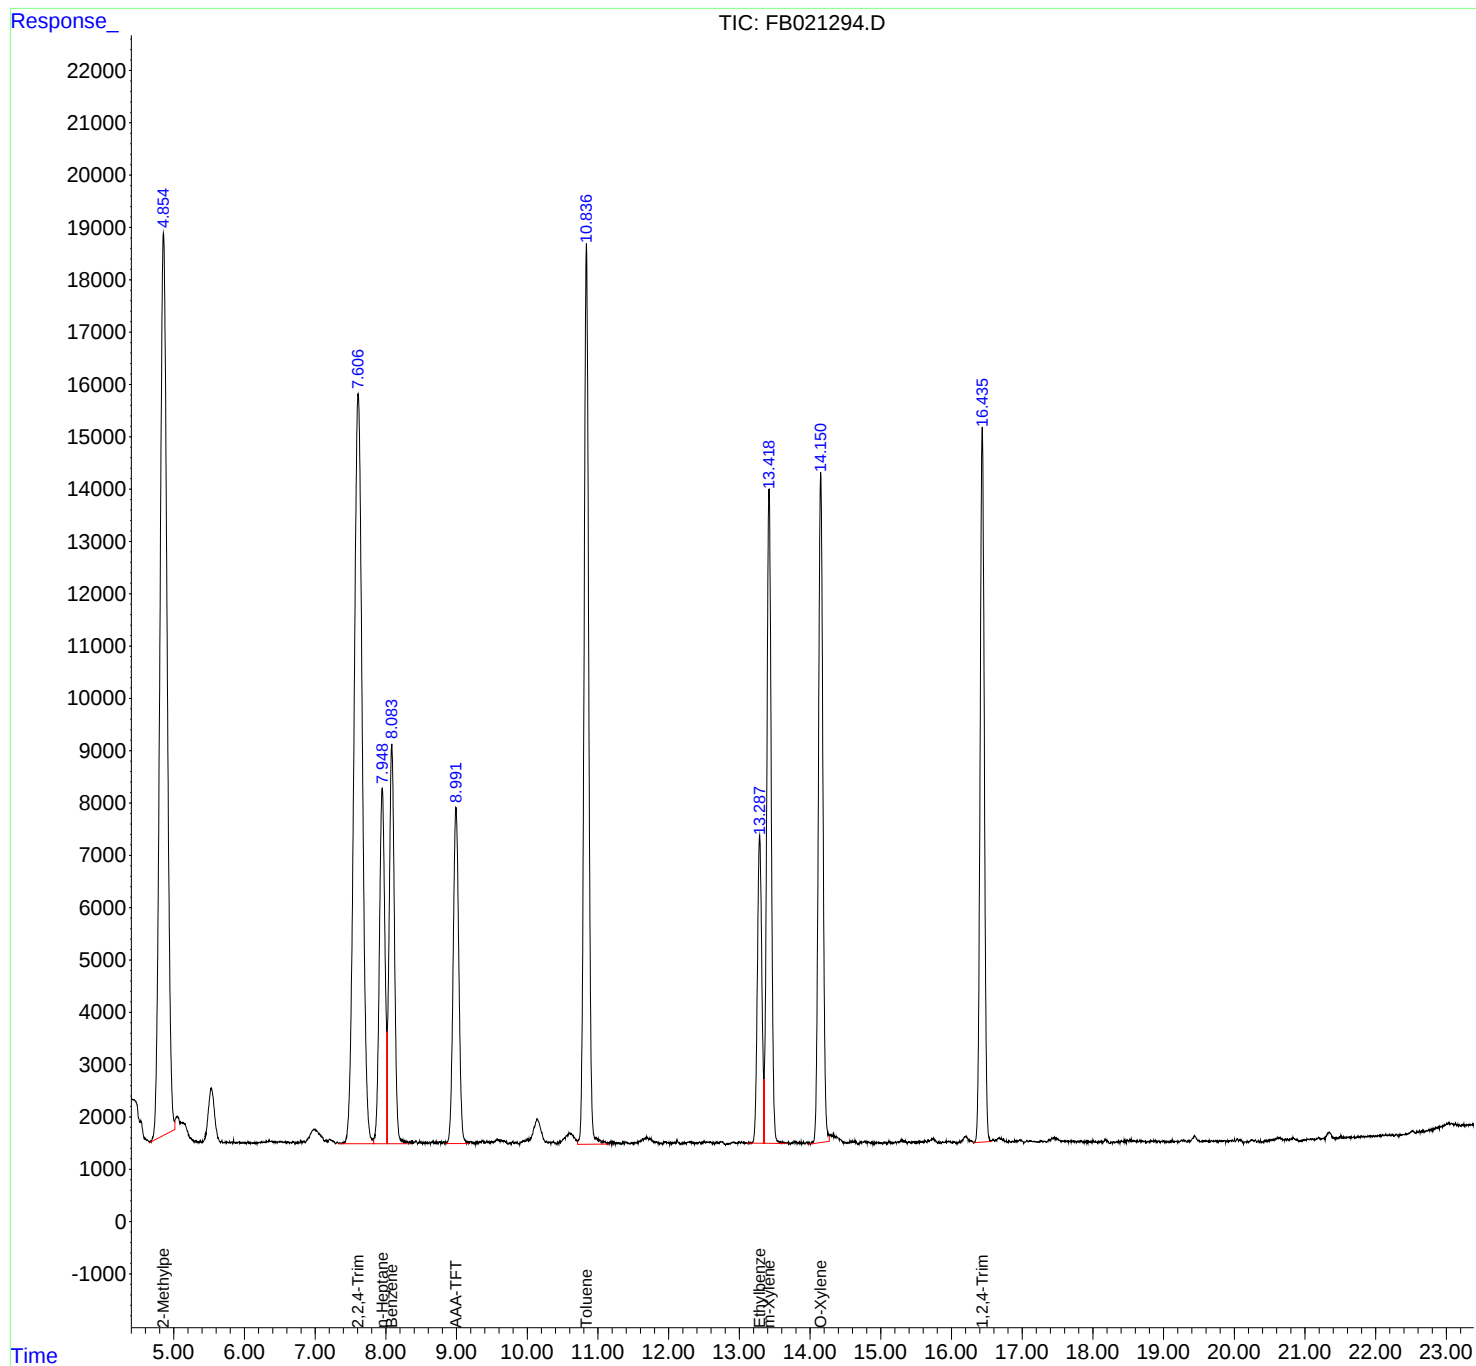

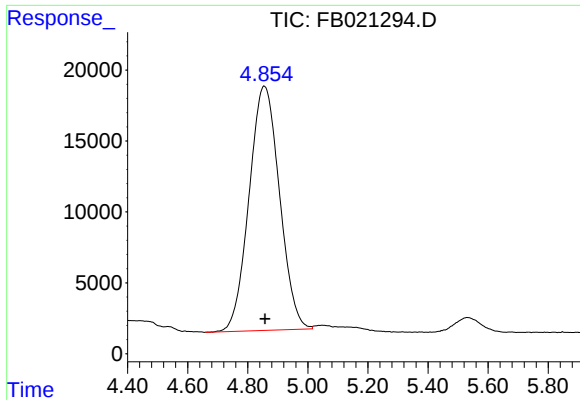


#1 2-Methylpentane

R.T.: 4.855 min
Delta R.T.: -0.003 min
Response: 1212485
Conc: 32.25 ng/ml

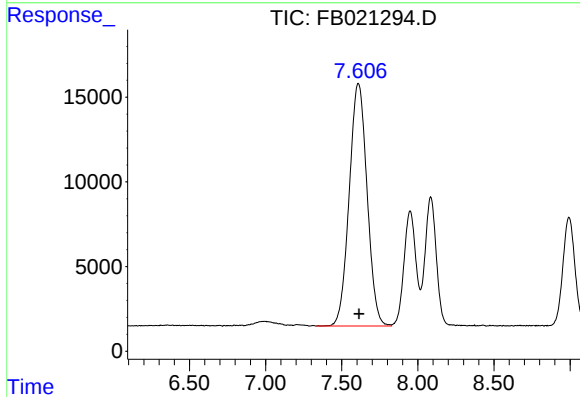


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: -0.005 min
Response: 1168543
Conc: 34.22 ng/ml

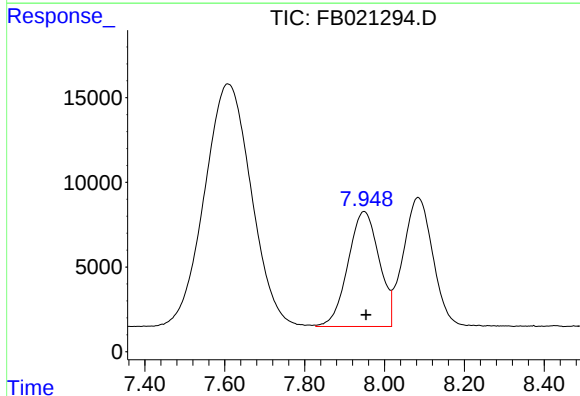


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: -0.005 min
Response: 368237
Conc: 11.30 ng/ml

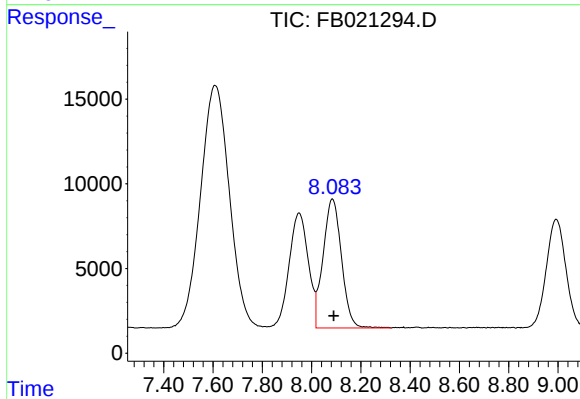


#4 Benzene

R.T.: 8.085 min
Delta R.T.: -0.005 min
Response: 395941
Conc: 11.47 ng/ml

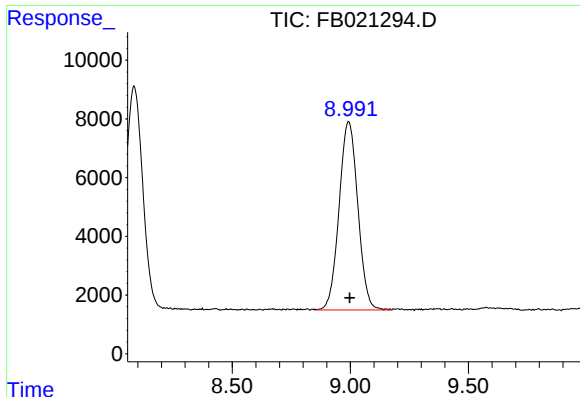


#5 AAA-TFT

R.T.: 8.993 min
Delta R.T.: -0.005 min
Response: 354078
Conc: 24.01 ng/ml

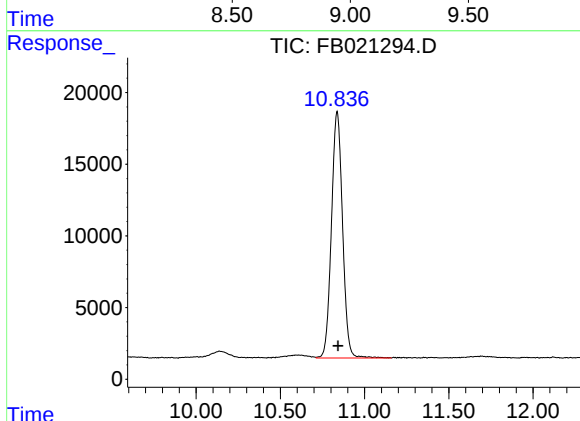


#6 Toluene

R.T.: 10.837 min
Delta R.T.: -0.005 min
Response: 789865
Conc: 33.32 ng/ml

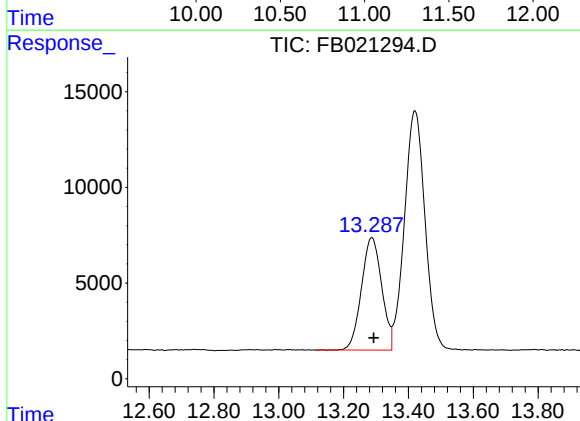


#7 Ethylbenzene

R.T.: 13.287 min
Delta R.T.: -0.006 min
Response: 254525
Conc: 10.89 ng/ml

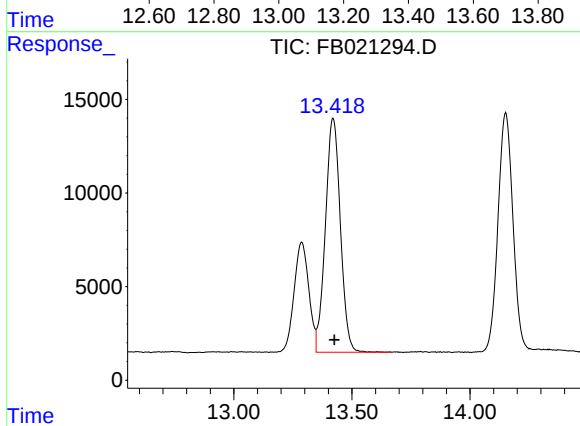

#8 m-Xylene

R.T.: 13.421 min
Delta R.T.: -0.005 min
Response: 550830
Conc: 22.07 ng/ml

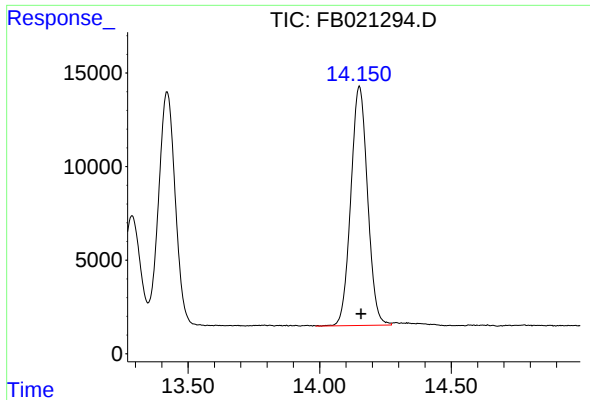


#9 O-Xylene

R.T.: 14.151 min

Delta R.T.: -0.006 min

Response: 564357

Conc: 21.63 ng/ml

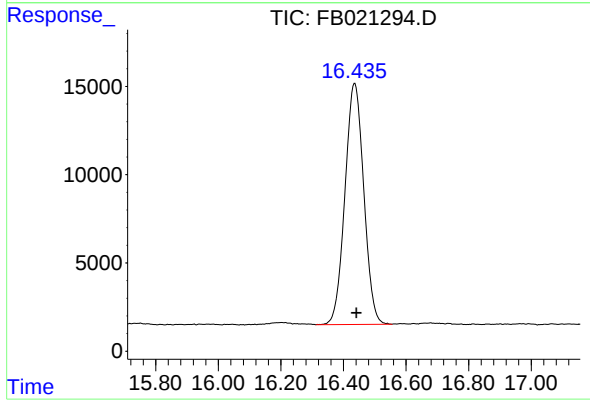

#10 1,2,4-Trimethylbenzene

R.T.: 16.436 min

Delta R.T.: -0.005 min

Response: 569335

Conc: 21.20 ng/ml