

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060319\
 Data File : FB021300.D
 Signal(s) : FID2B.CH
 Acq On : 3 Jun 2019 12:44
 Operator : MJ/SJ
 Sample : K2641-13MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 04 03:09:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.995	301134	20.424 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.856	908709	24.172 ng/ml
2) t 2,2,4-Trimethylpentane	7.610	710230	20.797 ng/ml
3) t n-Heptane	7.950	72964	2.238 ng/ml
4) t Benzene	8.086	333200	9.653 ng/ml
6) t Toluene	10.839	622440	26.261 ng/ml
7) t Ethylbenzene	13.289	193439	8.278 ng/ml
8) t m-Xylene	13.423	365426	14.640 ng/ml
9) t O-Xylene	14.154	442904	16.978 ng/ml
10) t 1,2,4-Trimethylbenzene	16.438	264723	9.857 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060319\
Data File : FB021300.D
Signal(s) : FID2B.CH
Acq On : 3 Jun 2019 12:44
Operator : MJ/SJ
Sample : K2641-13MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 04 03:09:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

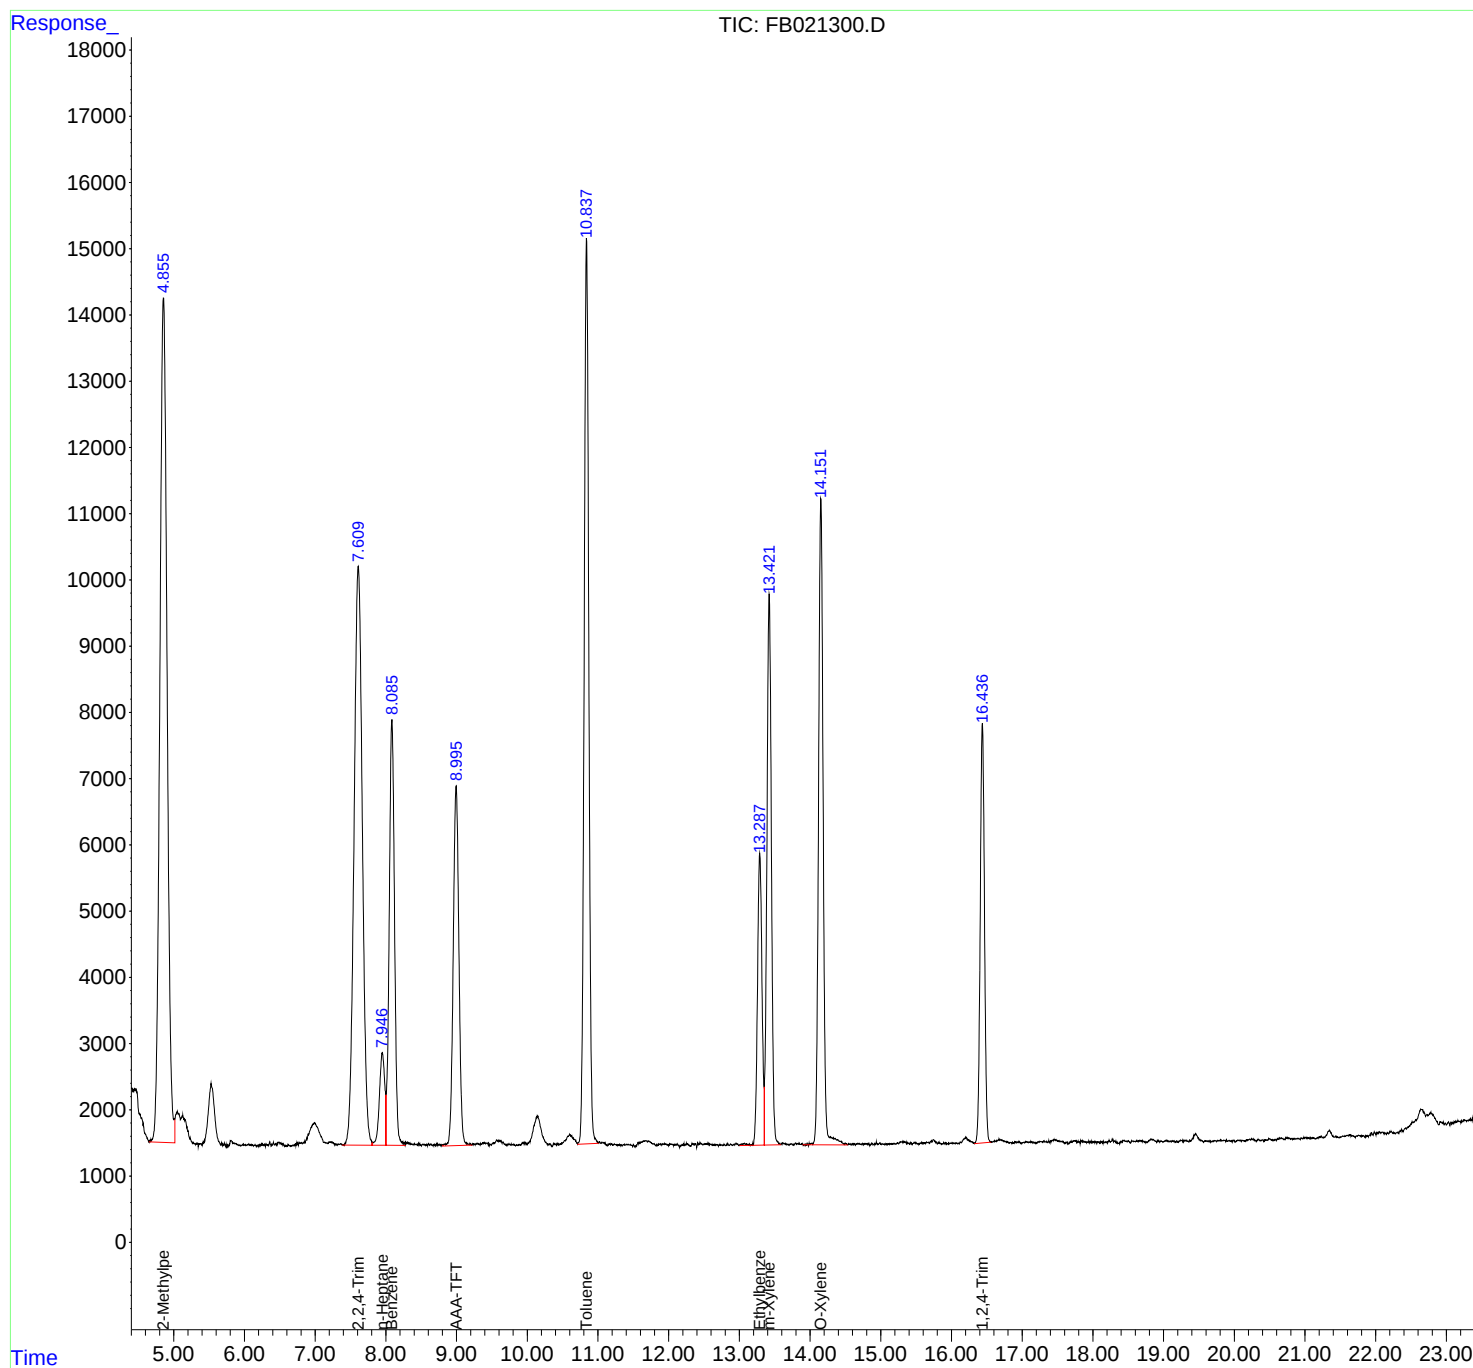

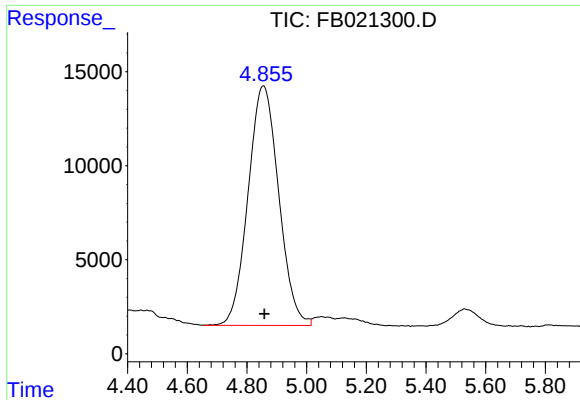


#1 2-Methylpentane

R.T.: 4.856 min
Delta R.T.: -0.002 min
Response: 908709
Conc: 24.17 ng/ml

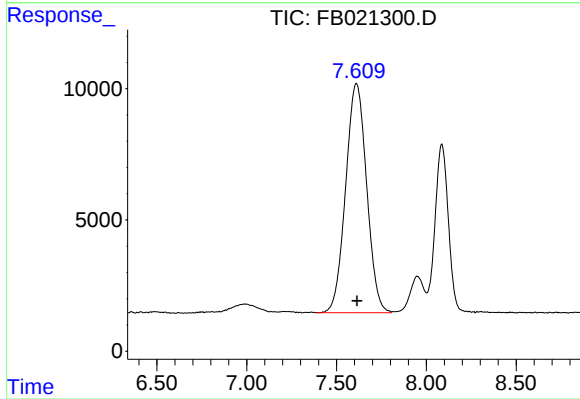


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: -0.004 min
Response: 710230
Conc: 20.80 ng/ml

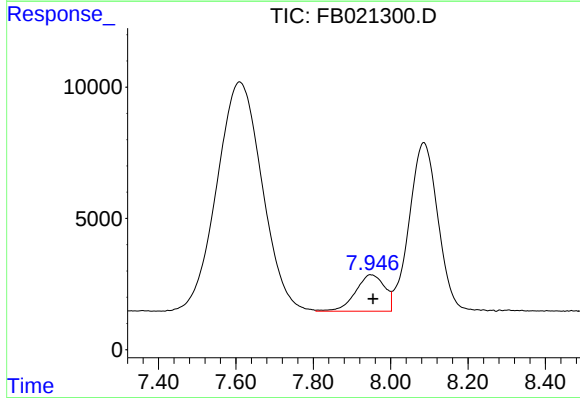


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: -0.005 min
Response: 72964
Conc: 2.24 ng/ml

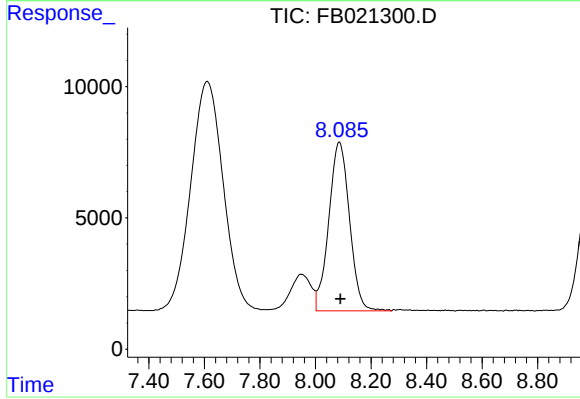


#4 Benzene

R.T.: 8.086 min
Delta R.T.: -0.004 min
Response: 333200
Conc: 9.65 ng/ml

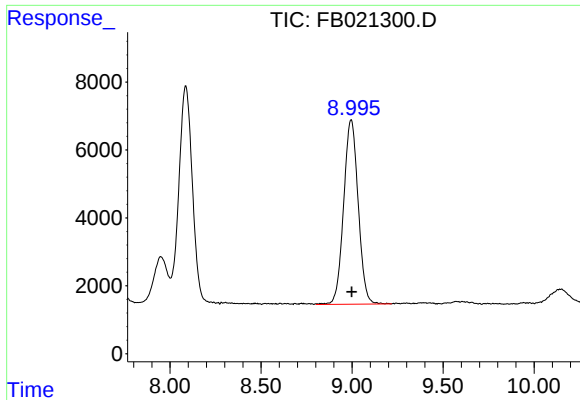


#5 AAA-TFT

R.T.: 8.995 min
Delta R.T.: -0.003 min
Response: 301134
Conc: 20.42 ng/ml

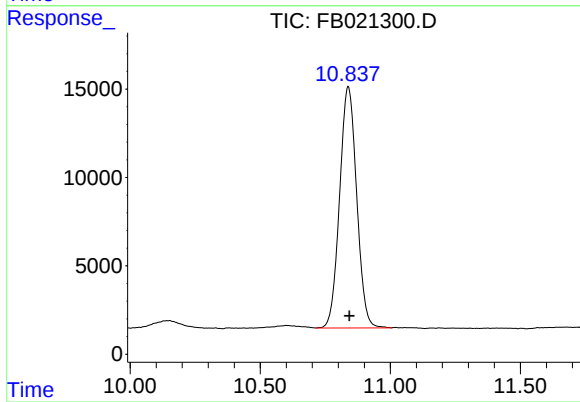


#6 Toluene

R.T.: 10.839 min
Delta R.T.: -0.004 min
Response: 622440
Conc: 26.26 ng/ml

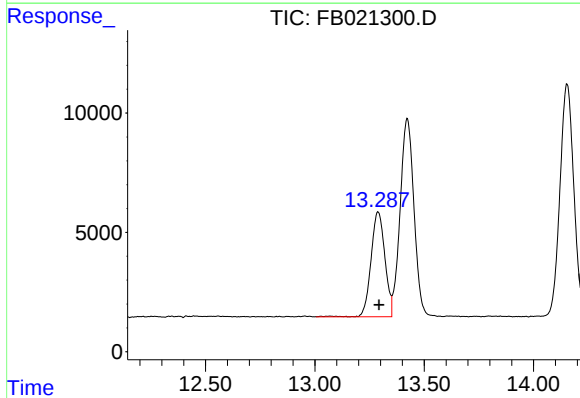


#7 Ethylbenzene

R.T.: 13.289 min
Delta R.T.: -0.004 min
Response: 193439
Conc: 8.28 ng/ml

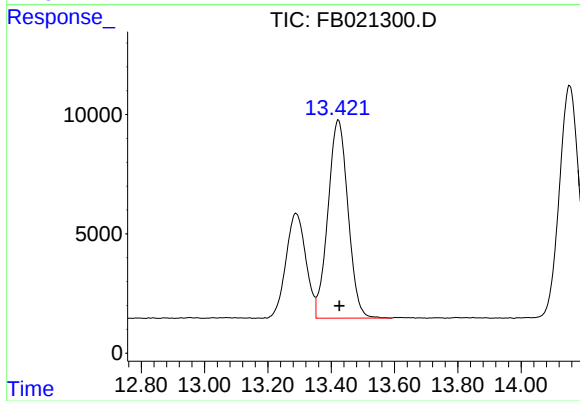

#8 m-Xylene

R.T.: 13.423 min
Delta R.T.: -0.003 min
Response: 365426
Conc: 14.64 ng/ml

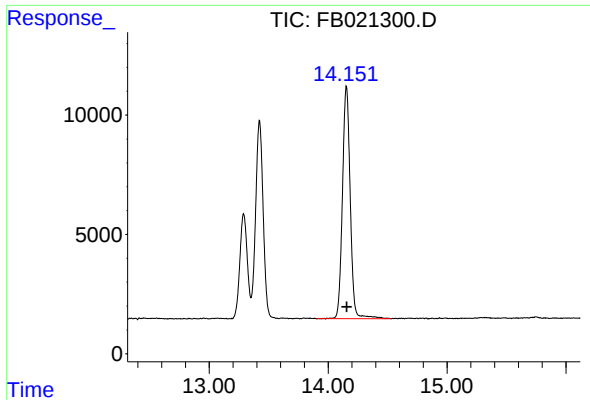


#9 O-Xylene

R.T.: 14.154 min

Delta R.T.: -0.003 min

Response: 442904

Conc: 16.98 ng/ml

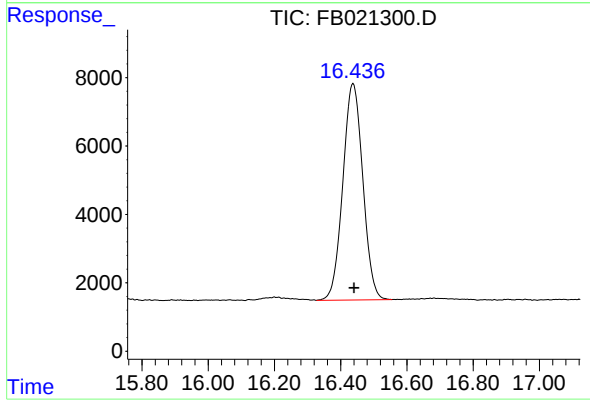

#10 1,2,4-Trimethylbenzene

R.T.: 16.438 min

Delta R.T.: -0.003 min

Response: 264723

Conc: 9.86 ng/ml