

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060319\
 Data File : FB021301.D
 Signal(s) : FID2B.CH
 Acq On : 3 Jun 2019 13:14
 Operator : MJ/SJ
 Sample : K2641-13MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 04 03:09:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.995	279127	18.931 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.857	866285	23.043 ng/ml
2) t 2,2,4-Trimethylpentane	7.611	711921	20.847 ng/ml
3) t n-Heptane	7.951	74425	2.283 ng/ml
4) t Benzene	8.087	329879	9.557 ng/ml
6) t Toluene	10.839	601671	25.385 ng/ml
7) t Ethylbenzene	13.290	186879	7.998 ng/ml
8) t m-Xylene	13.423	368840	14.777 ng/ml
9) t O-Xylene	14.153	432471	16.578 ng/ml
10) t 1,2,4-Trimethylbenzene	16.438	291654	10.860 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060319\
Data File : FB021301.D
Signal(s) : FID2B.CH
Acq On : 3 Jun 2019 13:14
Operator : MJ/SJ
Sample : K2641-13MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 04 03:09:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

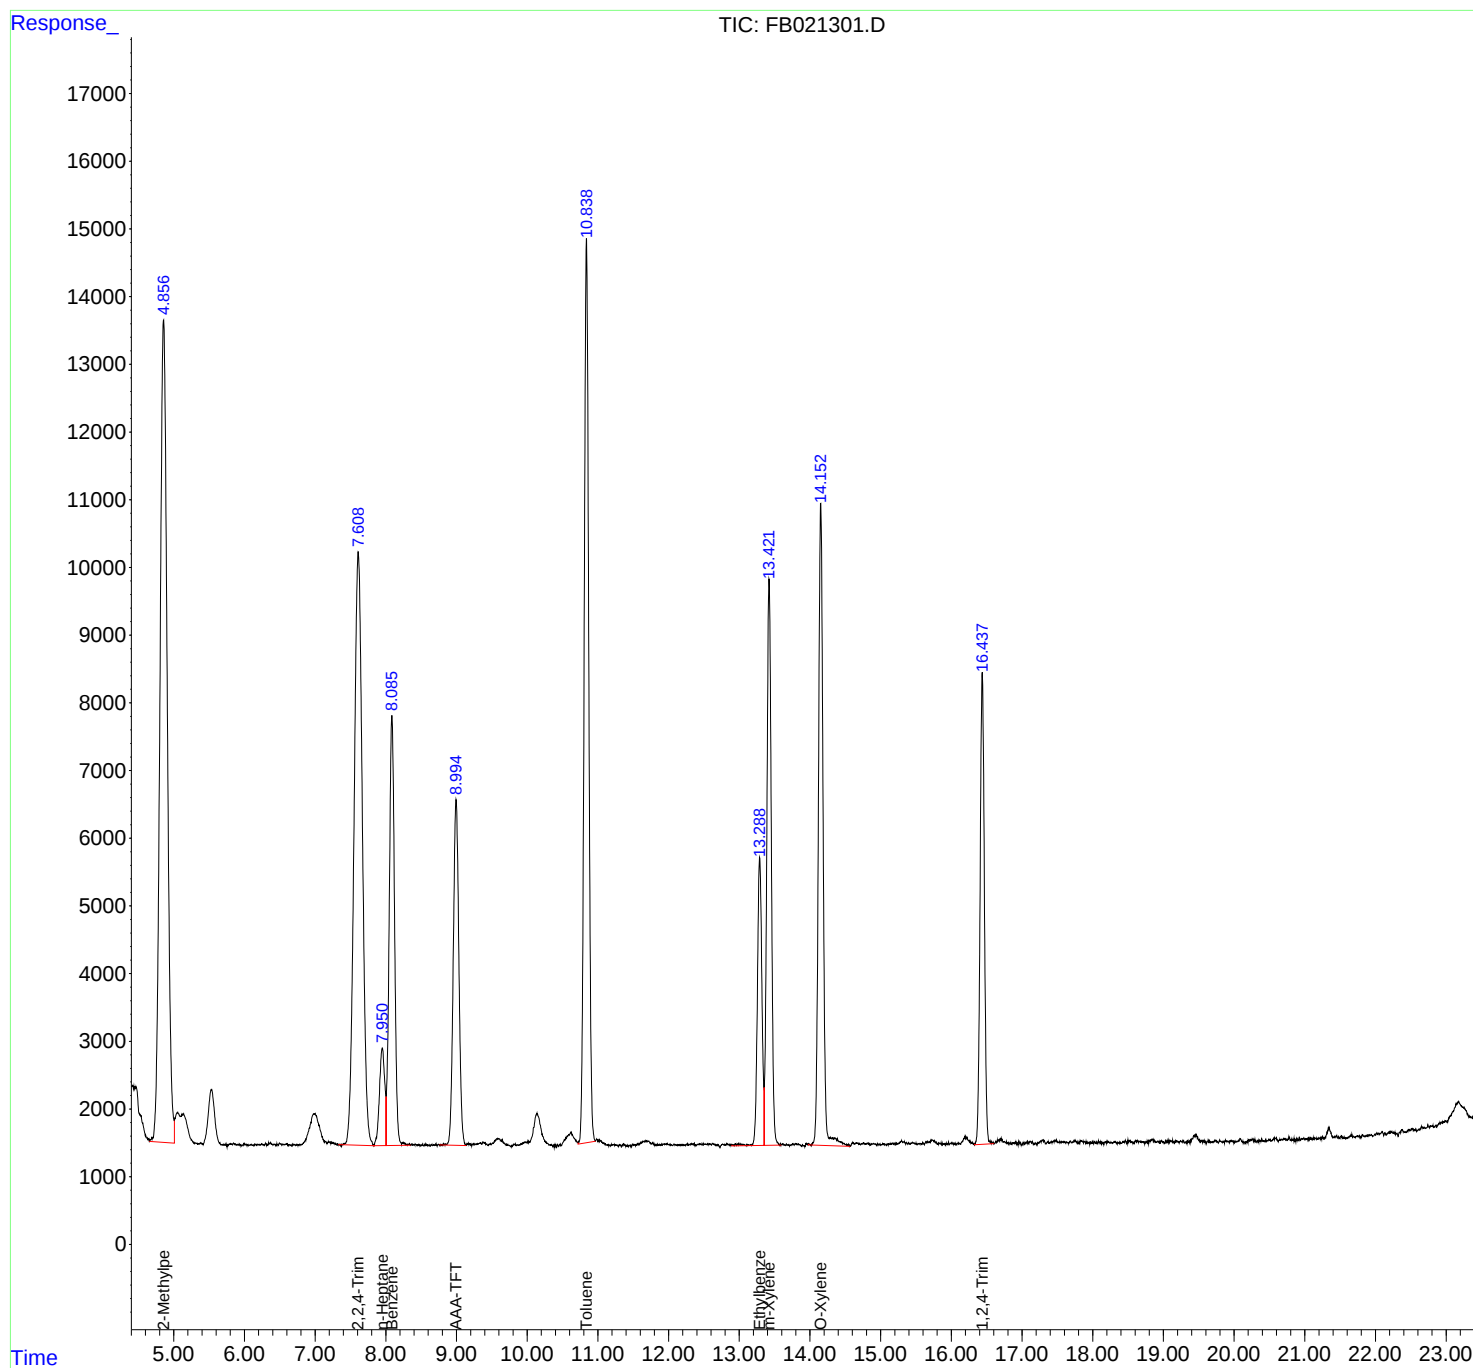

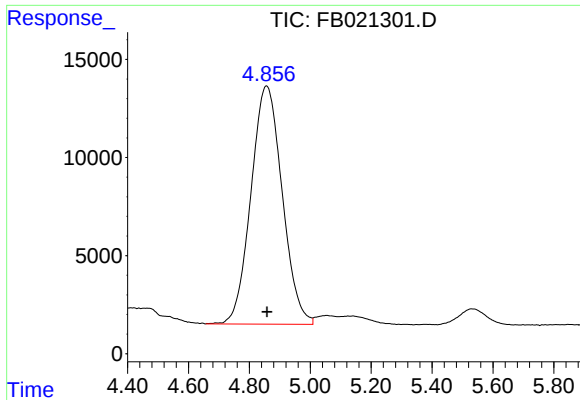


#1 2-Methylpentane

R.T.: 4.857 min
Delta R.T.: -0.001 min
Response: 866285
Conc: 23.04 ng/ml

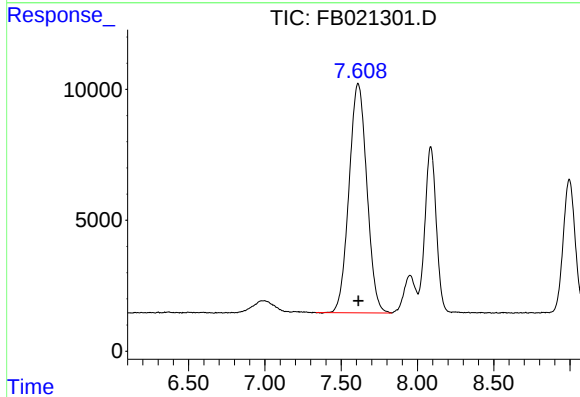


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: -0.003 min
Response: 711921
Conc: 20.85 ng/ml

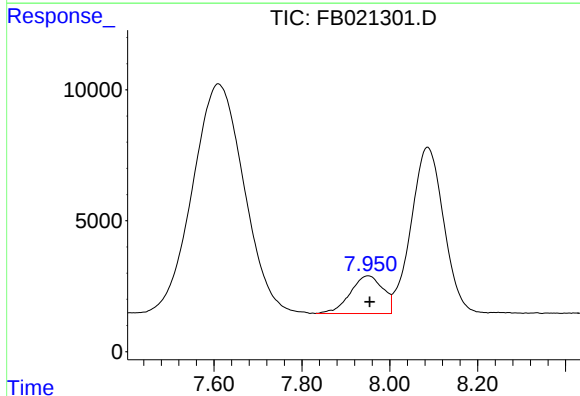


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: -0.003 min
Response: 74425
Conc: 2.28 ng/ml

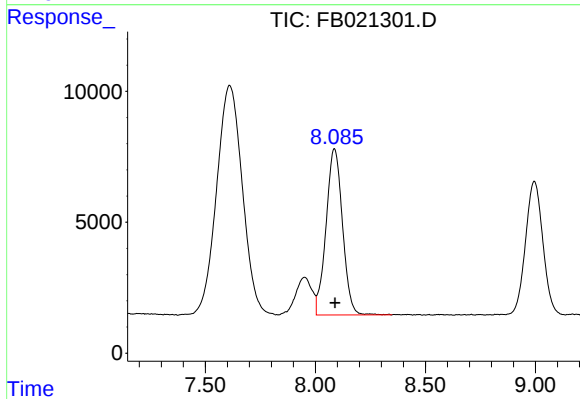


#4 Benzene

R.T.: 8.087 min
Delta R.T.: -0.003 min
Response: 329879
Conc: 9.56 ng/ml

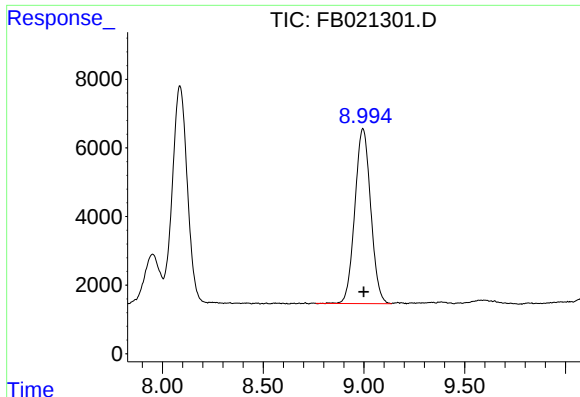


#5 AAA-TFT

R.T.: 8.995 min
Delta R.T.: -0.003 min
Response: 279127
Conc: 18.93 ng/ml

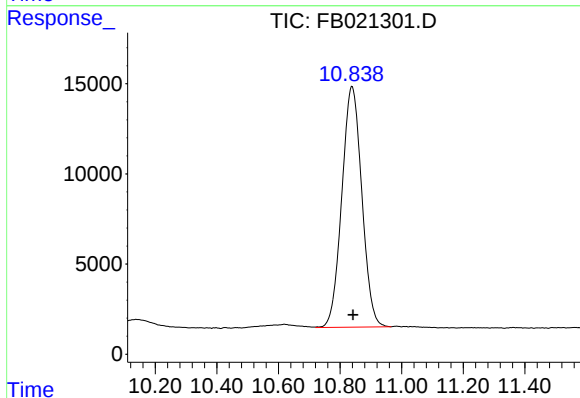


#6 Toluene

R.T.: 10.839 min
Delta R.T.: -0.003 min
Response: 601671
Conc: 25.38 ng/ml

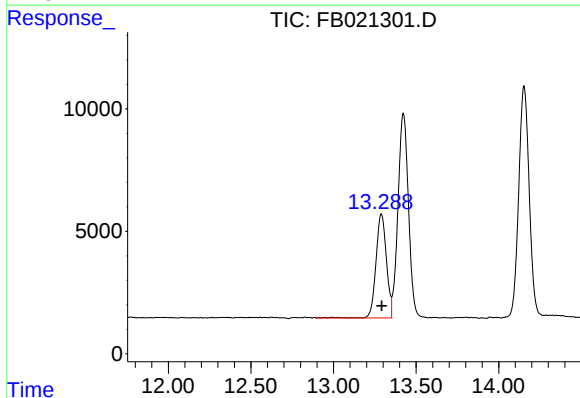


#7 Ethylbenzene

R.T.: 13.290 min
Delta R.T.: -0.004 min
Response: 186879
Conc: 8.00 ng/ml

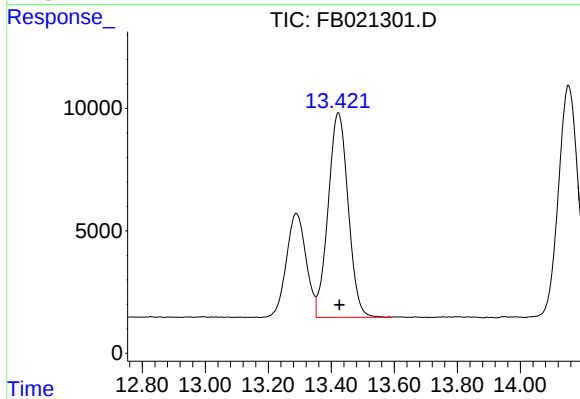


#8 m-Xylene

R.T.: 13.423 min
Delta R.T.: -0.003 min
Response: 368840
Conc: 14.78 ng/ml

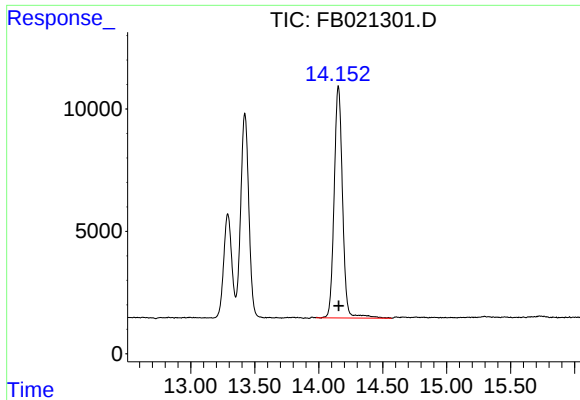

#9 O-Xylene

R.T.: 14.153 min
Delta R.T.: -0.003 min
Response: 432471
Conc: 16.58 ng/ml

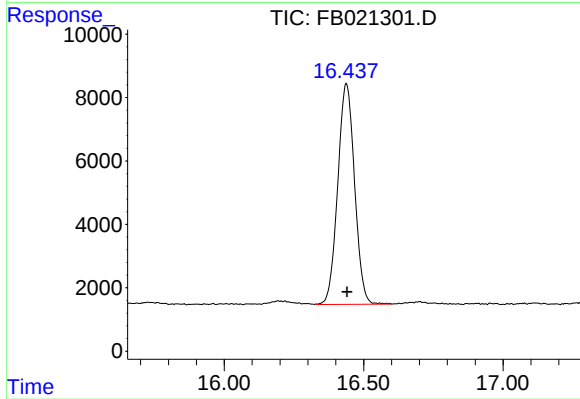

#10 1,2,4-Trimethylbenzene

R.T.: 16.438 min
Delta R.T.: -0.002 min
Response: 291654
Conc: 10.86 ng/ml