

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060321\
 Data File : FB025827.D
 Signal(s) : FID2B.CH
 Acq On : 3 Jun 2021 10:17
 Operator : DD/AJ
 Sample : BSF0603S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0603S1

Integration File: Calibration.e
 Quant Time: Jul 12 08:04:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060221.M
 Quant Title :
 QLast Update : Wed Jun 02 14:44:25 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.227	408566	16.131 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.211	717265	25.716 ng/ml
2) t 2,2,4-Trimethylpentane	7.890	623153	26.474 ng/ml
3) t n-Heptane	8.207	315038	8.619 ng/ml
4) t Benzene	8.359	360516	8.288 ng/ml
6) t Toluene	11.043	1010700	24.989 ng/ml
7) t Ethylbenzene	13.446	316038	8.174 ng/ml
8) t m-Xylene	13.576	620244	16.300 ng/ml
9) t O-Xylene	14.298	569459	15.928 ng/ml
10) t 1,2,4-Trimethylbenzene	16.549	404418	16.109 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060321\
Data File : FB025827.D
Signal(s) : FID2B.CH
Acq On : 3 Jun 2021 10:17
Operator : DD/AJ
Sample : BSF0603S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0603S1

Integration File: Calibration.e
Quant Time: Jul 12 08:04:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060221.M
Quant Title :
QLast Update : Wed Jun 02 14:44:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

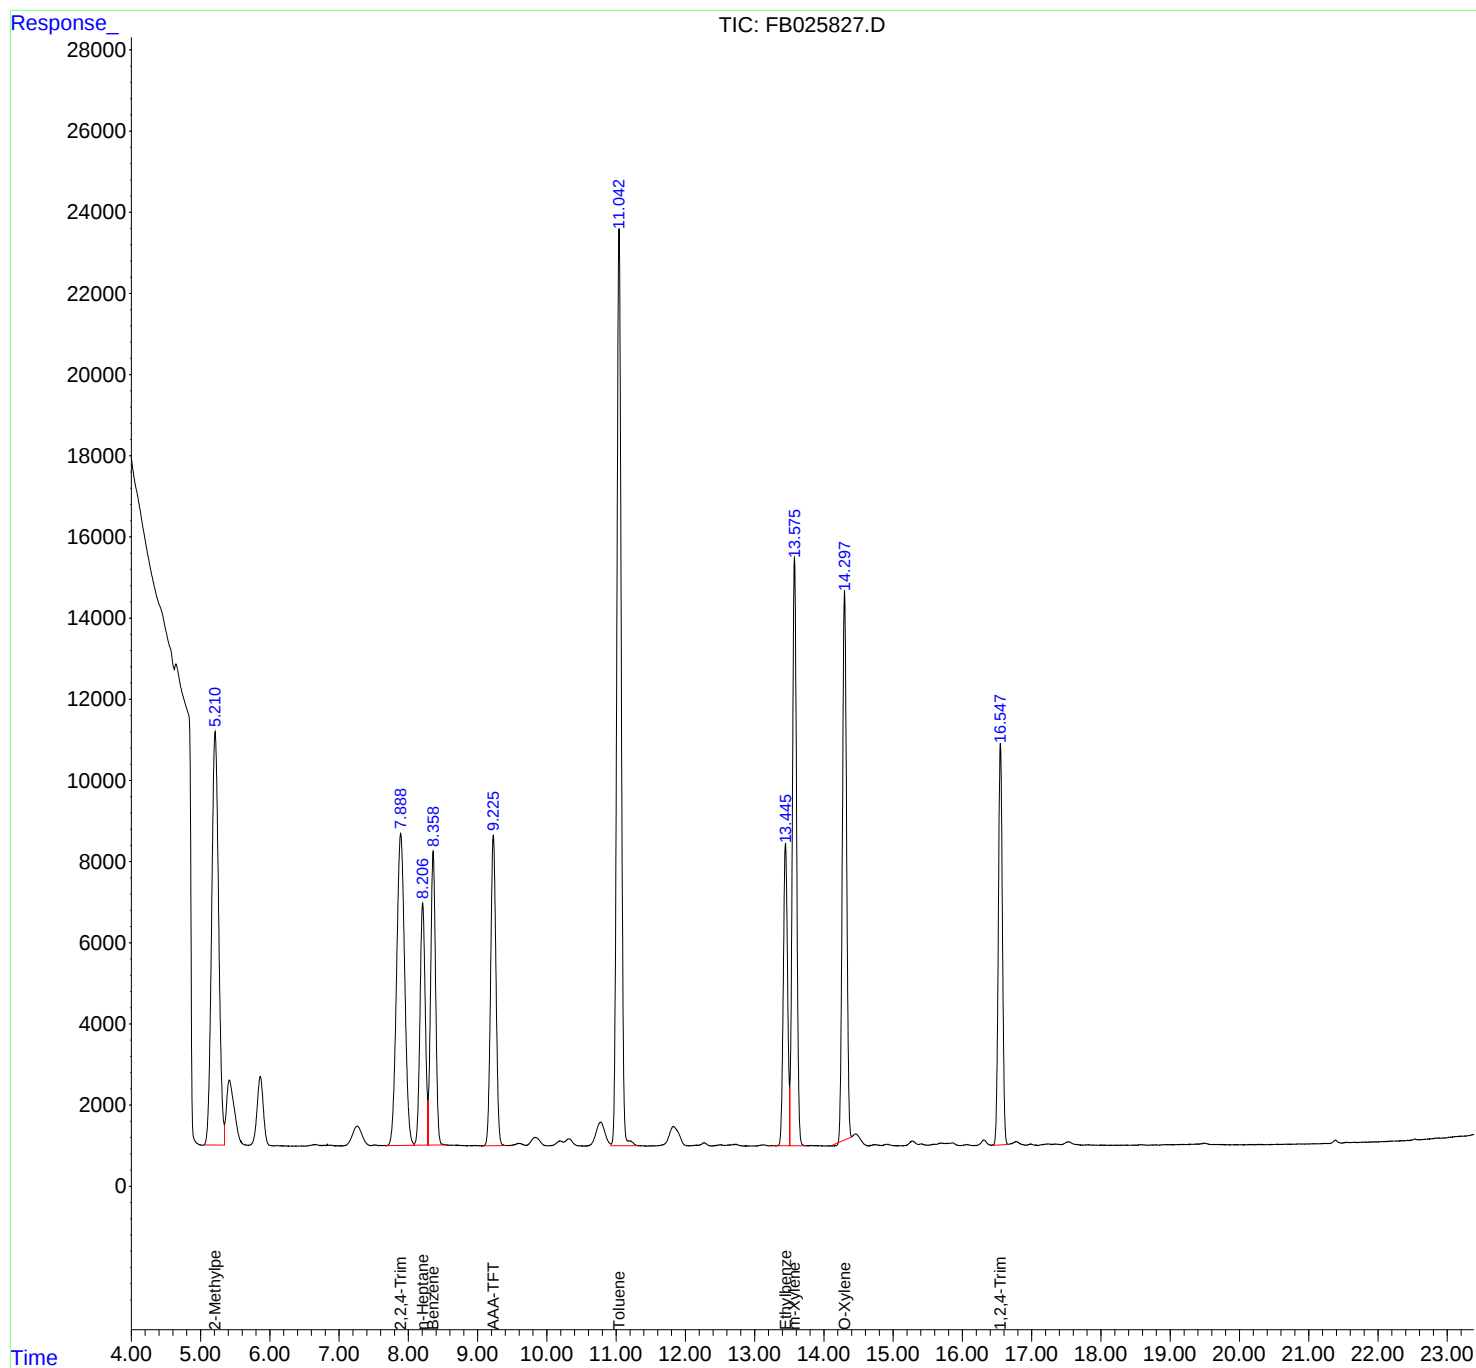


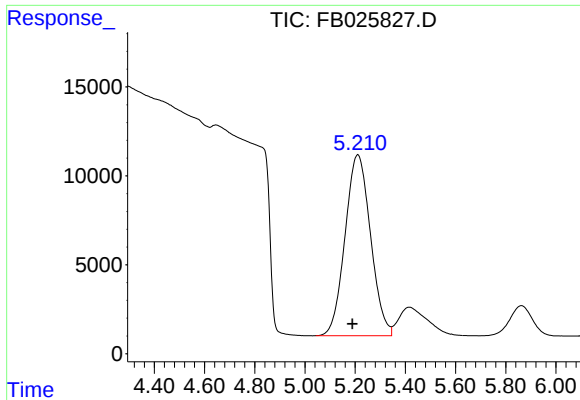

#1 2-Methylpentane


R.T.: 5.211 min
Delta R.T.: 0.022 min
Response: 717265
Conc: 25.72 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0603S1

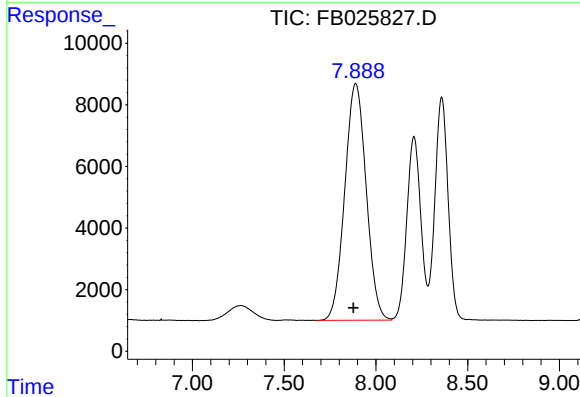


#2 2,2,4-Trimethylpentane

R.T.: 7.890 min
Delta R.T.: 0.011 min
Response: 623153
Conc: 26.47 ng/ml

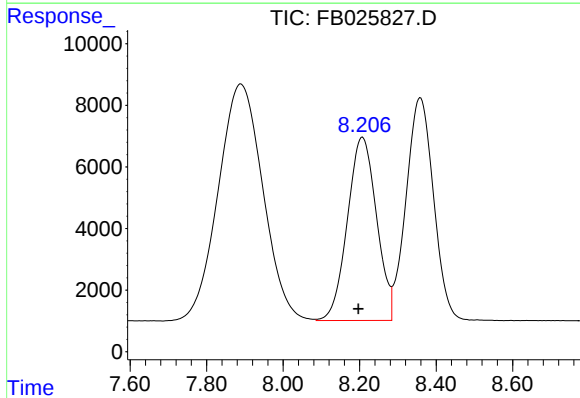


#3 n-Heptane

R.T.: 8.207 min
Delta R.T.: 0.010 min
Response: 315038
Conc: 8.62 ng/ml

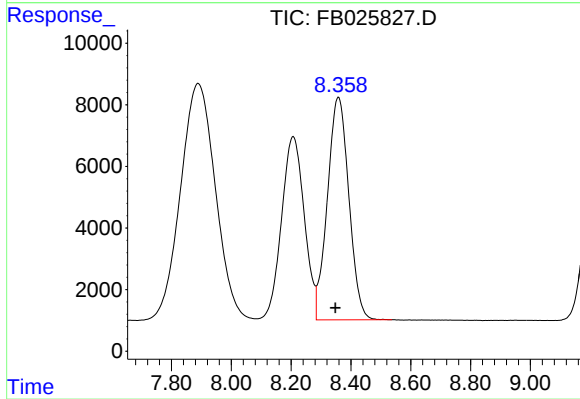

#4 Benzene


R.T.: 8.359 min
Delta R.T.: 0.011 min
Response: 360516
Conc: 8.29 ng/ml

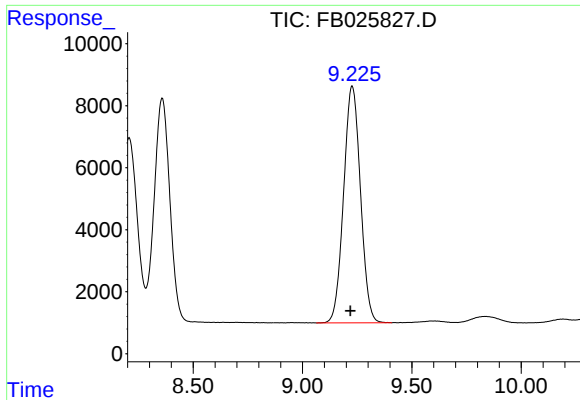

#5 AAA-TFT


R.T.: 9.227 min
 Delta R.T.: 0.008 min
 Response: 408566
 Conc: 16.13 ng/ml

Instrument :
 FID_B
 ClientSampleId :
 BSF0603S1

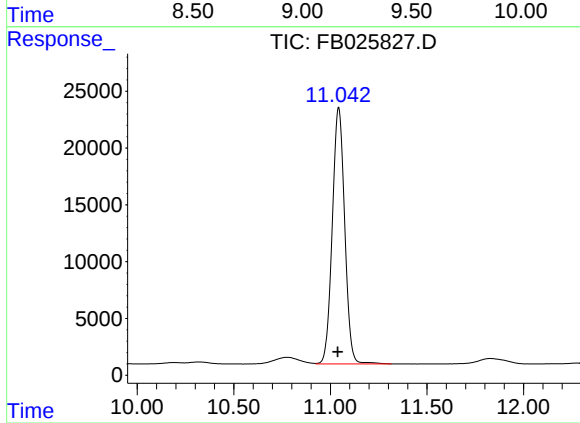


#6 Toluene

R.T.: 11.043 min
 Delta R.T.: 0.005 min
 Response: 1010700
 Conc: 24.99 ng/ml

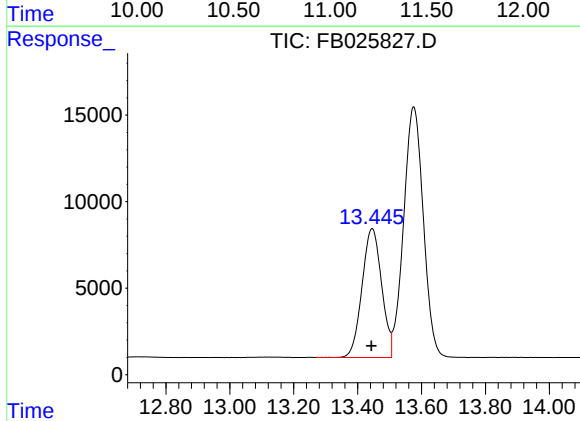


#7 Ethylbenzene

R.T.: 13.446 min
 Delta R.T.: 0.003 min
 Response: 316038
 Conc: 8.17 ng/ml

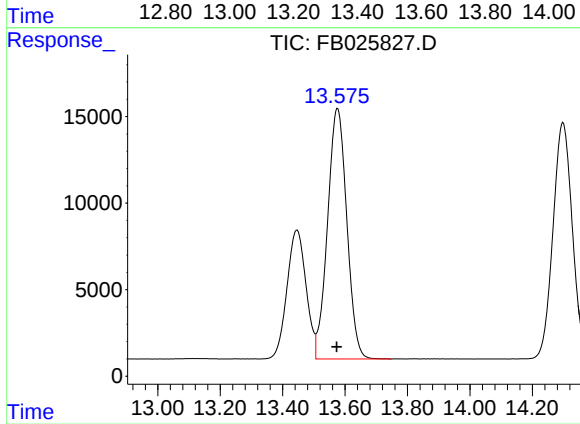

#8 m-Xylene


R.T.: 13.576 min
 Delta R.T.: 0.003 min
 Response: 620244
 Conc: 16.30 ng/ml

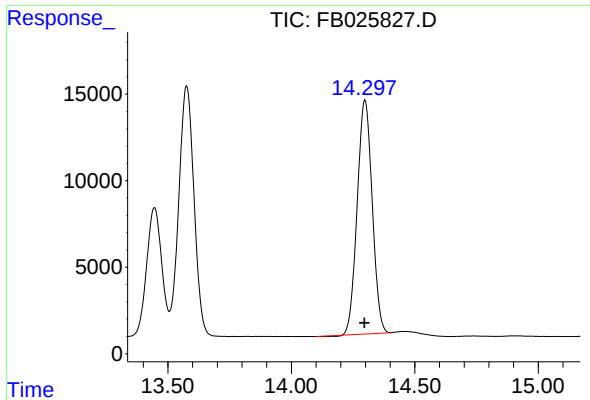

#9 O-Xylene

R.T.: 14.298 min
Delta R.T.: 0.003 min
Response: 569459
Conc: 15.93 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0603S1

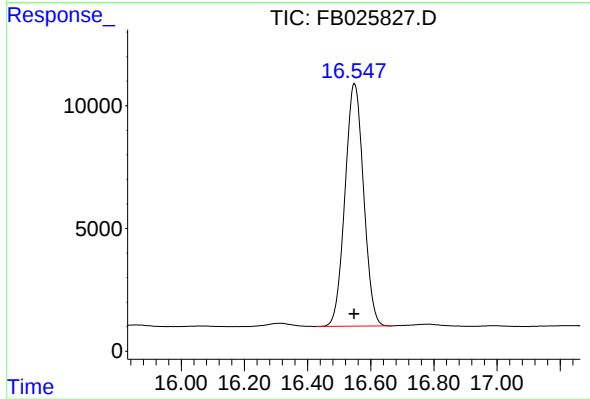

#10 1,2,4-Trimethylbenzene

R.T.: 16.549 min
Delta R.T.: 0.001 min
Response: 404418
Conc: 16.11 ng/ml