

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060321\
Data File : FB025830.D
Signal(s) : FID2B.CH
Acq On : 3 Jun 2021 14:24
Operator : DD/AJ
Sample : VBF0603S3
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0603S3

Integration File: Calibration.e
Quant Time: Jun 03 14:42:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060221.M
Quant Title :
QLast Update : Wed Jun 02 14:44:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.213	422915	16.698 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060321\
Data File : FB025830.D
Signal(s) : FID2B.CH
Acq On : 3 Jun 2021 14:24
Operator : DD/AJ
Sample : VBF0603S3
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0603S3

Integration File: Calibration.e
Quant Time: Jun 03 14:42:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060221.M
Quant Title :
QLast Update : Wed Jun 02 14:44:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

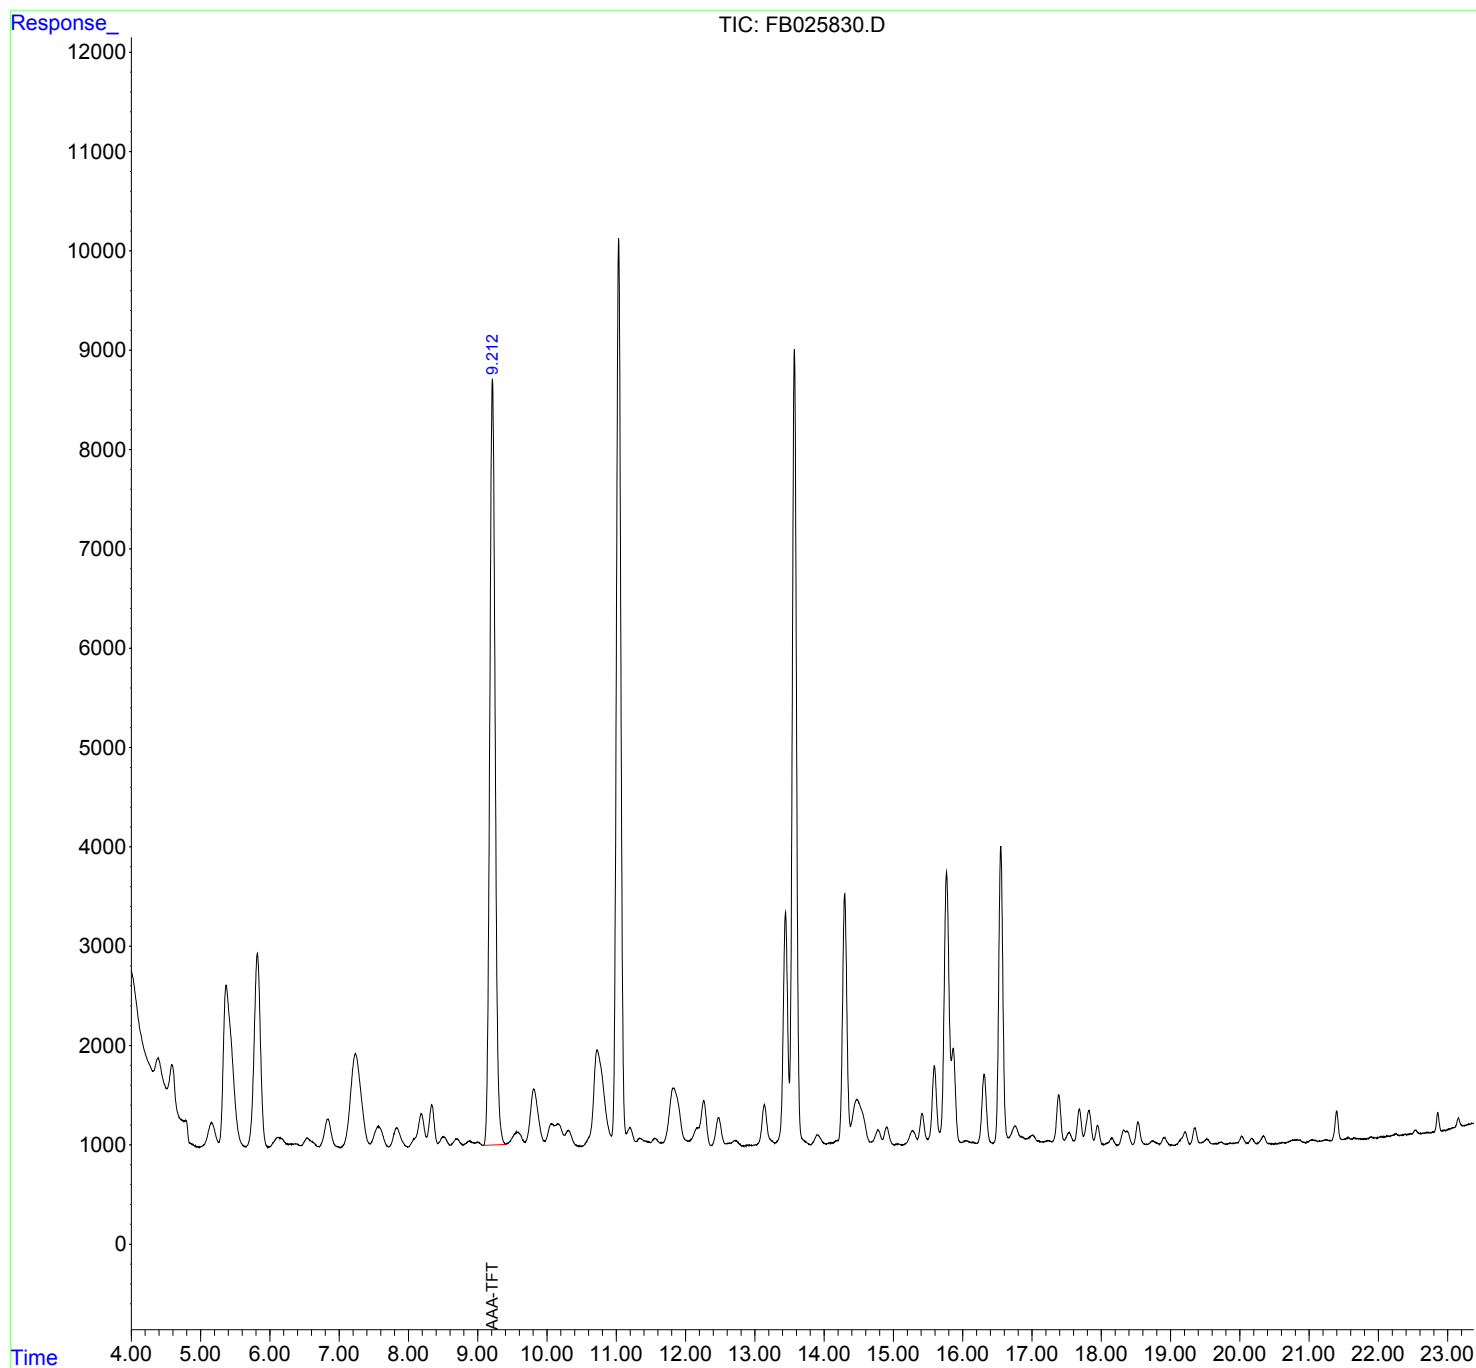

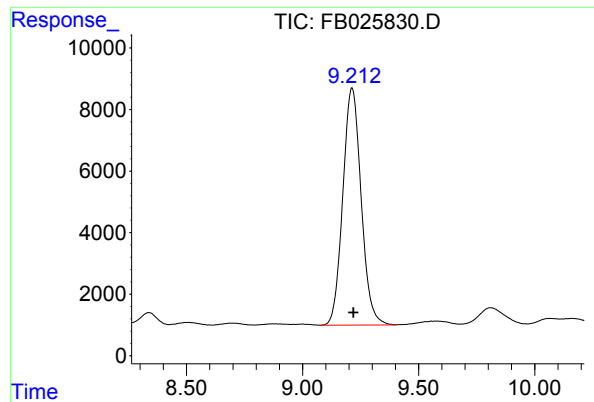

#5 AAA-TFT

R.T.: 9.213 min
Delta R.T.: -0.007 min
Response: 422915
Conc: 16.70 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0603S3