

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060321\
 Data File : FB025835.D
 Signal(s) : FID2B.CH
 Acq On : 3 Jun 2021 19:34
 Operator : DD/AJ
 Sample : BSF0603S2
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0603S2

Integration File: Calibration.e
 Quant Time: Jul 12 08:04:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060221.M
 Quant Title :
 QLast Update : Wed Jun 02 14:44:25 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.216	444951	17.568 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.167	719144	25.784 ng/ml
2) t 2,2,4-Trimethylpentane	7.869	568498	24.152 ng/ml
3) t n-Heptane	8.190	320539	8.770 ng/ml
4) t Benzene	8.341	381957	8.781 ng/ml
6) t Toluene	11.037	1272047	31.451 ng/ml
7) t Ethylbenzene	13.445	373119	9.651 ng/ml
8) t m-Xylene	13.575	807226	21.214 ng/ml
9) t O-Xylene	14.299	614595	17.191 ng/ml
10) t 1,2,4-Trimethylbenzene	16.552	415185	16.538 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060321\
Data File : FB025835.D
Signal(s) : FID2B.CH
Acq On : 3 Jun 2021 19:34
Operator : DD/AJ
Sample : BSF0603S2
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0603S2

Integration File: Calibration.e
Quant Time: Jul 12 08:04:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060221.M
Quant Title :
QLast Update : Wed Jun 02 14:44:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

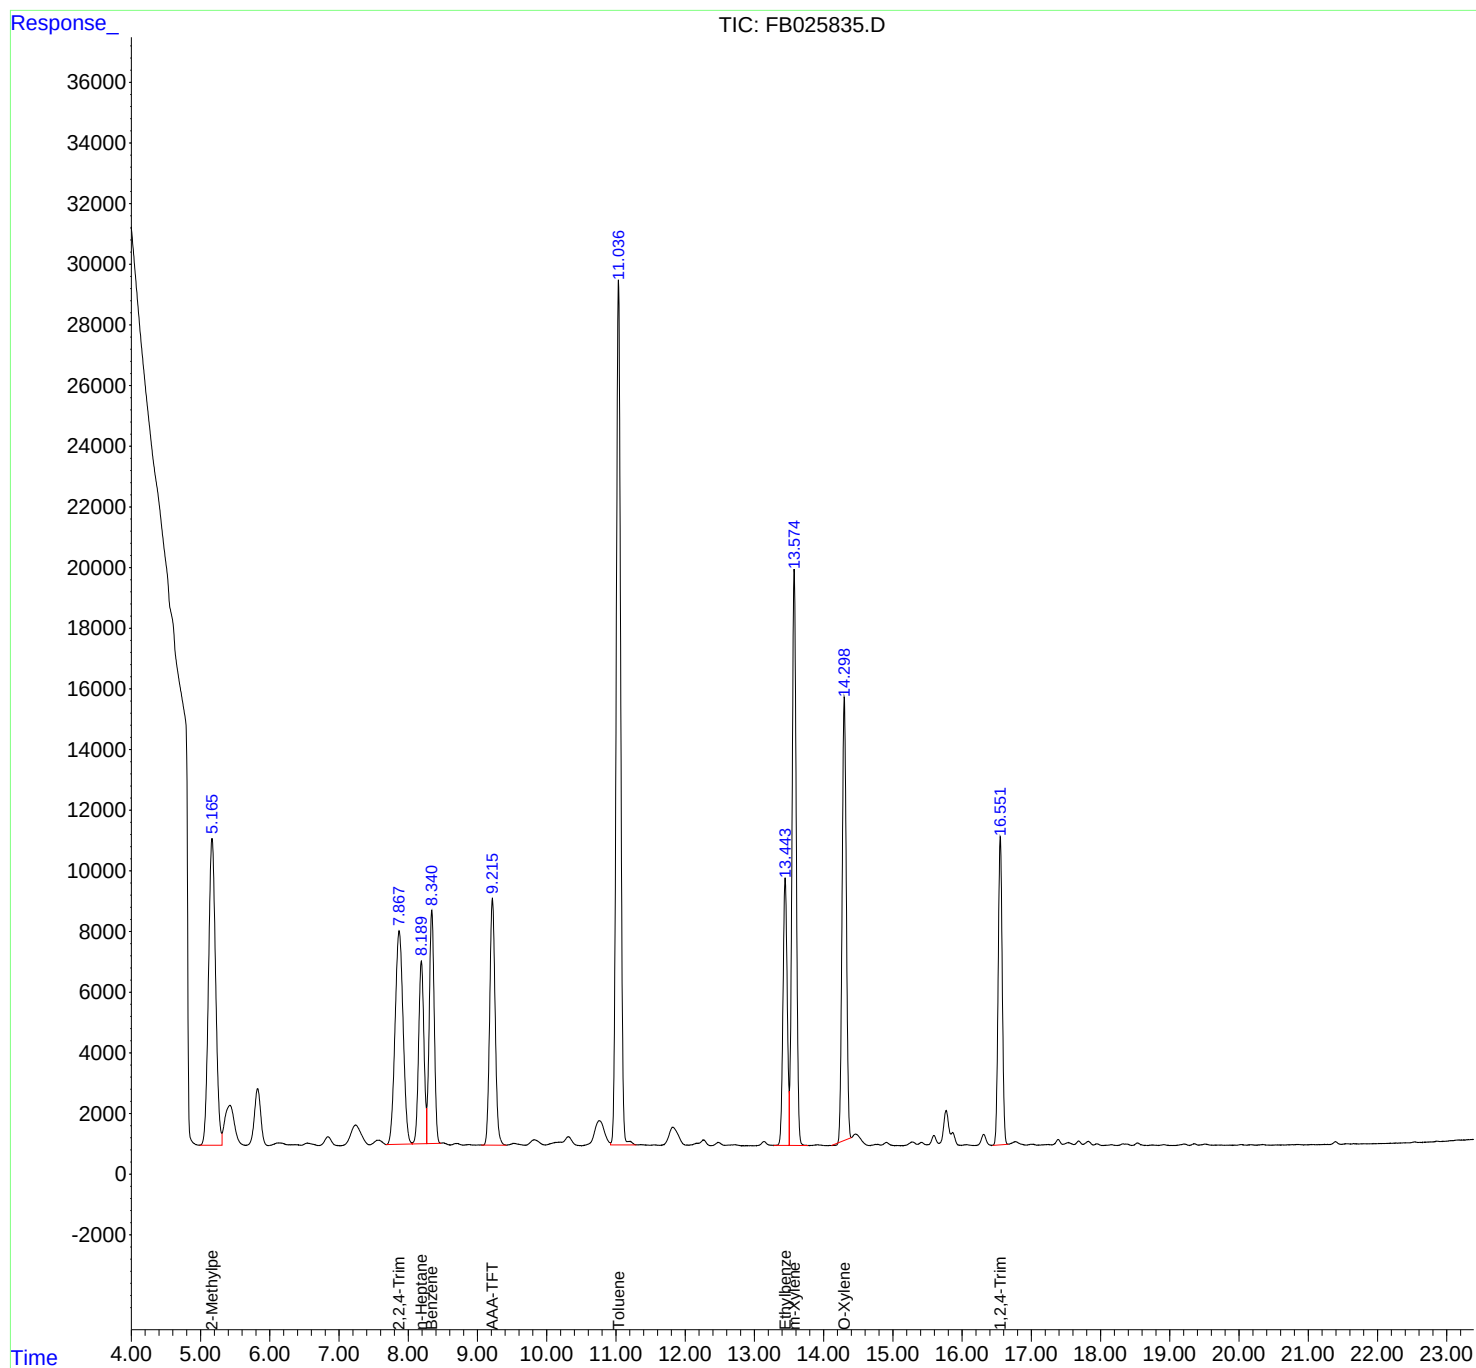


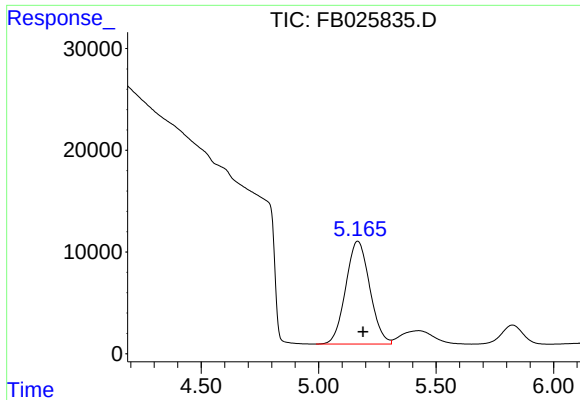

#1 2-Methylpentane


R.T.: 5.167 min
Delta R.T.: -0.022 min
Response: 719144
Conc: 25.78 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0603S2

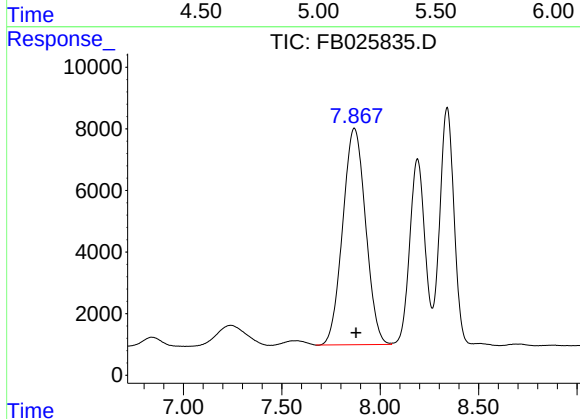


#2 2,2,4-Trimethylpentane

R.T.: 7.869 min
Delta R.T.: -0.010 min
Response: 568498
Conc: 24.15 ng/ml

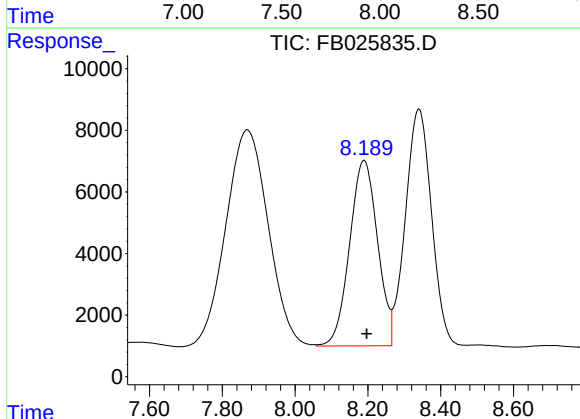


#3 n-Heptane

R.T.: 8.190 min
Delta R.T.: -0.007 min
Response: 320539
Conc: 8.77 ng/ml

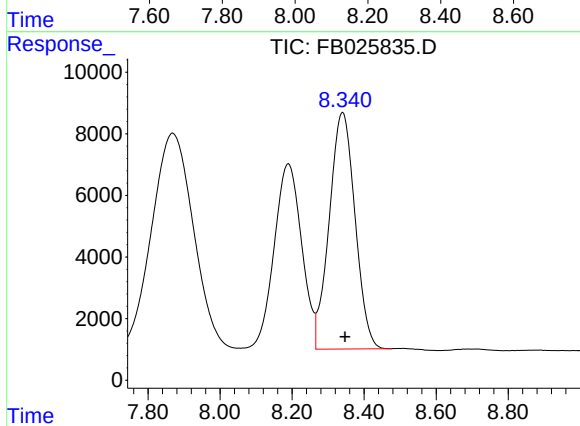

#4 Benzene


R.T.: 8.341 min
Delta R.T.: -0.007 min
Response: 381957
Conc: 8.78 ng/ml

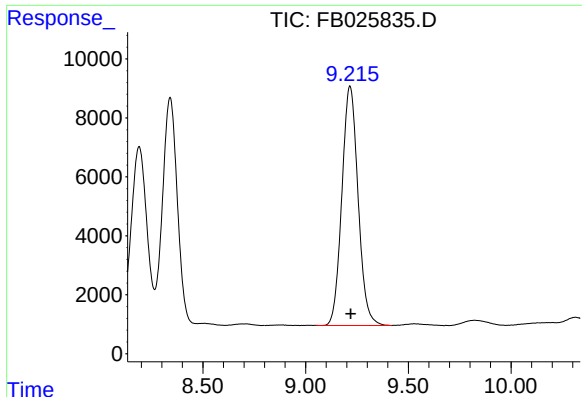

#5 AAA-TFT


R.T.: 9.216 min
Delta R.T.: -0.004 min
Response: 444951
Conc: 17.57 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0603S2

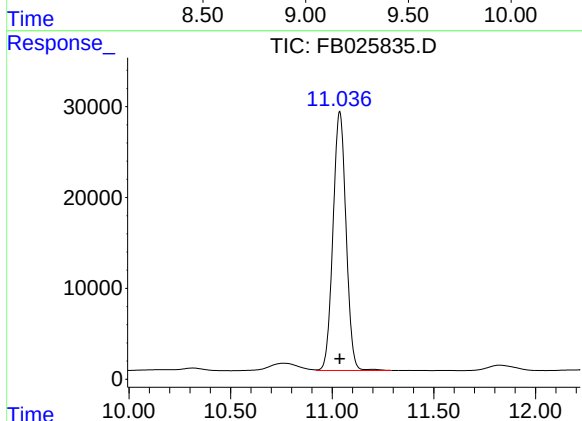


#6 Toluene

R.T.: 11.037 min
Delta R.T.: 0.000 min
Response: 1272047
Conc: 31.45 ng/ml

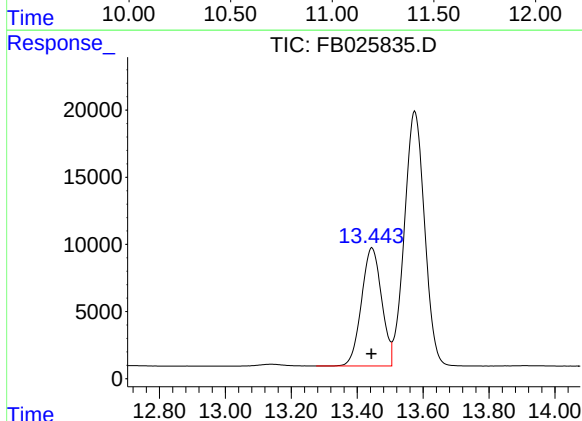


#7 Ethylbenzene

R.T.: 13.445 min
Delta R.T.: 0.002 min
Response: 373119
Conc: 9.65 ng/ml

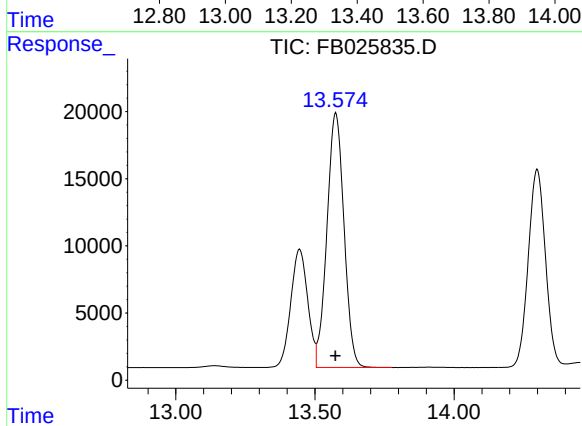

#8 m-Xylene


R.T.: 13.575 min
Delta R.T.: 0.002 min
Response: 807226
Conc: 21.21 ng/ml

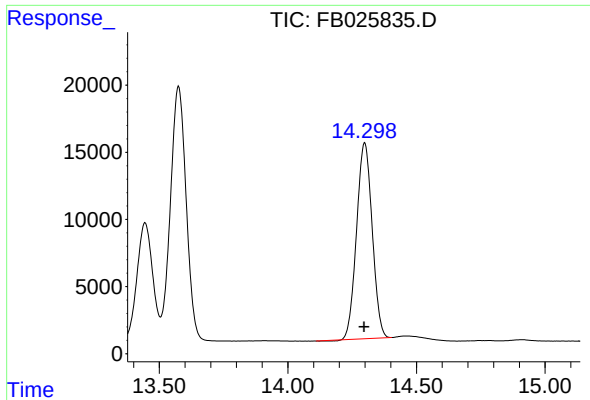

#9 O-Xylene

R.T.: 14.299 min
Delta R.T.: 0.003 min
Response: 614595
Conc: 17.19 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0603S2

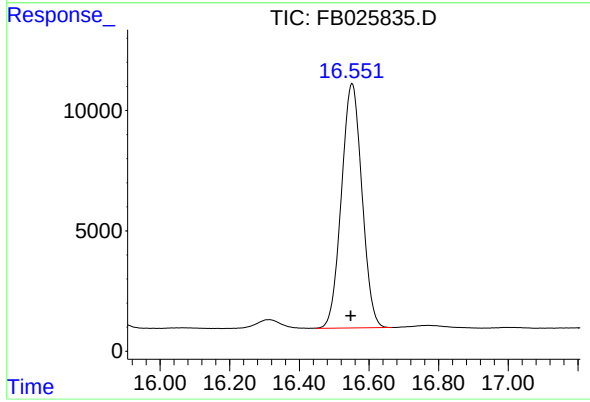

#10 1,2,4-Trimethylbenzene

R.T.: 16.552 min
Delta R.T.: 0.004 min
Response: 415185
Conc: 16.54 ng/ml