

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060323\
 Data File : FB029962.D
 Signal(s) : FID2B.CH
 Acq On : 3 Jun 2023 1:35
 Operator : YP/AJ
 Sample : 100 GRO STD
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 05 04:32:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:26:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	1305779	93.856 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	2828682	149.714 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	2973822	157.602 ng/ml
3) t n-Heptane	7.749	997082	51.511 ng/ml
4) t Benzene	7.886	1189476	53.139 ng/ml
6) t Toluene	10.620	3390778	156.234 ng/ml
7) t Ethylbenzene	13.056	1034455	51.159 ng/ml
8) t m-Xylene	13.189	2050638	101.969 ng/ml
9) t O-Xylene	13.915	1966938	100.918 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	1830935	97.753 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060323\
Data File : FB029962.D
Signal(s) : FID2B.CH
Acq On : 3 Jun 2023 1:35
Operator : YP/AJ
Sample : 100 GRO STD
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 05 04:32:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:26:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

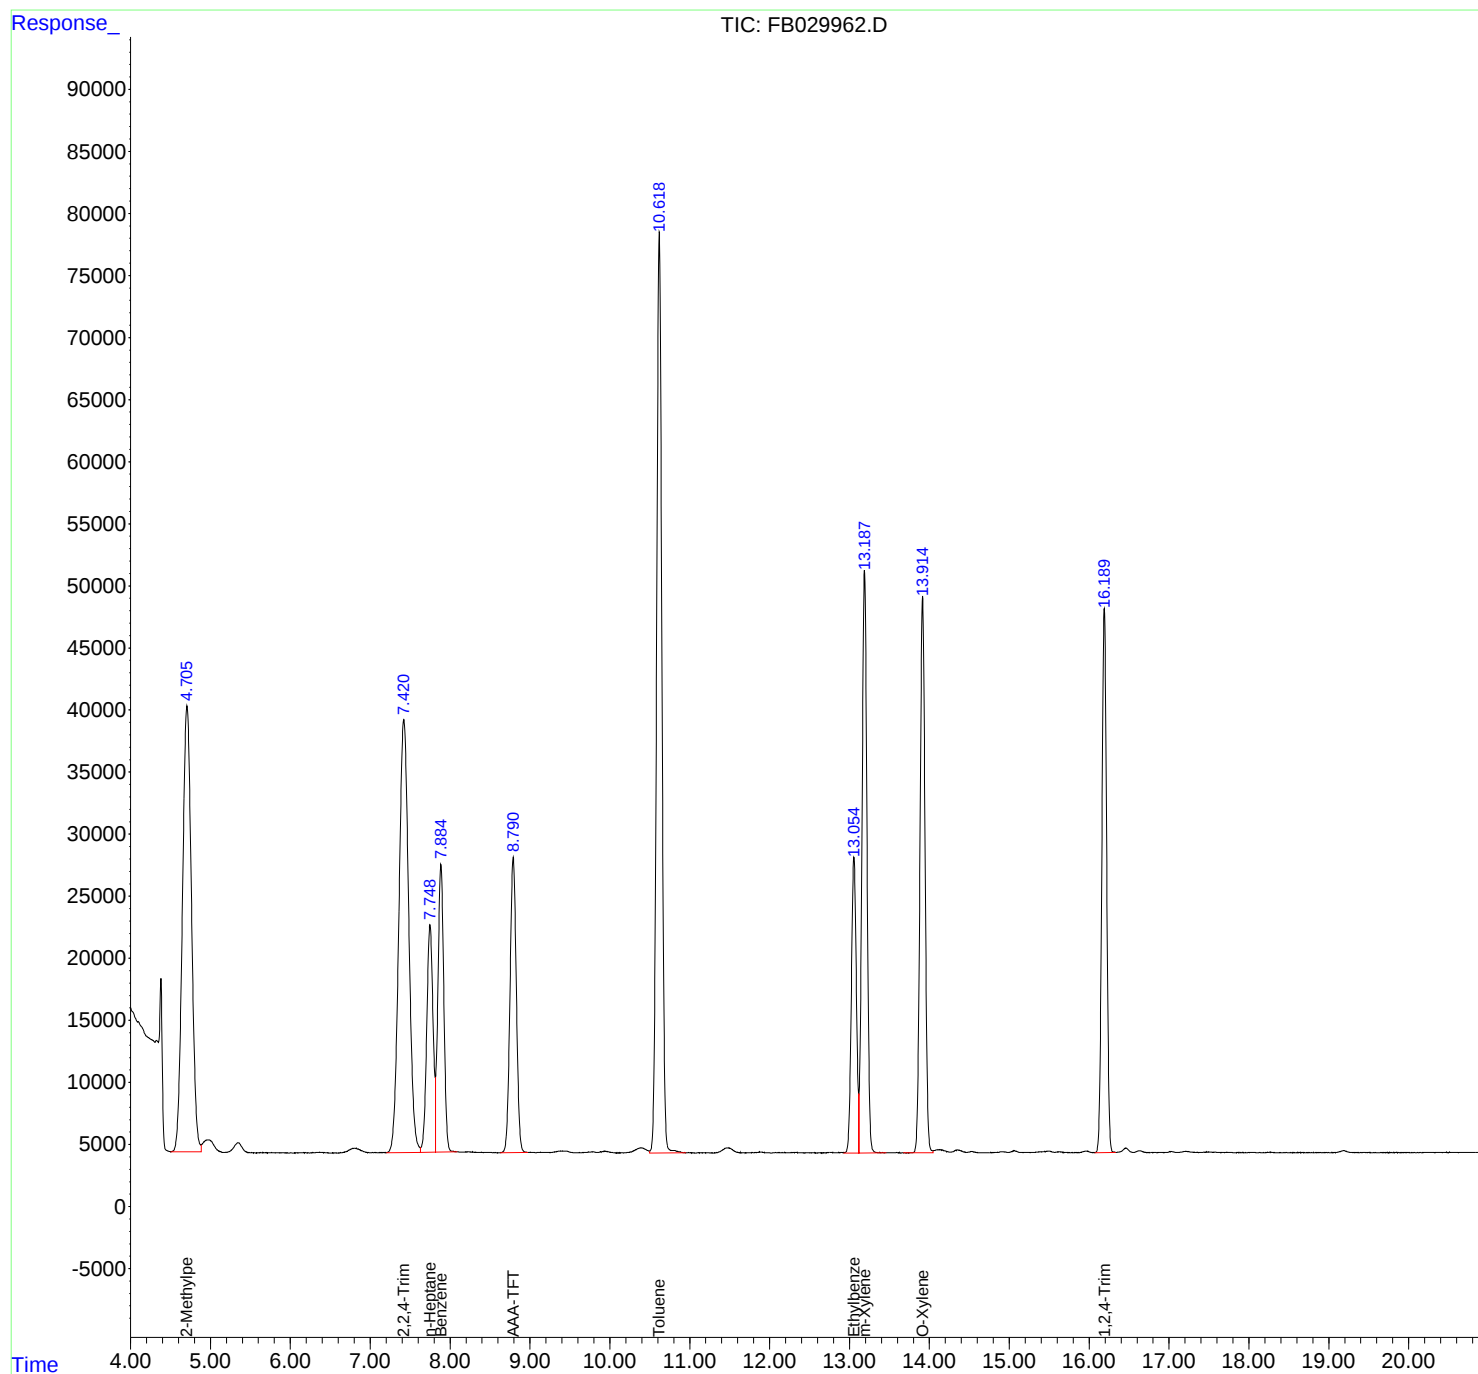


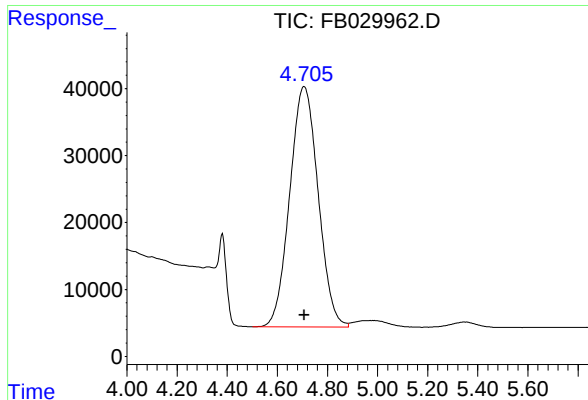

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: -0.001 min
Response: 2828682
Conc: 149.71 ng/ml

Instrument :
FID_B
ClientSampleId :

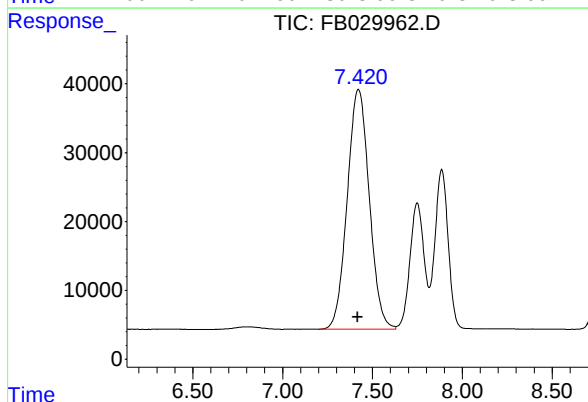


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: 0.003 min
Response: 2973822
Conc: 157.60 ng/ml

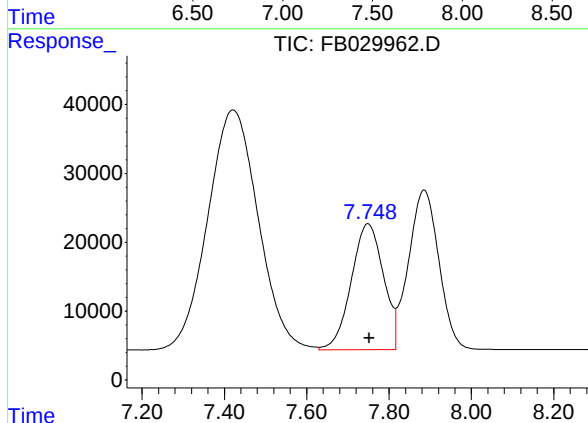


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.003 min
Response: 997082
Conc: 51.51 ng/ml

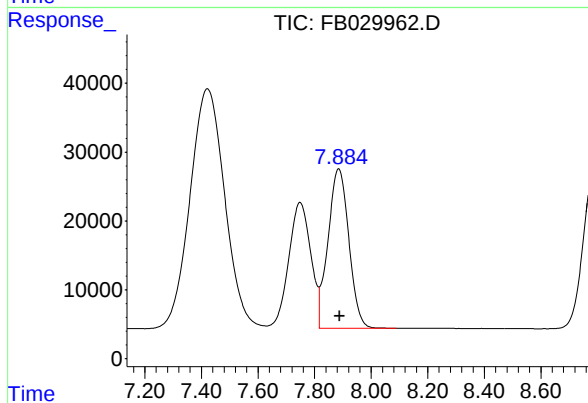

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.003 min
Response: 1189476
Conc: 53.14 ng/ml

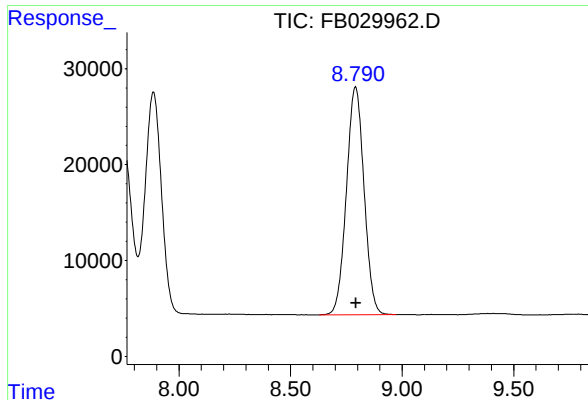

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: -0.001 min
Response: 1305779
Conc: 93.86 ng/ml

Instrument :
FID_B
ClientSampleId :

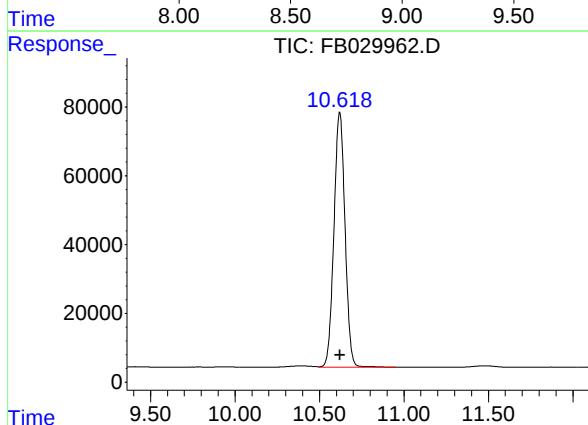


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.000 min
Response: 3390778
Conc: 156.23 ng/ml

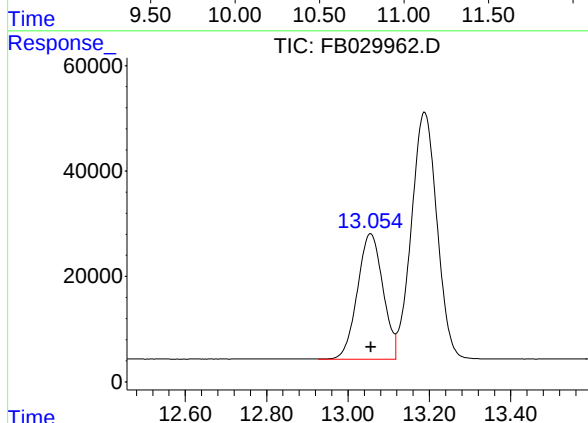


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 1034455
Conc: 51.16 ng/ml

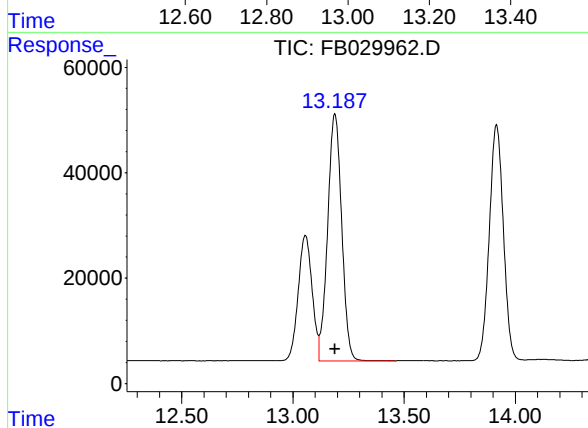

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 2050638
Conc: 101.97 ng/ml

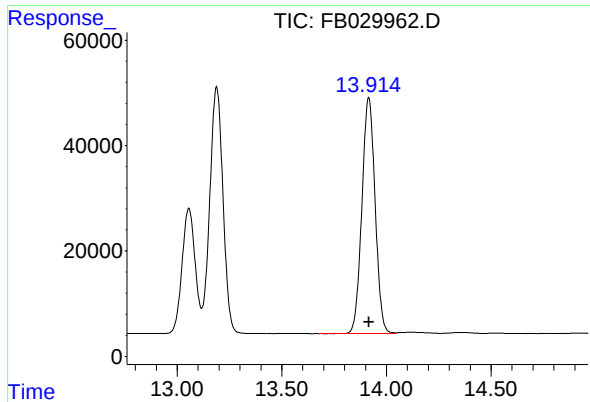

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: 0.000 min
Response: 1966938
Conc: 100.92 ng/ml

Instrument :
FID_B
ClientSampleId :

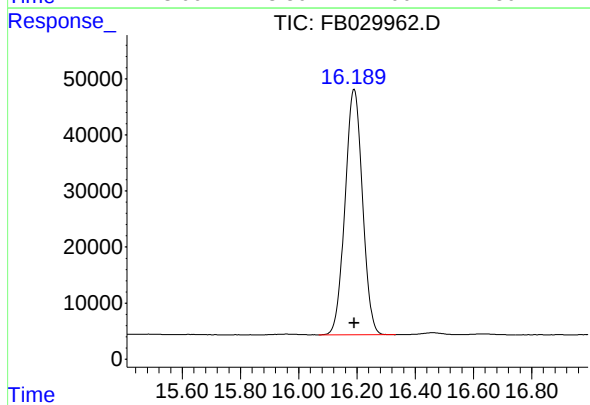

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: 0.000 min
Response: 1830935
Conc: 97.75 ng/ml