

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060323\
 Data File : FB029960.D
 Signal(s) : FID2B.CH
 Acq On : 3 Jun 2023 00:20
 Operator : YP/AJ
 Sample : 20 GRO STD
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 GRO STD

Integration File: Calibration.e
 Quant Time: Jun 05 04:27:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:26:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	300661	20.000 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	579930	30.000 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	577525	30.000 ng/ml
3) t n-Heptane	7.752	198620	10.000 ng/ml
4) t Benzene	7.889	224494	10.000 ng/ml
6) t Toluene	10.620	663921	30.000 ng/ml
7) t Ethylbenzene	13.057	209272	10.000 ng/ml
8) t m-Xylene	13.189	417192	20.000 ng/ml
9) t O-Xylene	13.916	399171	20.000 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	386843	20.000 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060323\
Data File : FB029960.D
Signal(s) : FID2B.CH
Acq On : 3 Jun 2023 00:20
Operator : YP/AJ
Sample : 20 GRO STD
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 GRO STD

Integration File: Calibration.e
Quant Time: Jun 05 04:27:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:26:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

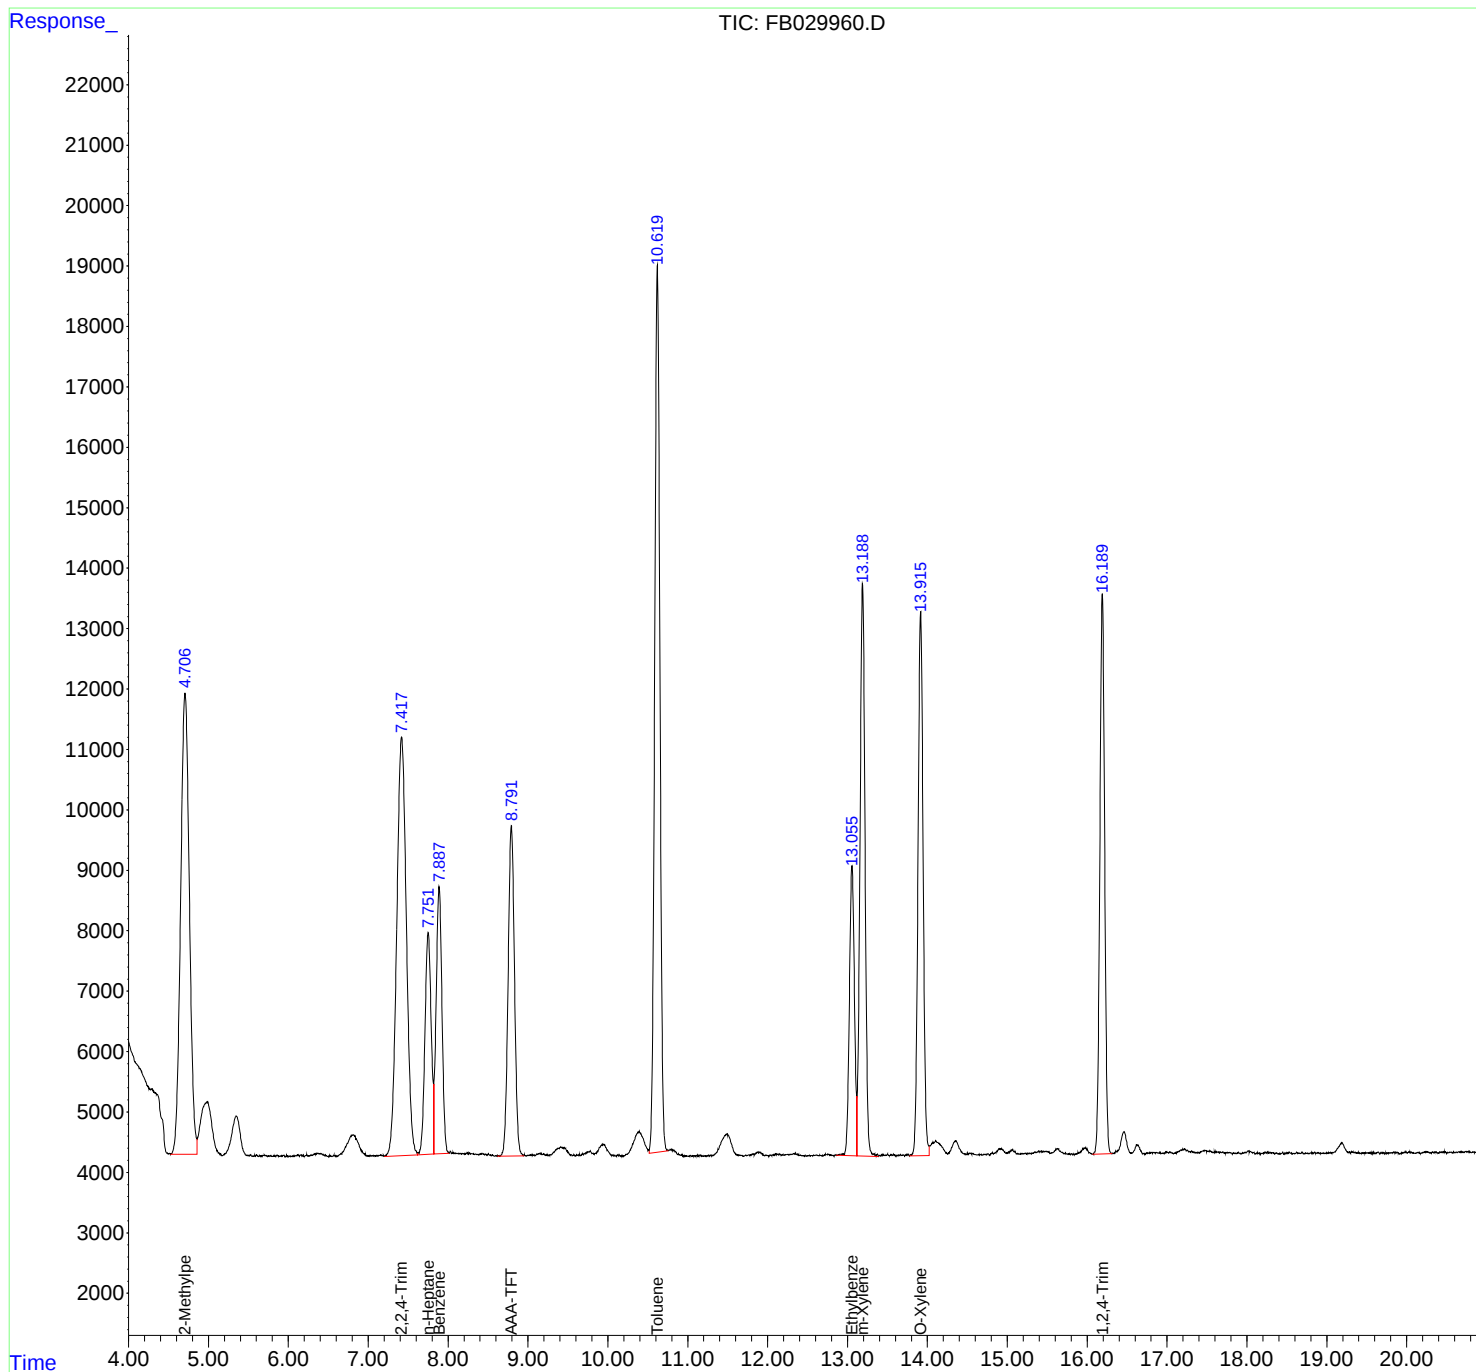


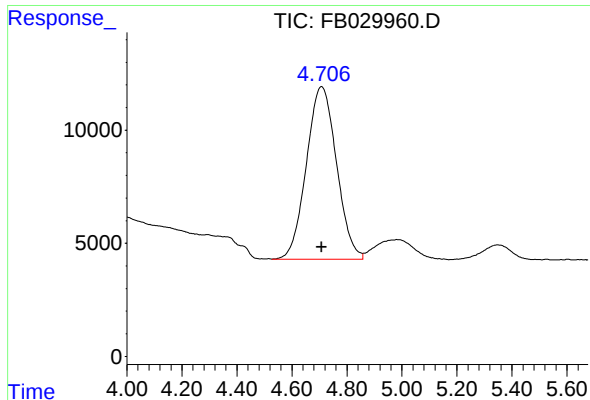

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 579930
Conc: 30.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

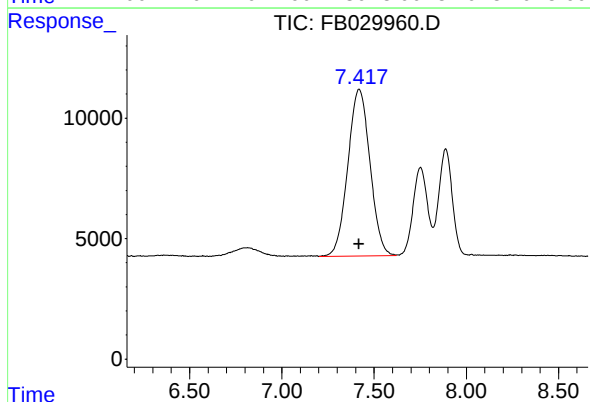


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 577525
Conc: 30.00 ng/ml

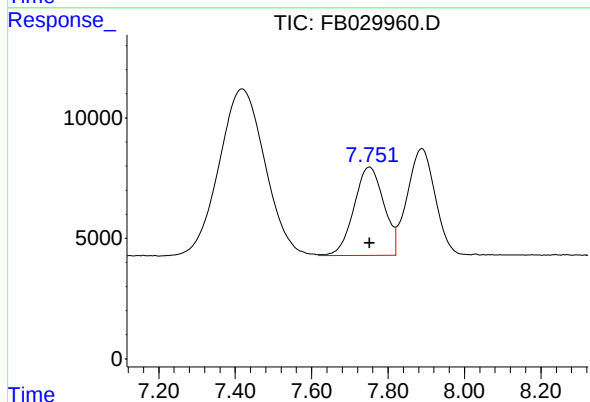


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 198620
Conc: 10.00 ng/ml

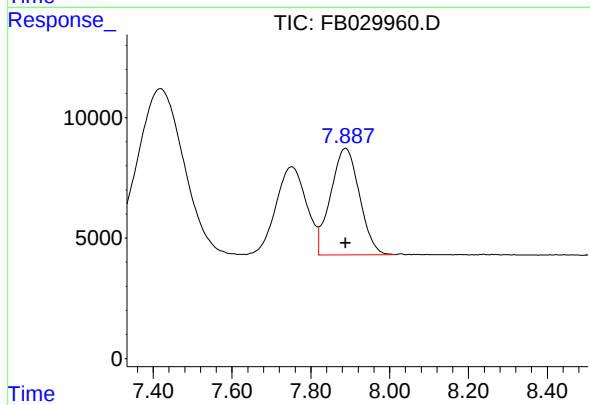

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.000 min
Response: 224494
Conc: 10.00 ng/ml

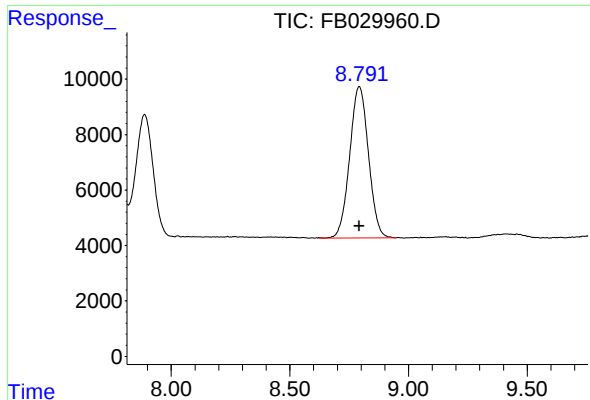

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 300661
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

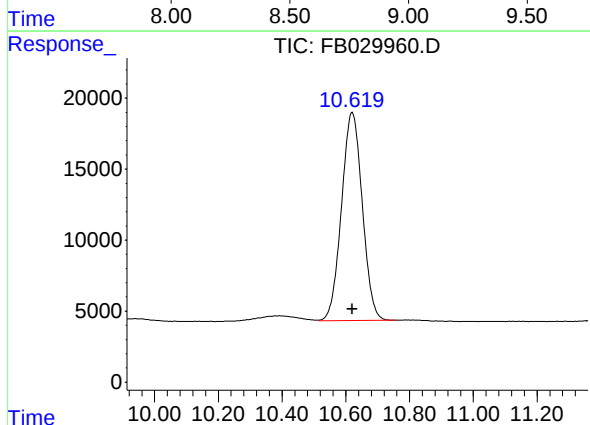


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.000 min
Response: 663921
Conc: 30.00 ng/ml

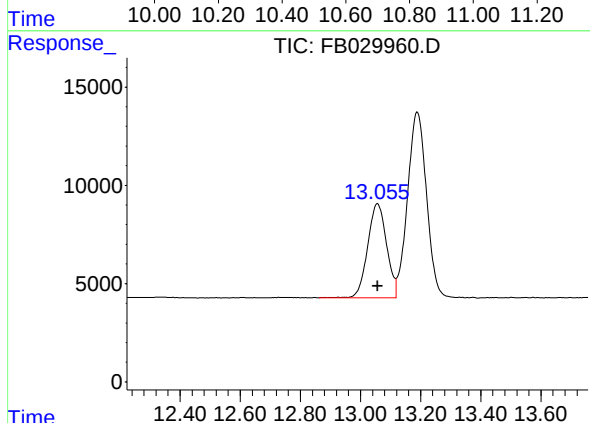


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.000 min
Response: 209272
Conc: 10.00 ng/ml

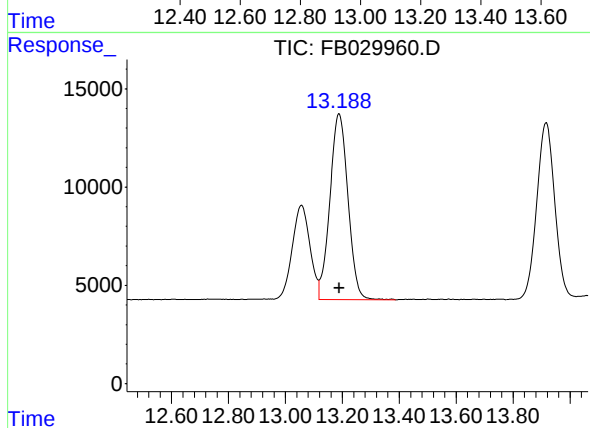

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 417192
Conc: 20.00 ng/ml

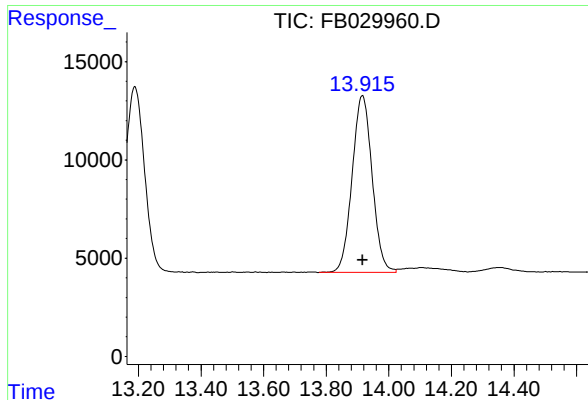

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 399171
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

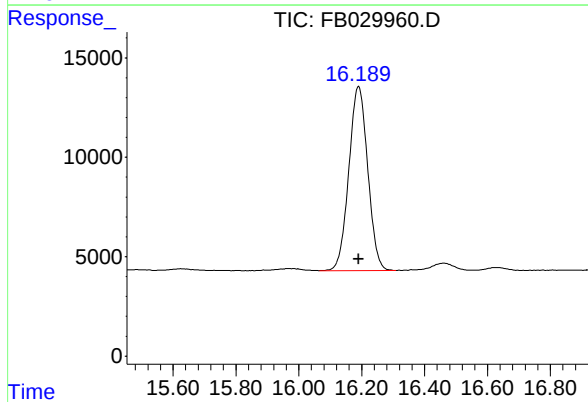

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 386843
Conc: 20.00 ng/ml