

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060323\
 Data File : FB029963.D
 Signal(s) : FID2B.CH
 Acq On : 3 Jun 2023 2:13
 Operator : YP/AJ
 Sample : FB060323GROICV
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 FB060323GROICV

Integration File: Calibration.e
 Quant Time: Jun 05 04:34:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:33:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	275923	19.833 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	518603	27.448 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	567647	30.083 ng/ml
3) t n-Heptane	7.752	165602	8.555 ng/ml
4) t Benzene	7.887	199984	8.934 ng/ml
6) t Toluene	10.621	578346	26.648 ng/ml
7) t Ethylbenzene	13.056	190066	9.400 ng/ml
8) t m-Xylene	13.188	383943	19.092 ng/ml
9) t O-Xylene	13.915	380839	19.540 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	397627	21.229 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060323\
Data File : FB029963.D
Signal(s) : FID2B.CH
Acq On : 3 Jun 2023 2:13
Operator : YP/AJ
Sample : FB060323GROICV
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
FB060323GROICV

Integration File: Calibration.e
Quant Time: Jun 05 04:34:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

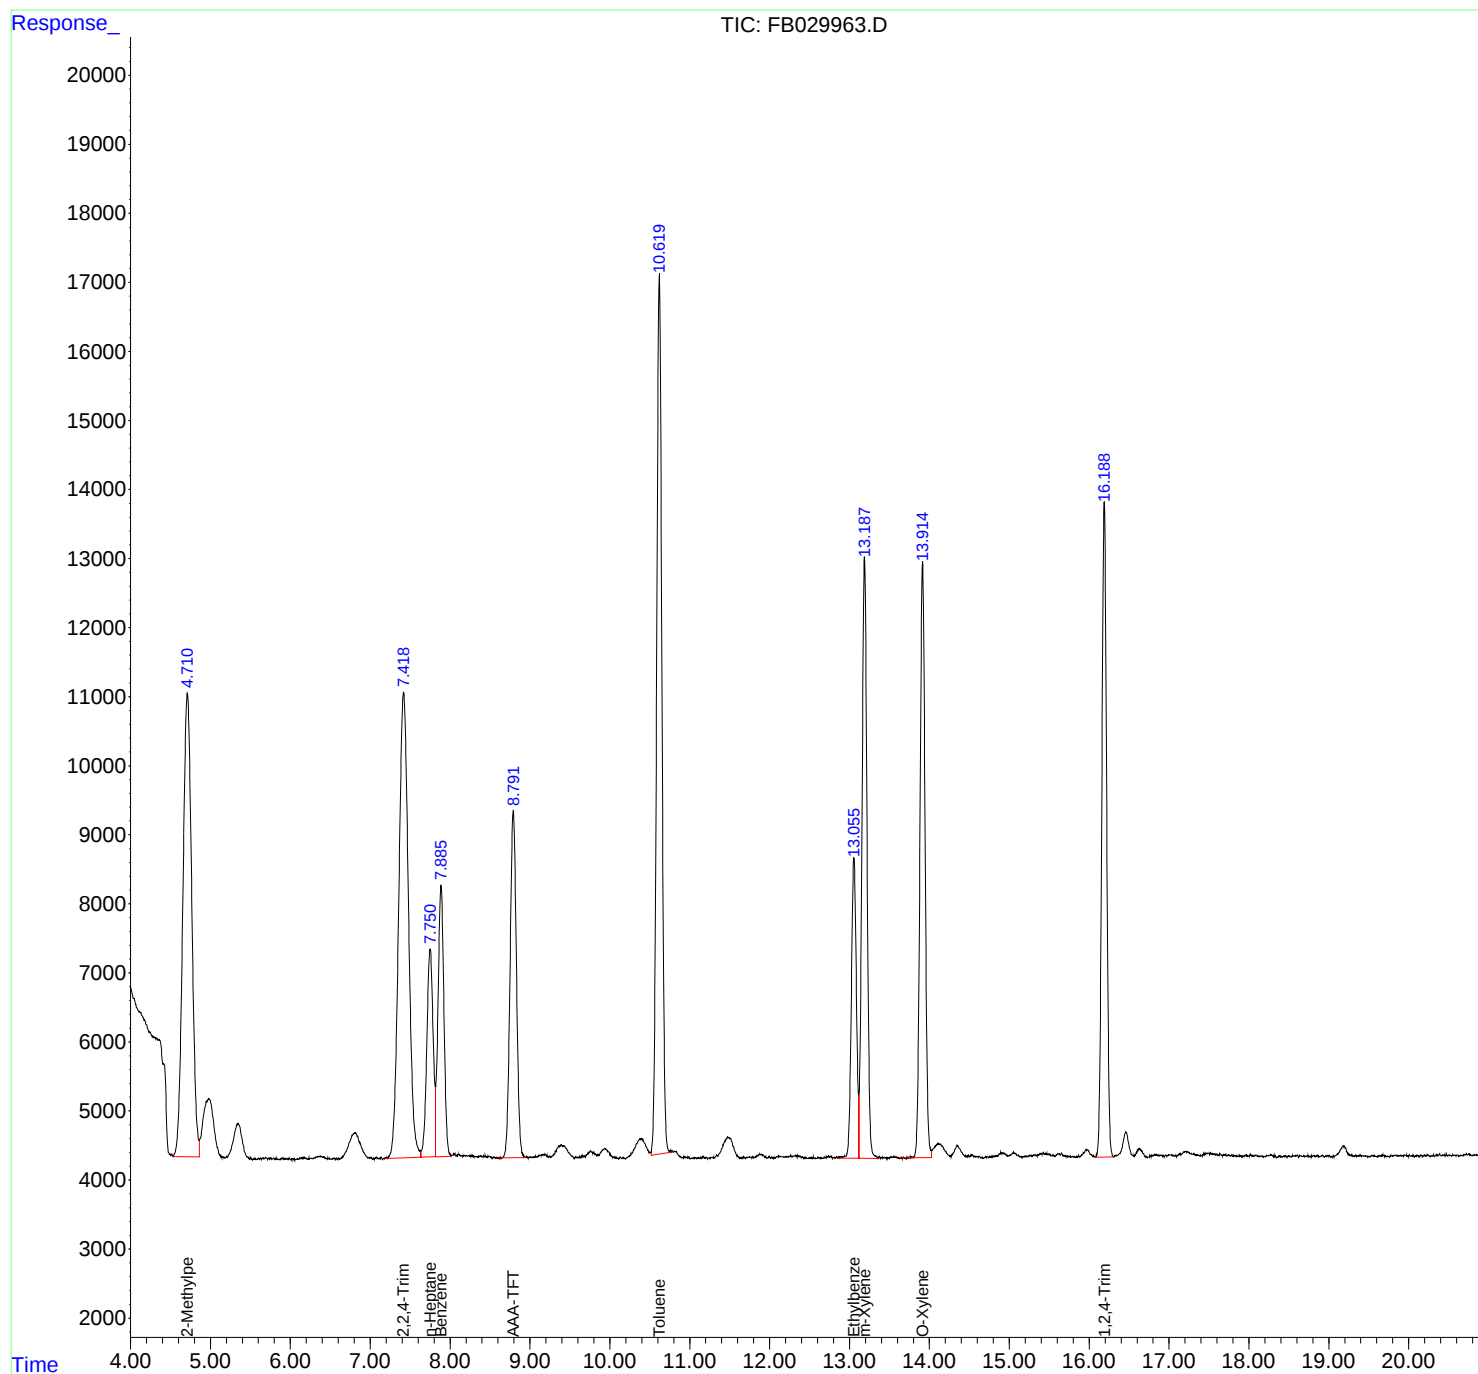


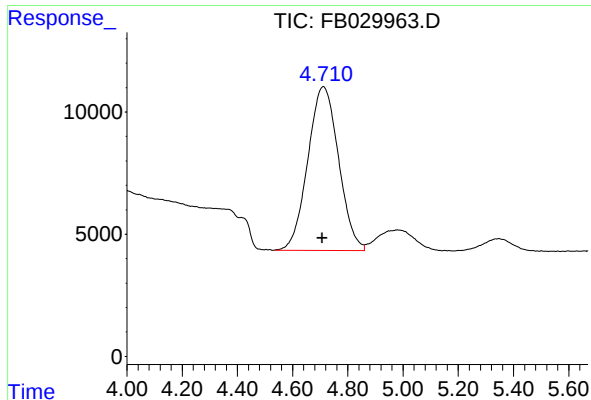

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.004 min
Response: 518603
Conc: 27.45 ng/ml

Instrument :
FID_B
ClientSampleId :
FB060323GROICV

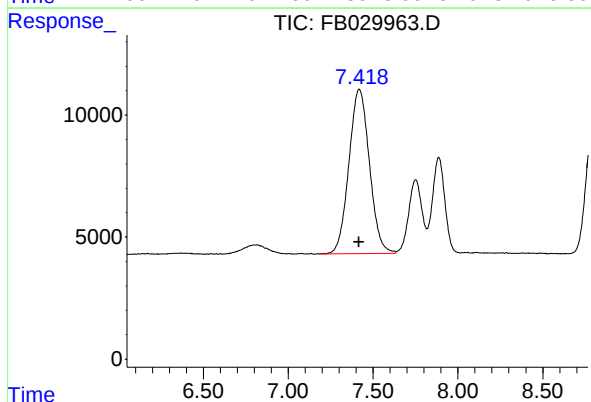


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 567647
Conc: 30.08 ng/ml

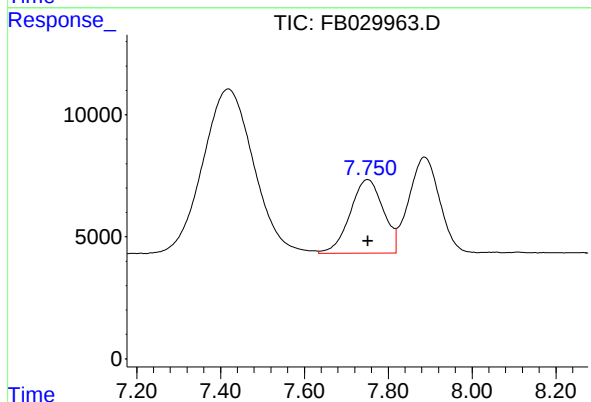


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 165602
Conc: 8.56 ng/ml

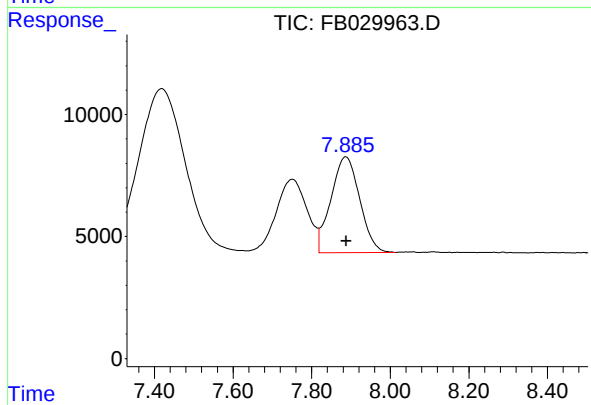

#4 Benzene


R.T.: 7.887 min
Delta R.T.: -0.002 min
Response: 199984
Conc: 8.93 ng/ml

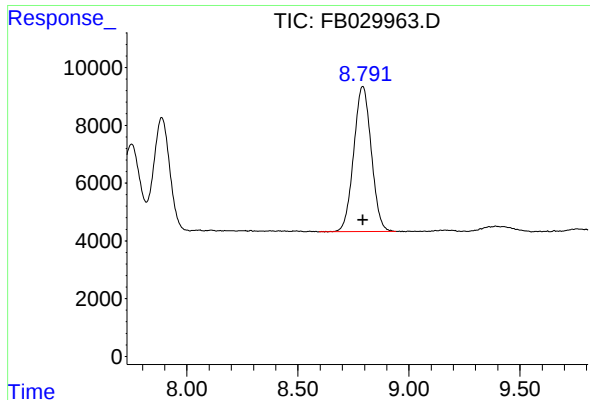

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 275923
Conc: 19.83 ng/ml

Instrument :
FID_B
ClientSampleId :
FB060323GROICV

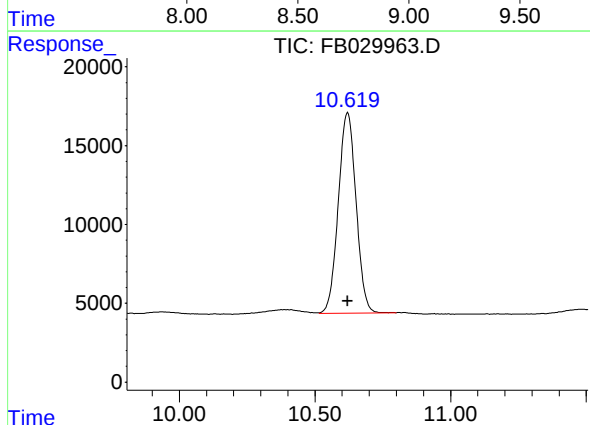


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 578346
Conc: 26.65 ng/ml

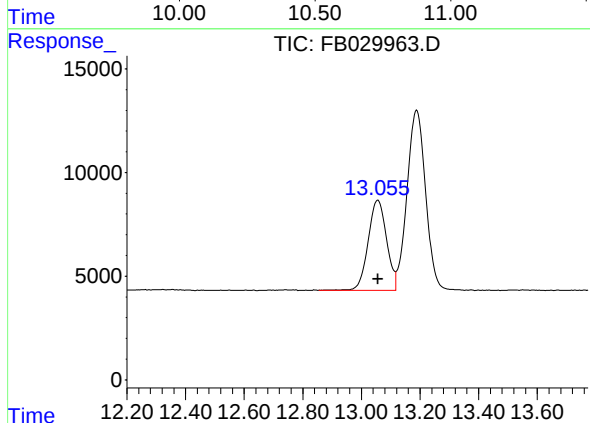


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 190066
Conc: 9.40 ng/ml

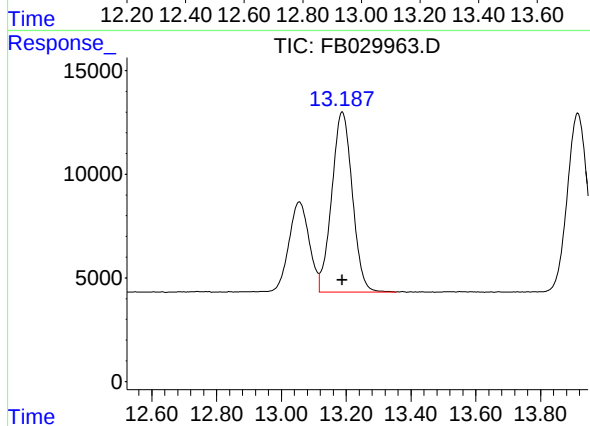

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: 0.000 min
Response: 383943
Conc: 19.09 ng/ml

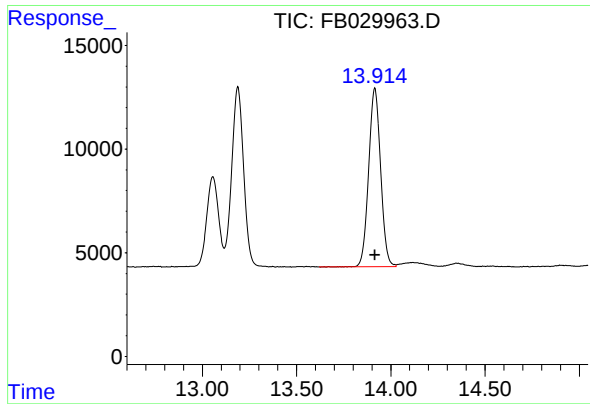

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: 0.000 min
Response: 380839
Conc: 19.54 ng/ml

Instrument :
FID_B
ClientSampleId :
FB060323GROICV

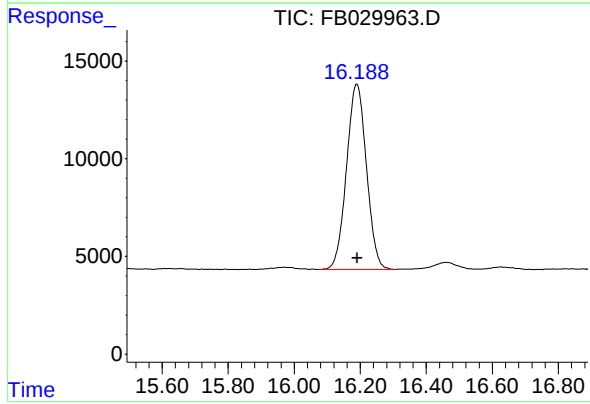

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: 0.000 min
Response: 397627
Conc: 21.23 ng/ml