

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060324\
 Data File : FB030773.D
 Signal(s) : FID2B.CH
 Acq On : 3 Jun 2024 11:54
 Operator : YP/AJ
 Sample : BSF0603S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0603S1

Integration File: Calibration.e
 Quant Time: Jun 04 06:32:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050824.M
 Quant Title :
 QLast Update : Wed May 08 14:36:01 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	253013	18.335 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	542400	30.959 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	556895	30.991 ng/ml
3) t n-Heptane	7.747	197200	9.890 ng/ml
4) t Benzene	7.884	231601	10.226 ng/ml
6) t Toluene	10.616	676714	30.401 ng/ml
7) t Ethylbenzene	13.053	210674	10.209 ng/ml
8) t m-Xylene	13.185	419068	20.118 ng/ml
9) t O-Xylene	13.912	407268	21.335 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	399466	21.121 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060324\
Data File : FB030773.D
Signal(s) : FID2B.CH
Acq On : 3 Jun 2024 11:54
Operator : YP/AJ
Sample : BSF0603S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0603S1

Integration File: Calibration.e
Quant Time: Jun 04 06:32:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050824.M
Quant Title :
QLast Update : Wed May 08 14:36:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

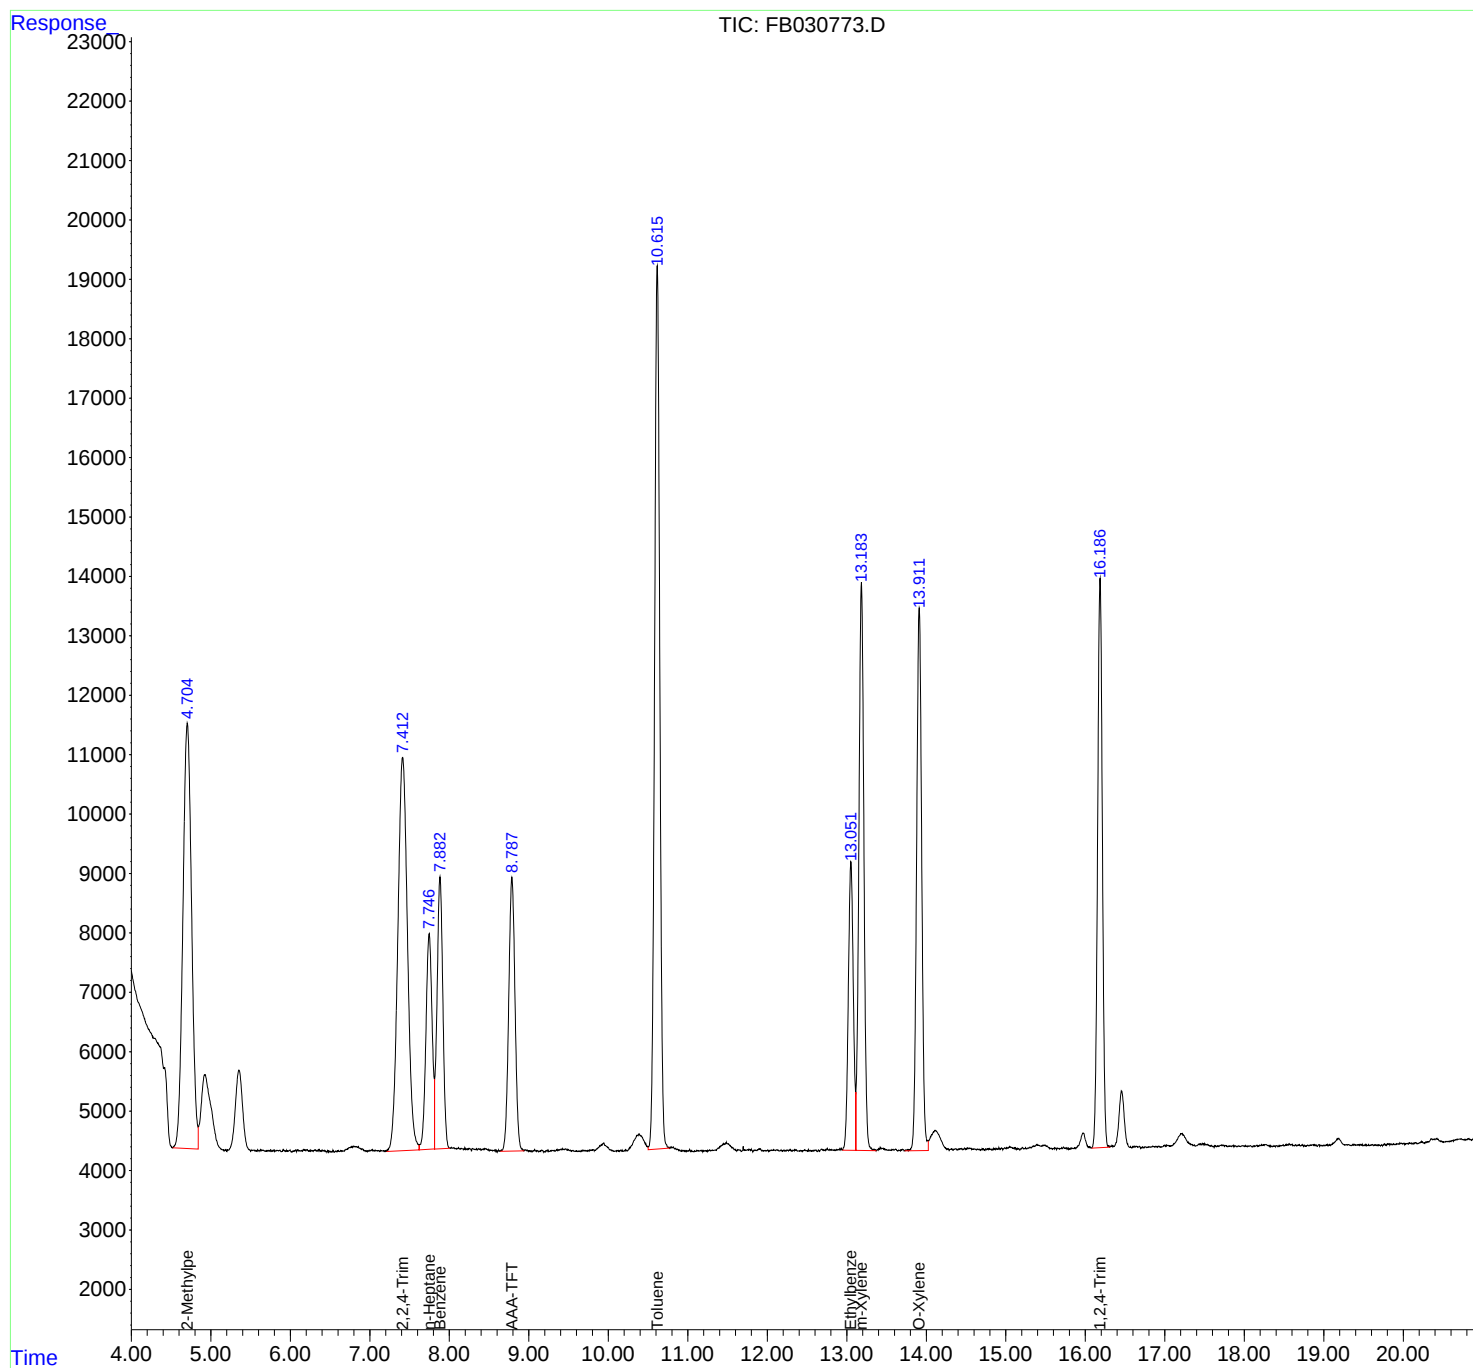


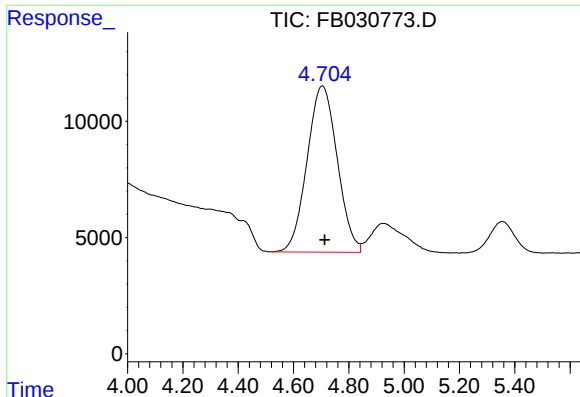

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.008 min
Response: 542400
Conc: 30.96 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0603S1

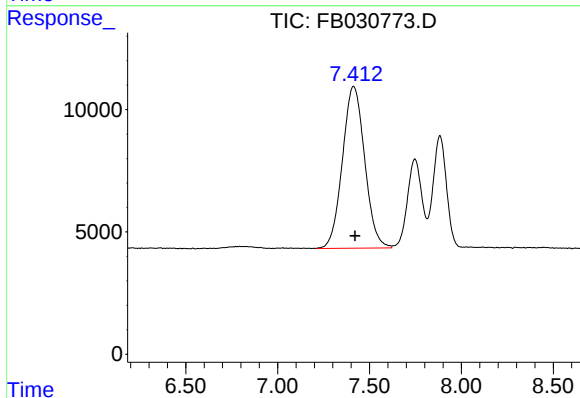


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.008 min
Response: 556895
Conc: 30.99 ng/ml

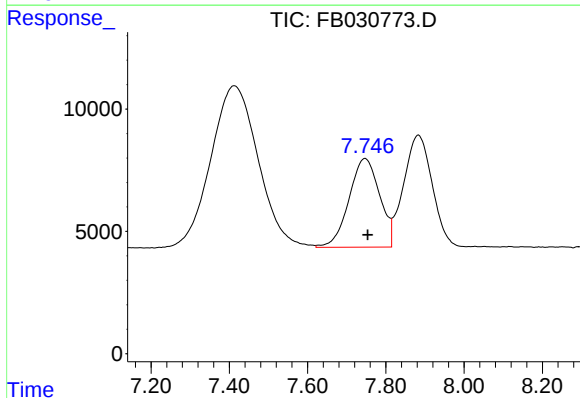


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.006 min
Response: 197200
Conc: 9.89 ng/ml

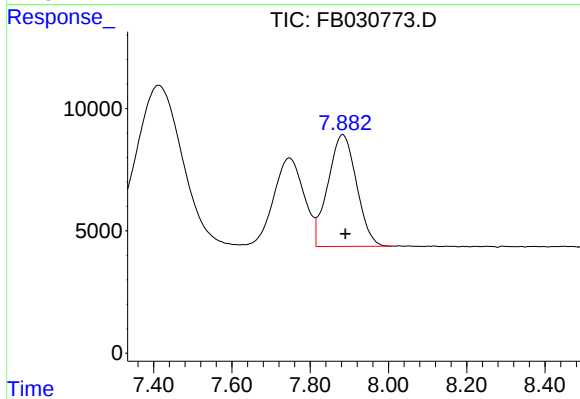

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.006 min
Response: 231601
Conc: 10.23 ng/ml

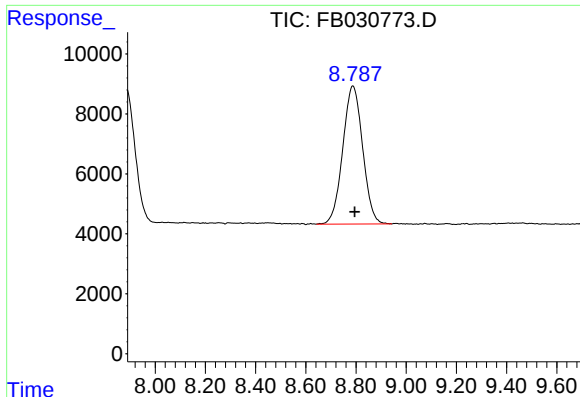

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: -0.007 min
Response: 253013
Conc: 18.33 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0603S1

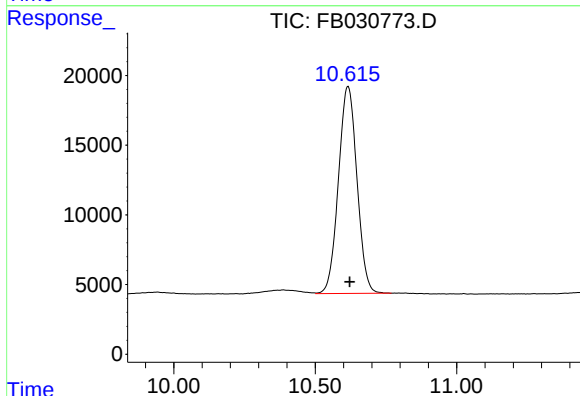


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.006 min
Response: 676714
Conc: 30.40 ng/ml

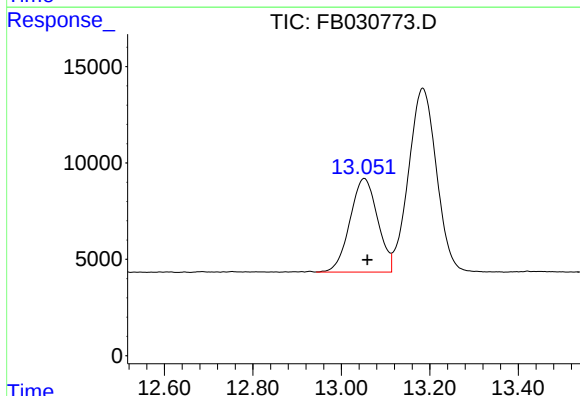


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.006 min
Response: 210674
Conc: 10.21 ng/ml

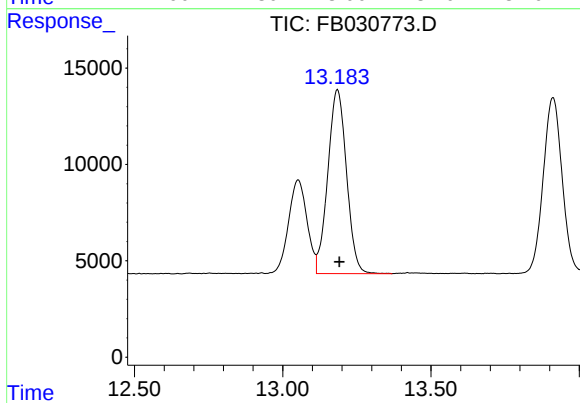

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.007 min
Response: 419068
Conc: 20.12 ng/ml

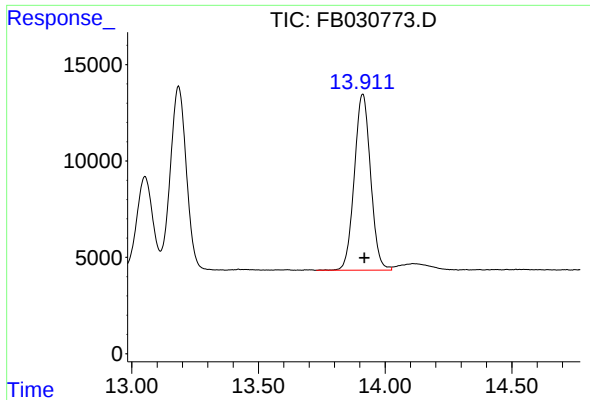

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.007 min
Response: 407268
Conc: 21.33 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0603S1

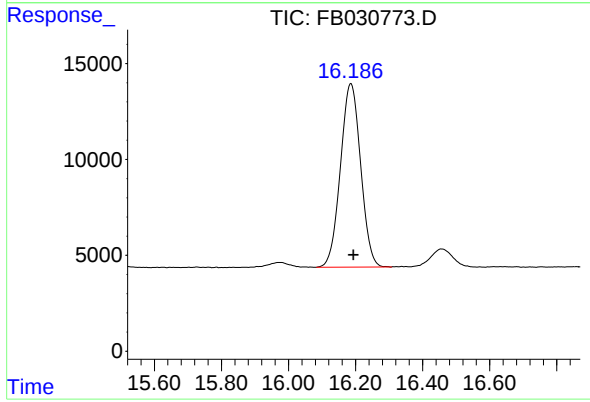

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: -0.007 min
Response: 399466
Conc: 21.12 ng/ml