

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060324\
 Data File : FB030778.D
 Signal(s) : FID2B.CH
 Acq On : 3 Jun 2024 15:14
 Operator : YP/AJ
 Sample : BSF0603S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0603S2

Integration File: Calibration.e
 Quant Time: Jun 04 06:33:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050824.M
 Quant Title :
 QLast Update : Wed May 08 14:36:01 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	248341	17.996 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	531468	30.335 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	549083	30.556 ng/ml
3) t n-Heptane	7.749	194148	9.737 ng/ml
4) t Benzene	7.886	233144	10.294 ng/ml
6) t Toluene	10.619	673246	30.246 ng/ml
7) t Ethylbenzene	13.055	207650	10.062 ng/ml
8) t m-Xylene	13.188	413625	19.857 ng/ml
9) t O-Xylene	13.914	399963	20.952 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	379820	20.082 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060324\
Data File : FB030778.D
Signal(s) : FID2B.CH
Acq On : 3 Jun 2024 15:14
Operator : YP/AJ
Sample : BSF0603S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0603S2

Integration File: Calibration.e
Quant Time: Jun 04 06:33:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050824.M
Quant Title :
QLast Update : Wed May 08 14:36:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

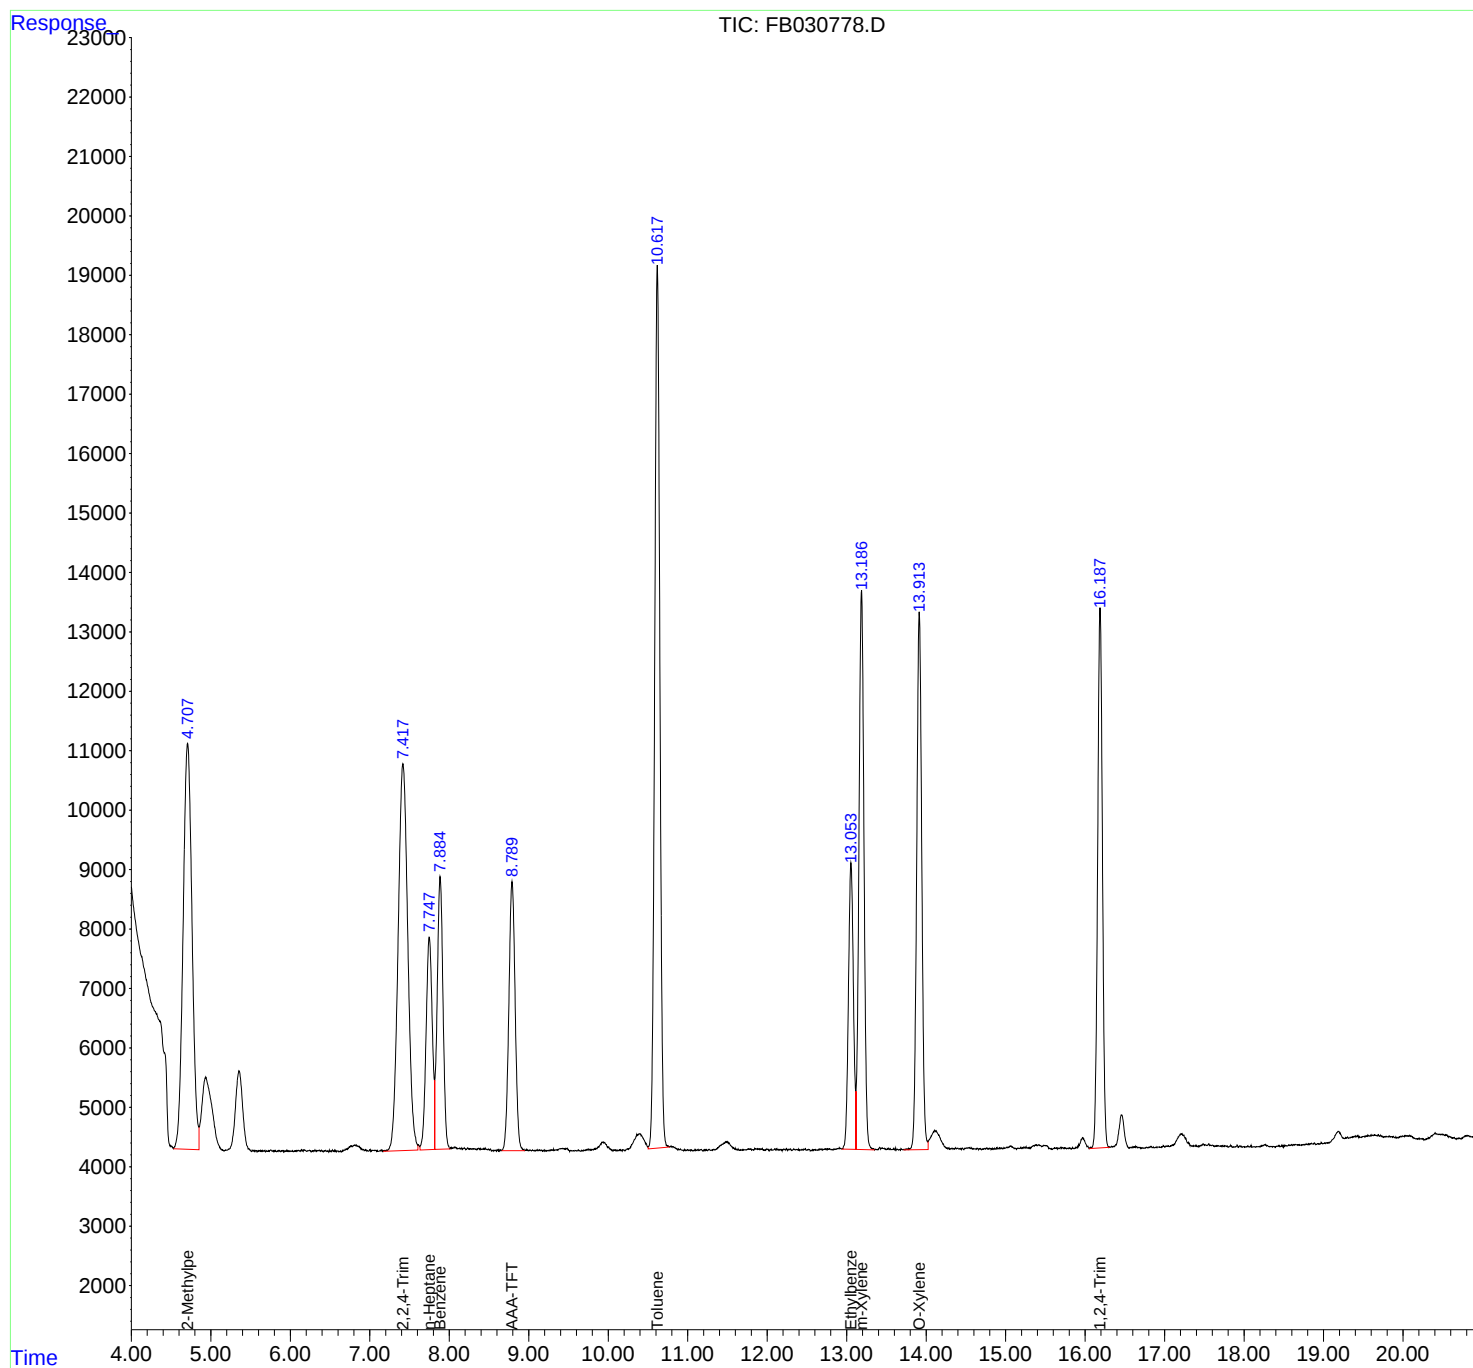


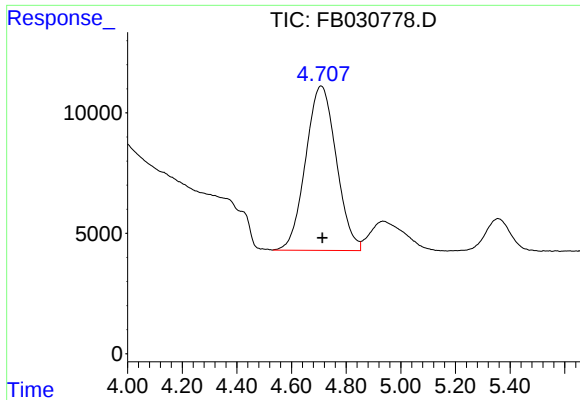

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: -0.004 min
Response: 531468
Conc: 30.34 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0603S2

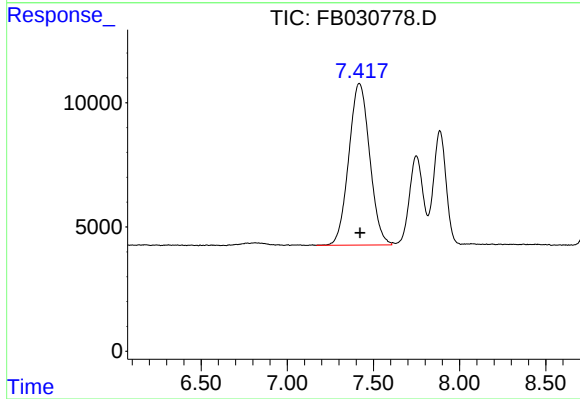


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.003 min
Response: 549083
Conc: 30.56 ng/ml

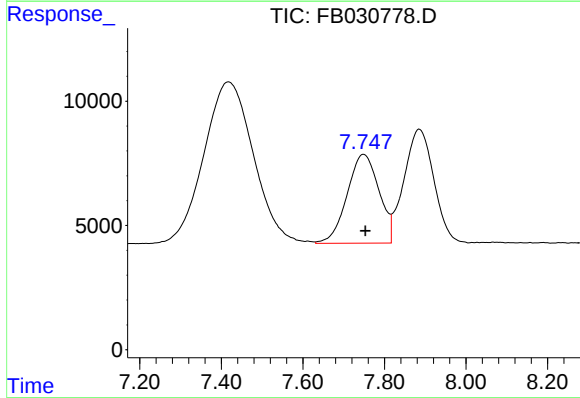


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.005 min
Response: 194148
Conc: 9.74 ng/ml

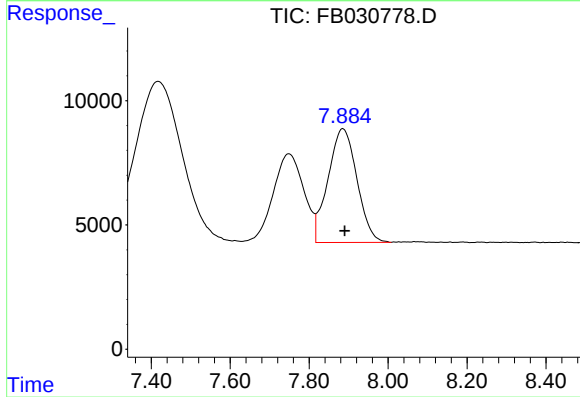

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.005 min
Response: 233144
Conc: 10.29 ng/ml

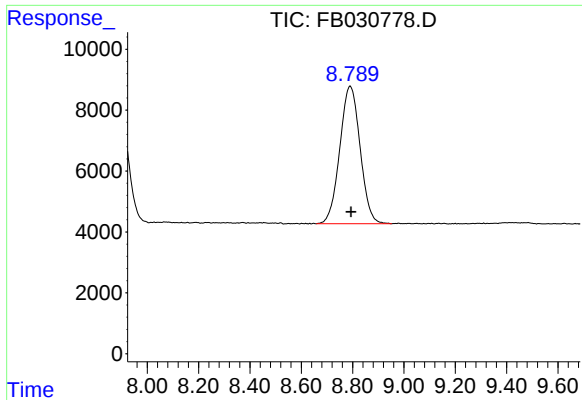

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: -0.004 min
Response: 248341
Conc: 18.00 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0603S2

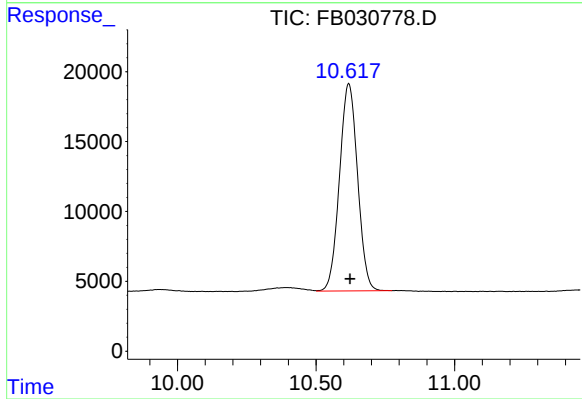


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.004 min
Response: 673246
Conc: 30.25 ng/ml

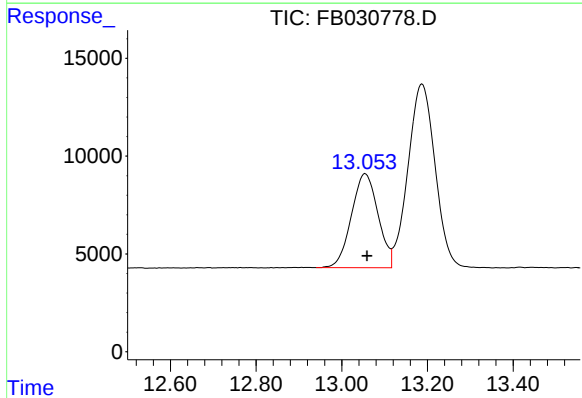


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.004 min
Response: 207650
Conc: 10.06 ng/ml

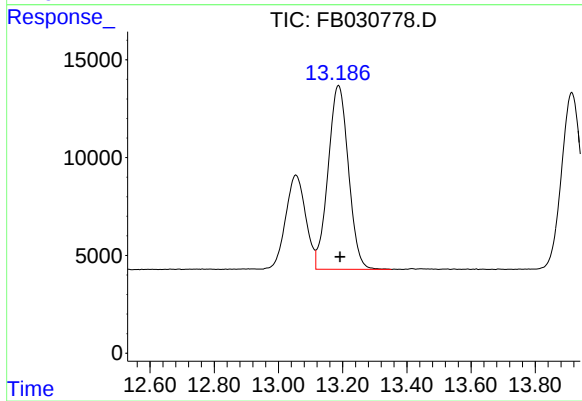

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.004 min
Response: 413625
Conc: 19.86 ng/ml

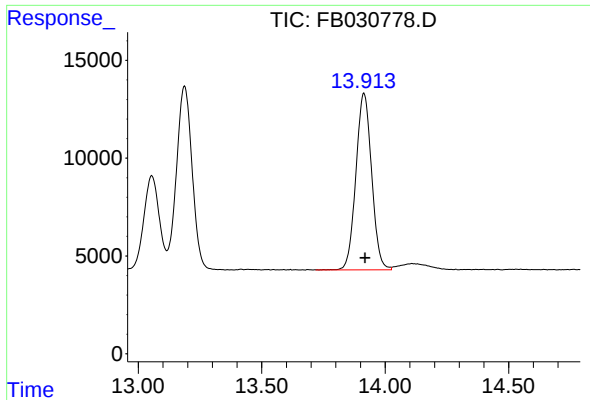

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.004 min
Response: 399963
Conc: 20.95 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0603S2

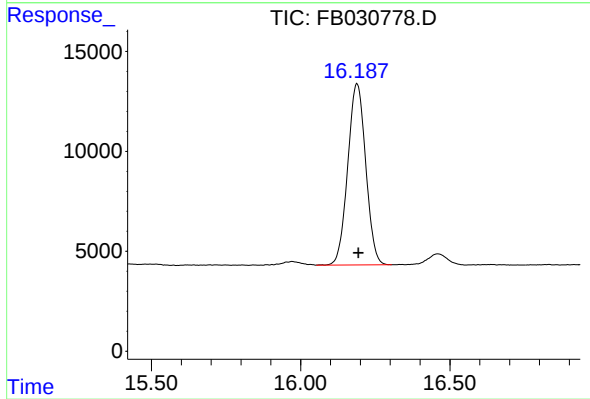

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.004 min
Response: 379820
Conc: 20.08 ng/ml