

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060325\
Data File : FB031870.D
Signal(s) : FID2B.CH
Acq On : 3 Jun 2025 17:15
Operator : YP/AJ
Sample : Q2176-04
Misc : 4.69G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-26

Integration File: Calibration.e
Quant Time: Jun 04 01:22:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB053025.M
Quant Title :
QLast Update : Fri May 30 15:30:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	228438	18.721 ng/ml
Target Compounds			
6) t Toluene	10.626	4995	0.266 ng/ml
7) t Ethylbenzene	13.055	5705	0.374 ng/ml
8) t m-Xylene	13.190	7656	0.448 ng/ml
9) t O-Xylene	13.937	2808	0.177 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	10292	0.892 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060325\
Data File : FB031870.D
Signal(s) : FID2B.CH
Acq On : 3 Jun 2025 17:15
Operator : YP/AJ
Sample : Q2176-04
Misc : 4.69G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-26

Integration File: Calibration.e
Quant Time: Jun 04 01:22:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB053025.M
Quant Title :
QLast Update : Fri May 30 15:30:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

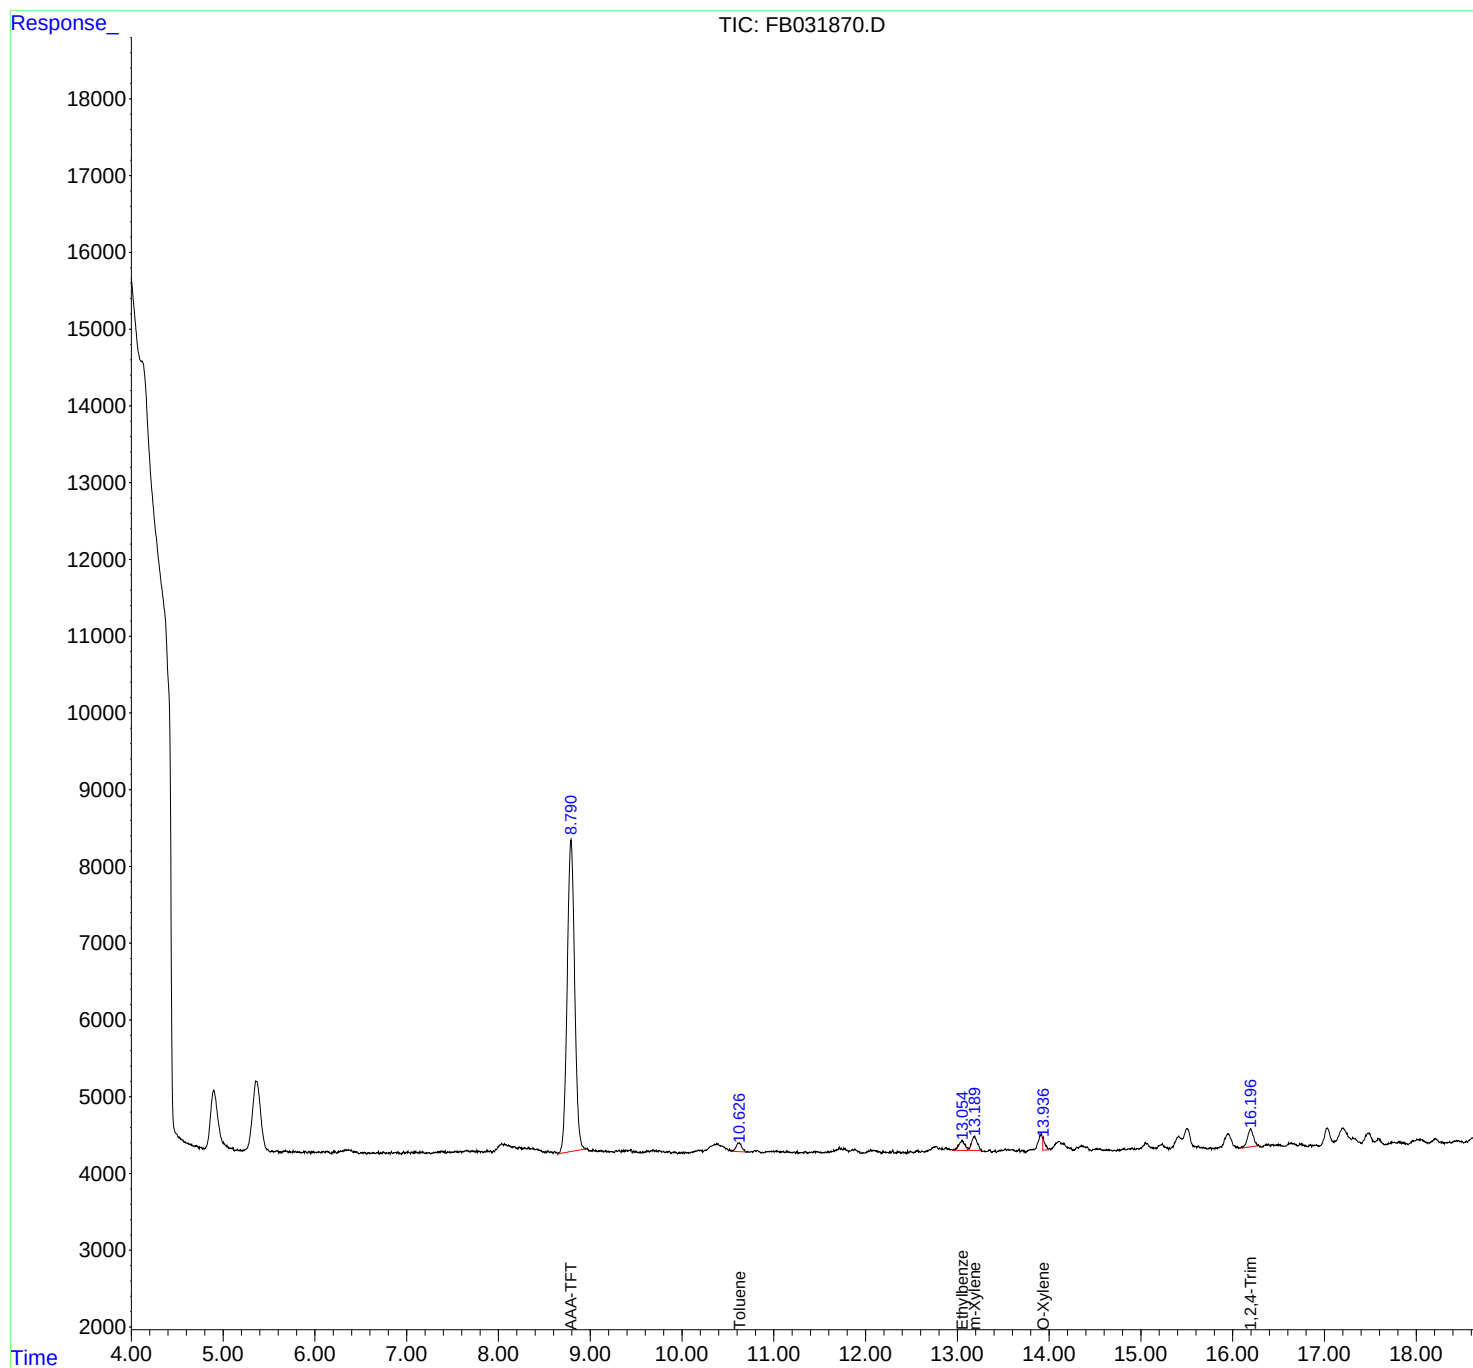


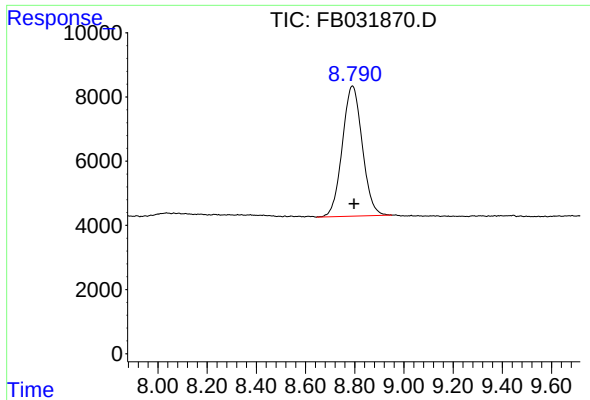

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: -0.006 min
Response: 228438
Conc: 18.72 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-26

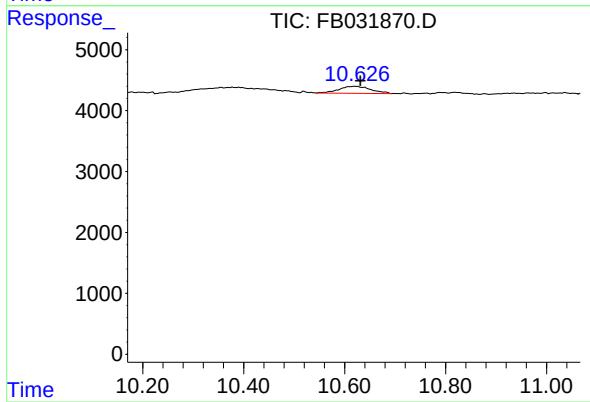


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.005 min
Response: 4995
Conc: 0.27 ng/ml

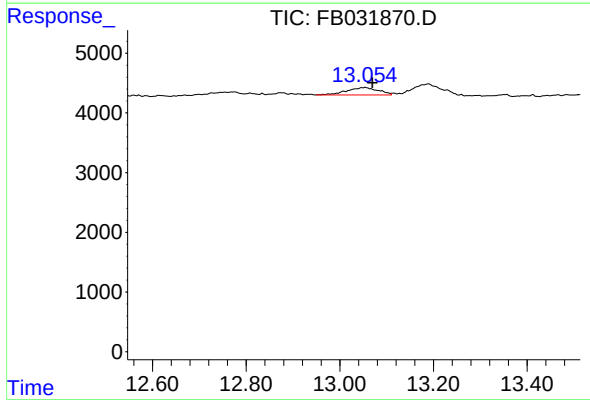


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.015 min
Response: 5705
Conc: 0.37 ng/ml

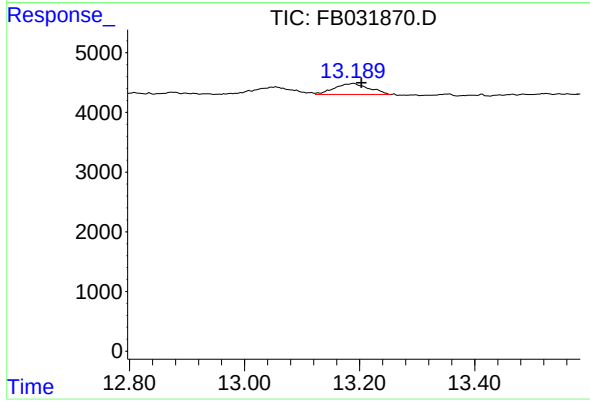

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: -0.013 min
Response: 7656
Conc: 0.45 ng/ml

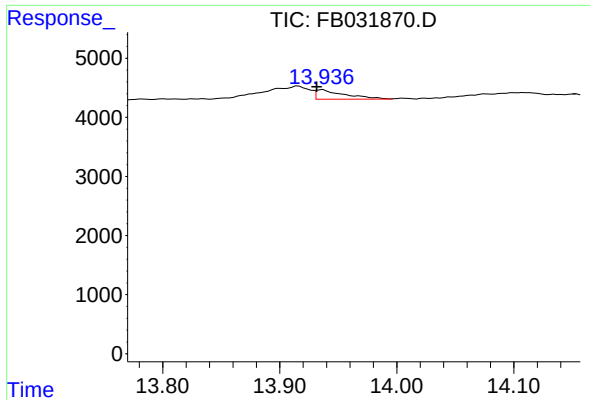

#9 O-Xylene

R.T.: 13.937 min
Delta R.T.: 0.005 min
Response: 2808
Conc: 0.18 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-26

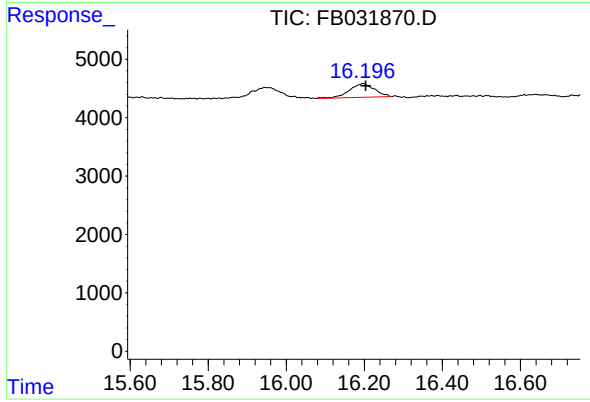

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: -0.007 min
Response: 10292
Conc: 0.89 ng/ml