

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060420\
 Data File : FB024421.D
 Signal(s) : FID2B.CH
 Acq On : 4 Jun 2020 9:29
 Operator : DD/AJ
 Sample : BSF0604S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 05 00:39:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.800	473032	21.422 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.692	956795	32.423 ng/ml
2) t	2,2,4-Trimethylpentane	7.418	1043789	34.167 ng/ml
3) t	n-Heptane	7.759	339328	11.201 ng/ml
4) t	Benzene	7.894	409229	10.825 ng/ml
6) t	Toluene	10.631	1184684	32.693 ng/ml
7) t	Ethylbenzene	13.071	359426	10.602 ng/ml
8) t	m-Xylene	13.204	696709	21.113 ng/ml
9) t	O-Xylene	13.931	680719	21.094 ng/ml
10) t	1,2,4-Trimethylbenzene	16.209	568355	21.074 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060420\
Data File : FB024421.D
Signal(s) : FID2B.CH
Acq On : 4 Jun 2020 9:29
Operator : DD/AJ
Sample : BSF0604S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 05 00:39:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

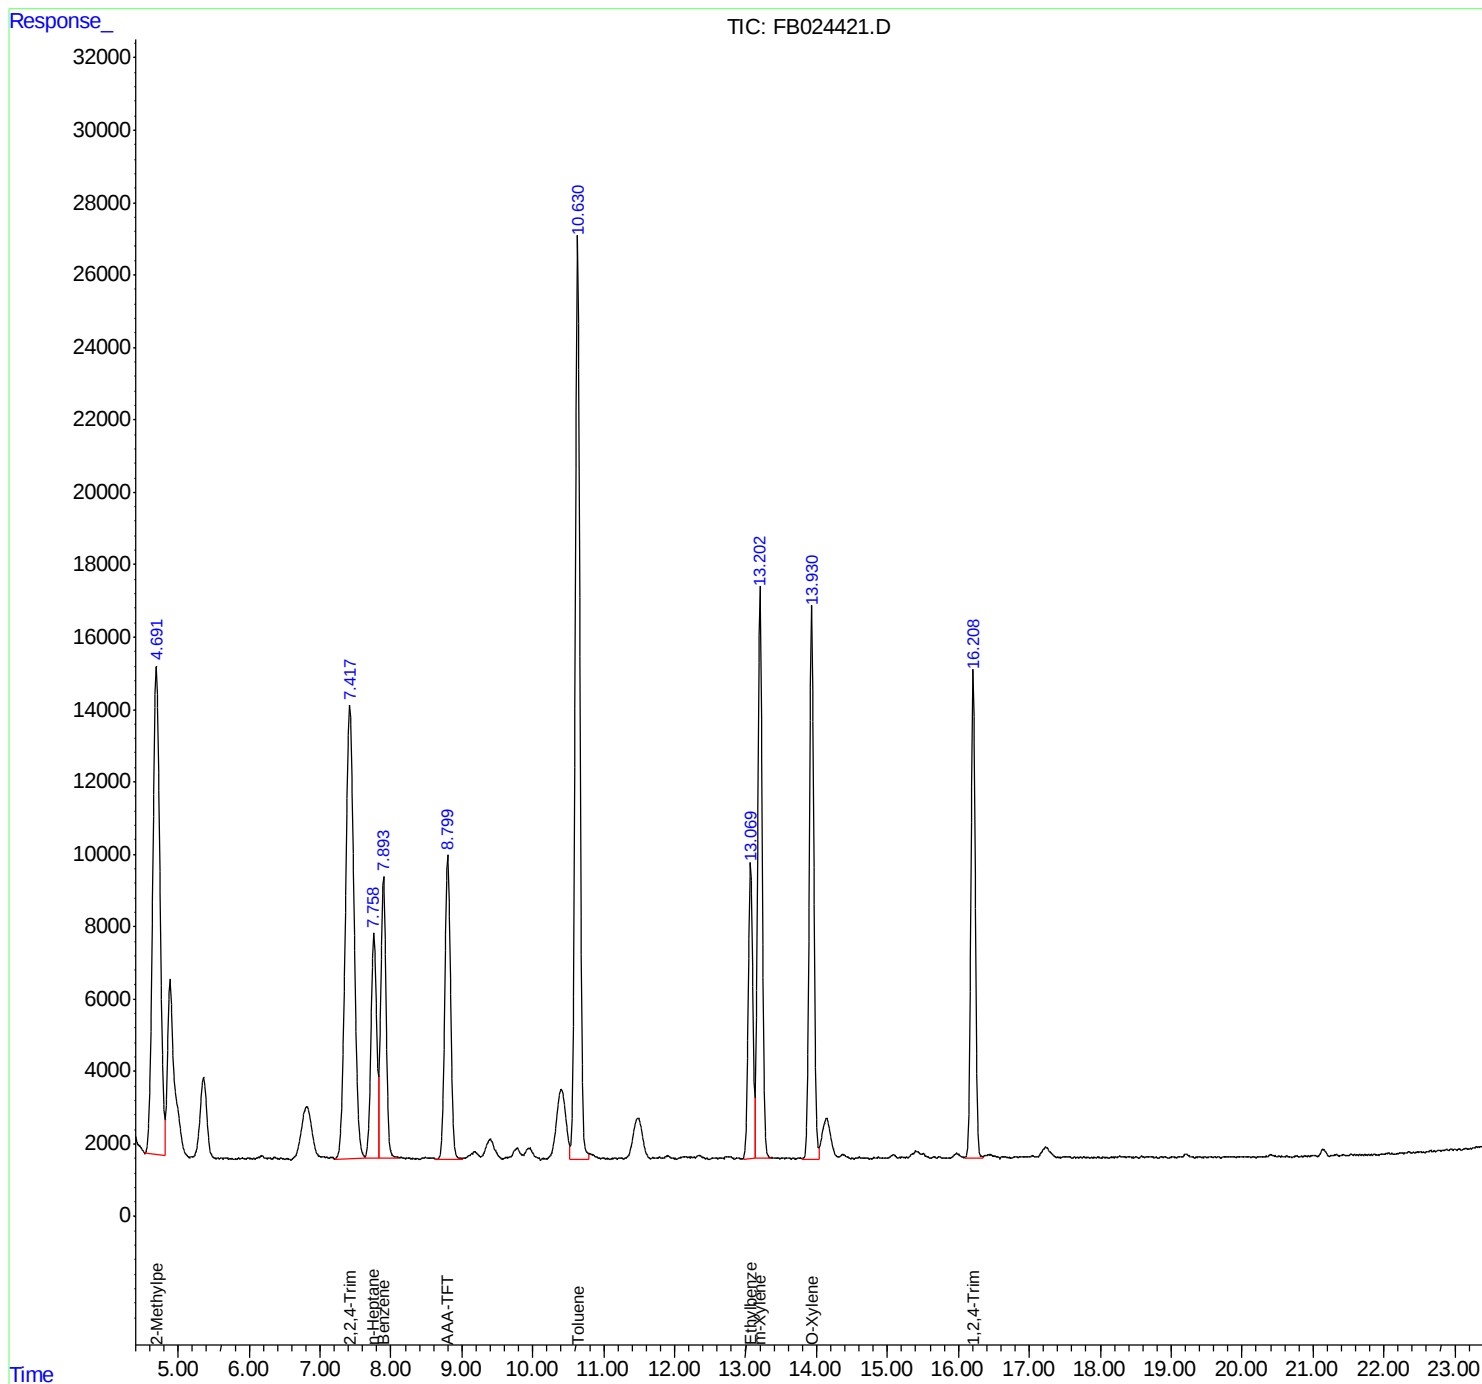

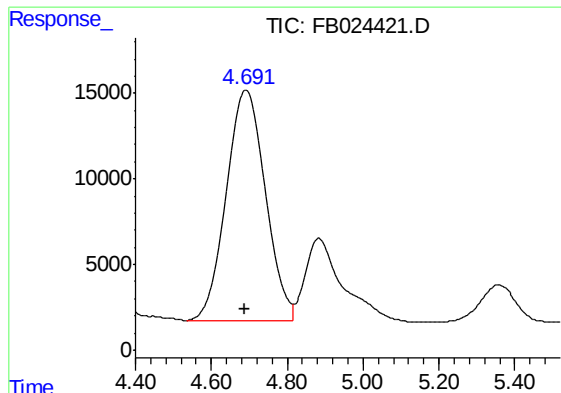


#1 2-Methylpentane

R.T.: 4.692 min
Delta R.T.: 0.003 min
Response: 956795
Conc: 32.42 ng/ml

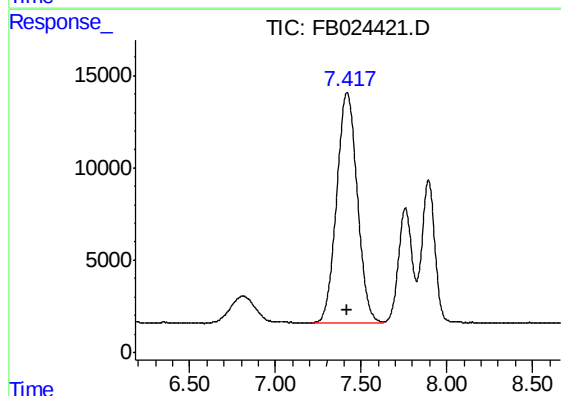


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.001 min
Response: 1043789
Conc: 34.17 ng/ml

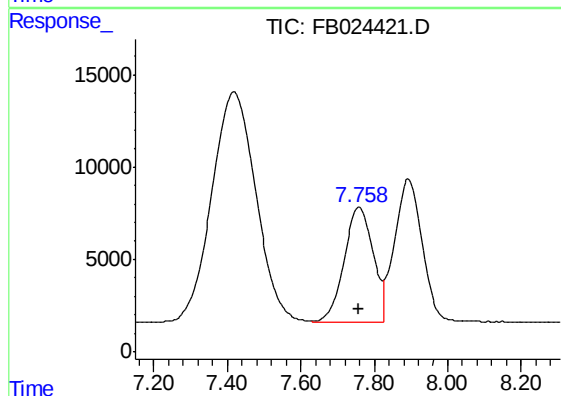


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.001 min
Response: 339328
Conc: 11.20 ng/ml

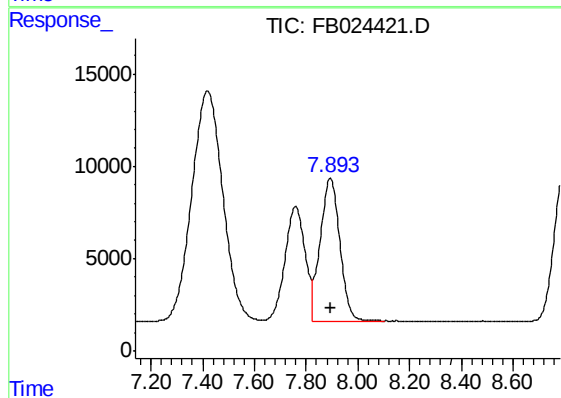


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 409229
Conc: 10.82 ng/ml

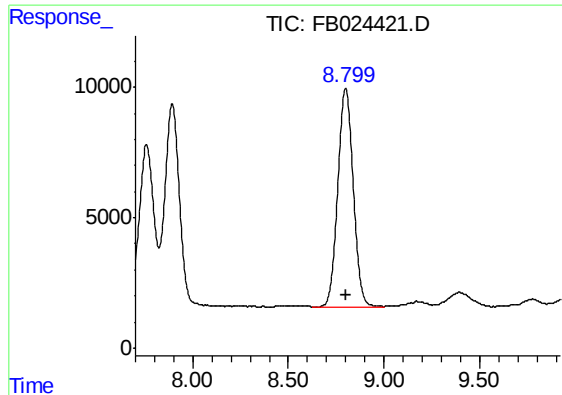


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.001 min
Response: 473032
Conc: 21.42 ng/ml

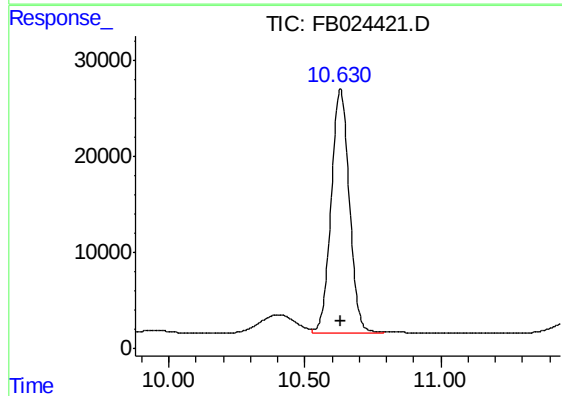


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1184684
Conc: 32.69 ng/ml

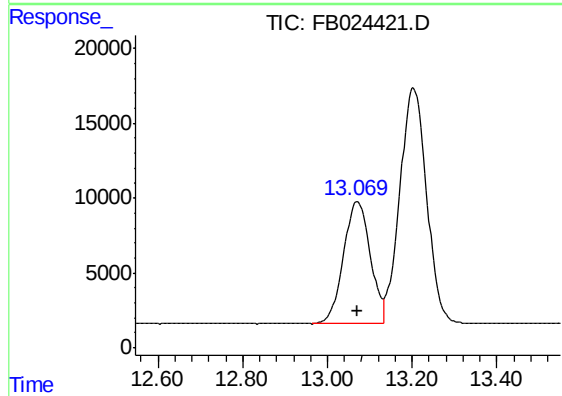


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 359426
Conc: 10.60 ng/ml

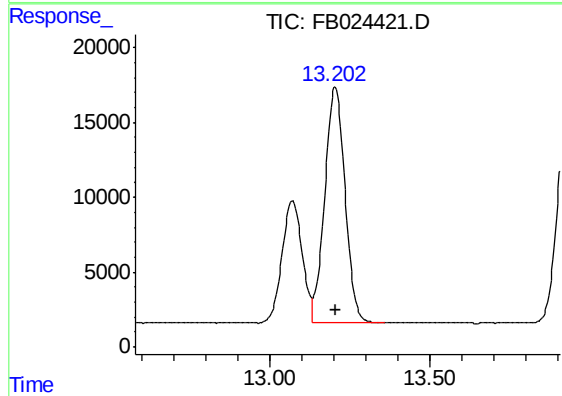


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 696709
Conc: 21.11 ng/ml

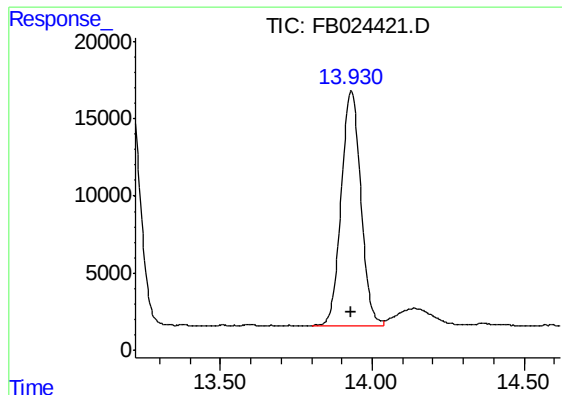

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 680719
Conc: 21.09 ng/ml

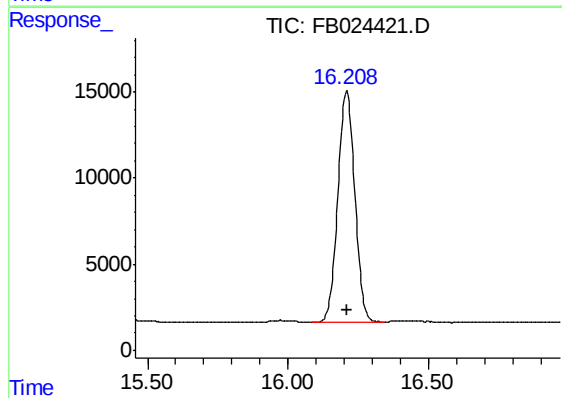

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 568355
Conc: 21.07 ng/ml