

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060420\
Data File : FB024424.D
Signal(s) : FID2B.CH
Acq On : 4 Jun 2020 11:00
Operator : DD/AJ
Sample : L2871-03
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 05 00:39:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	495256	22.428 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.684	2225	0.075 ng/ml
2) t 2,2,4-Trimethylpentane	7.409	925	0.030 ng/ml
4) t Benzene	7.892	2081	0.055 ng/ml
6) t Toluene	10.631	29936	0.826 ng/ml
8) t m-Xylene	13.199	2168	0.066 ng/ml
9) t O-Xylene	13.993	620	0.019 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060420\
Data File : FB024424.D
Signal(s) : FID2B.CH
Acq On : 4 Jun 2020 11:00
Operator : DD/AJ
Sample : L2871-03
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 05 00:39:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

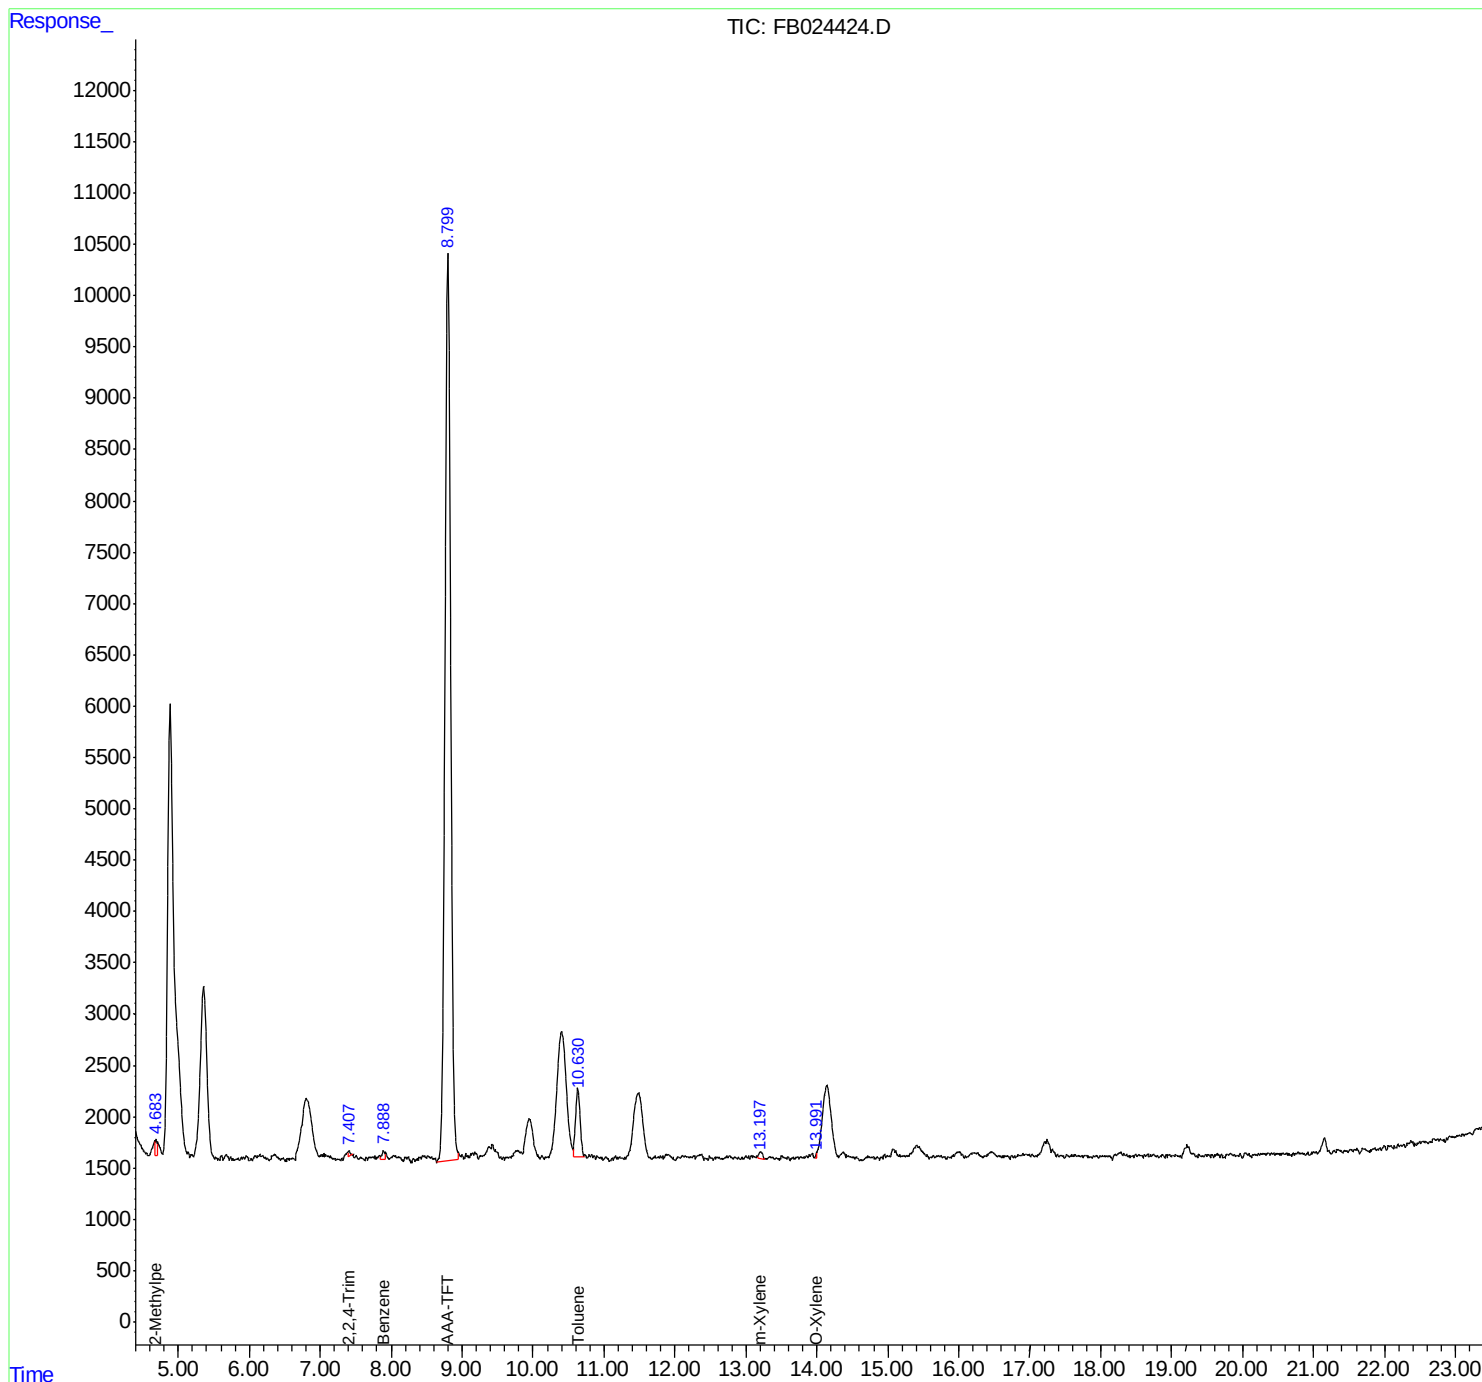

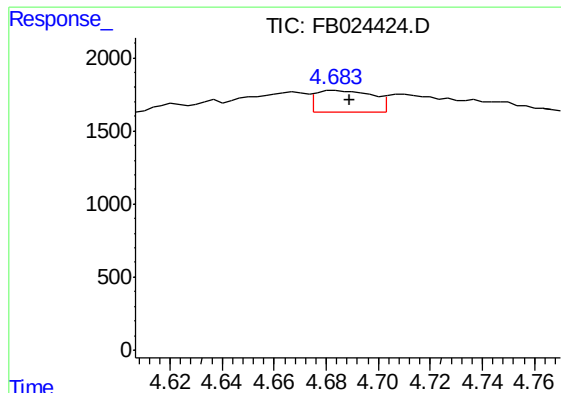


#1 2-Methylpentane

R.T.: 4.684 min
Delta R.T.: -0.005 min
Response: 2225
Conc: 0.08 ng/ml

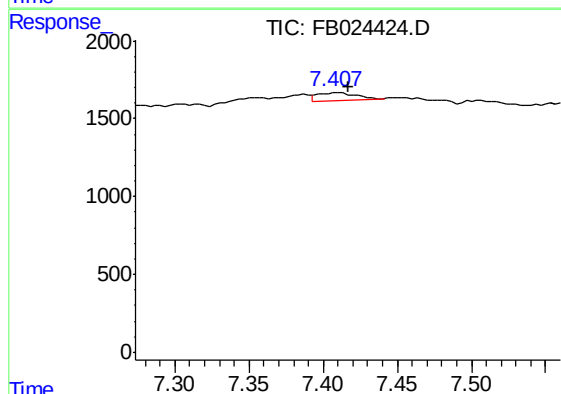


#2 2,2,4-Trimethylpentane

R.T.: 7.409 min
Delta R.T.: -0.008 min
Response: 925
Conc: 0.03 ng/ml

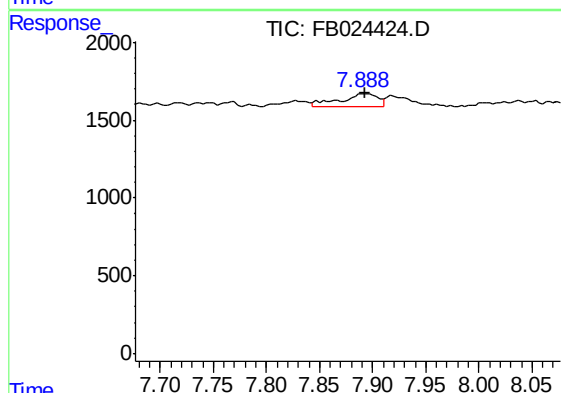


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 2081
Conc: 0.06 ng/ml

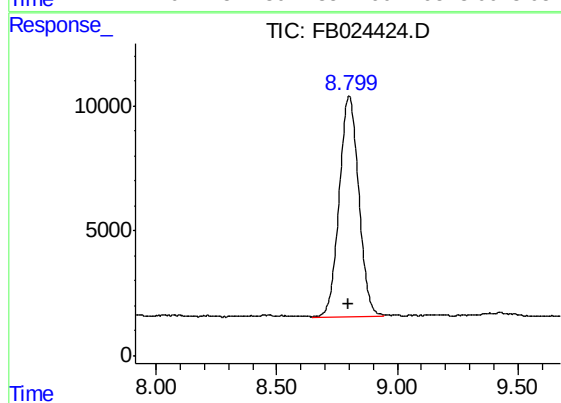


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 495256
Conc: 22.43 ng/ml

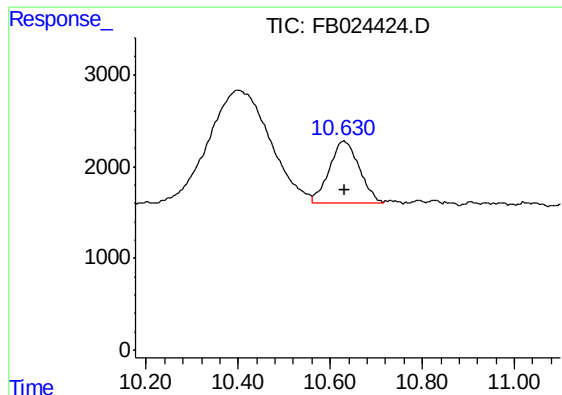


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 29936
Conc: 0.83 ng/ml

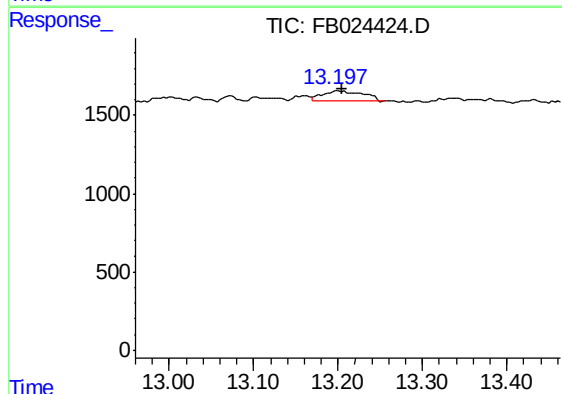

#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.006 min
Response: 2168
Conc: 0.07 ng/ml

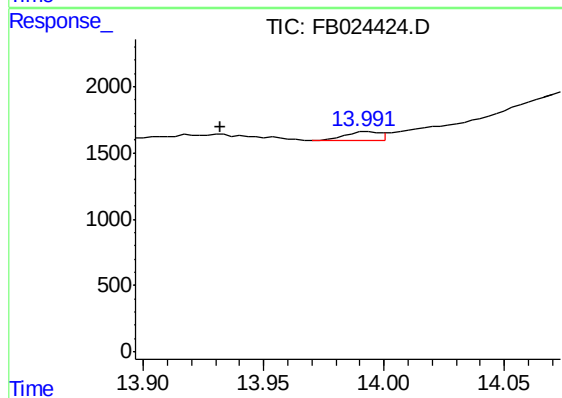

#9 O-Xylene

R.T.: 13.993 min
Delta R.T.: 0.061 min
Response: 620
Conc: 0.02 ng/ml