

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060421\
 Data File : FB025839.D
 Signal(s) : FID2B.CH
 Acq On : 4 Jun 2021 11:03
 Operator : DD/AJ
 Sample : BSF0604S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0604S1

Integration File: Calibration.e
 Quant Time: Jun 04 22:30:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060221.M
 Quant Title :
 QLast Update : Wed Jun 02 14:44:25 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.225	453222	17.894 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.198	750937	26.924 ng/ml
2) t 2,2,4-Trimethylpentane	7.885	628045	26.682 ng/ml
3) t n-Heptane	8.203	341430	9.341 ng/ml
4) t Benzene	8.354	385509	8.863 ng/ml
6) t Toluene	11.042	1150108	28.436 ng/ml
7) t Ethylbenzene	13.446	349221	9.033 ng/ml
8) t m-Xylene	13.577	705658	18.545 ng/ml
9) t O-Xylene	14.299	603506	16.881 ng/ml
10) t 1,2,4-Trimethylbenzene	16.551	407371	16.227 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060421\
Data File : FB025839.D
Signal(s) : FID2B.CH
Acq On : 4 Jun 2021 11:03
Operator : DD/AJ
Sample : BSF0604S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0604S1

Integration File: Calibration.e
Quant Time: Jun 04 22:30:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060221.M
Quant Title :
QLast Update : Wed Jun 02 14:44:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

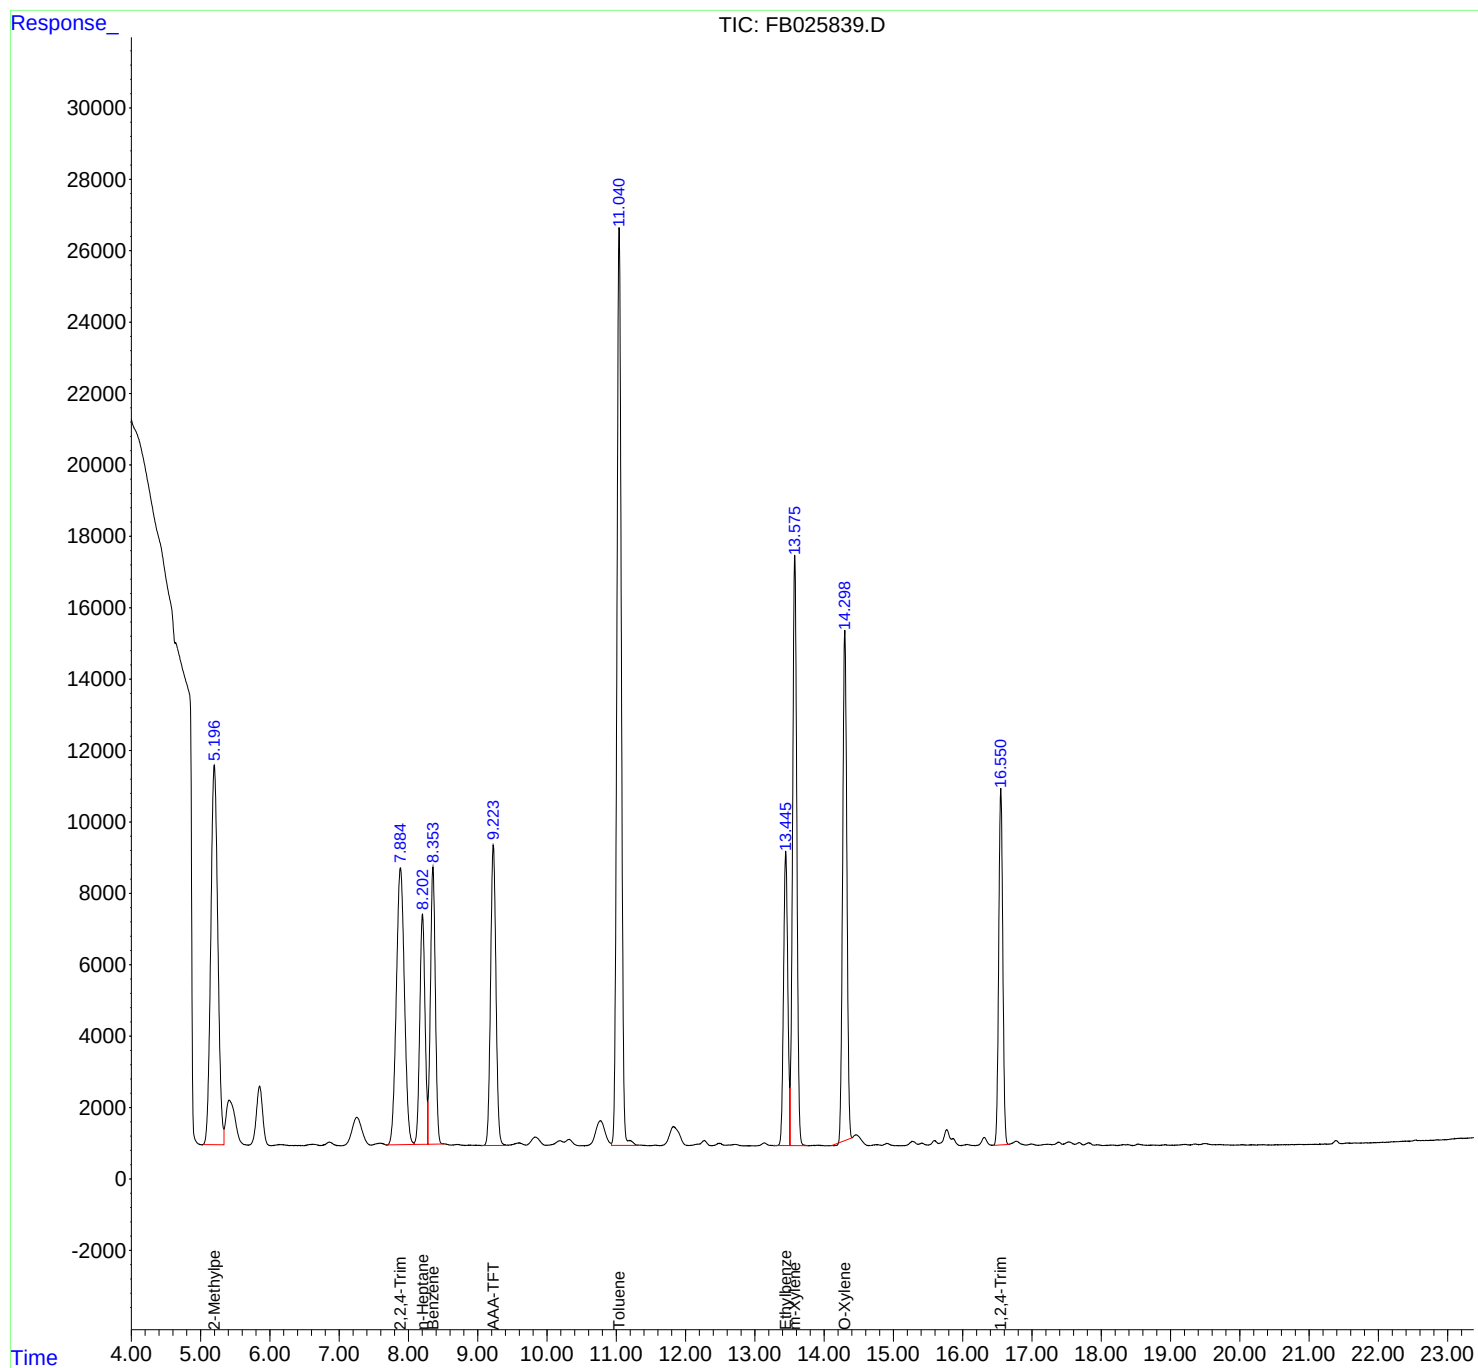


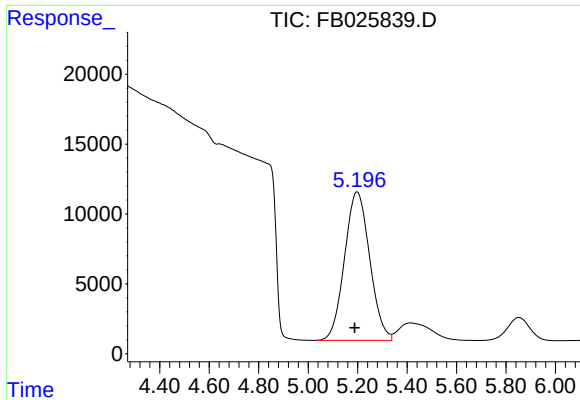

#1 2-Methylpentane


R.T.: 5.198 min
Delta R.T.: 0.009 min
Response: 750937
Conc: 26.92 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0604S1

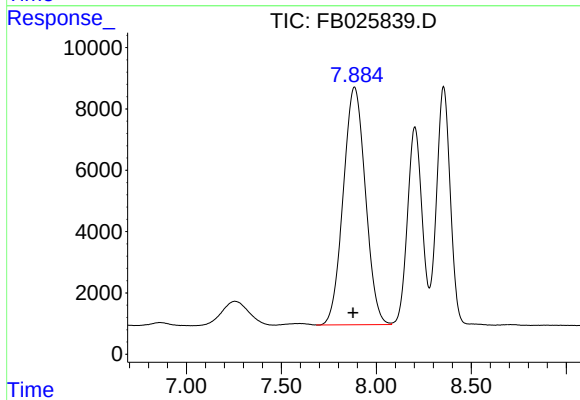


#2 2,2,4-Trimethylpentane

R.T.: 7.885 min
Delta R.T.: 0.007 min
Response: 628045
Conc: 26.68 ng/ml

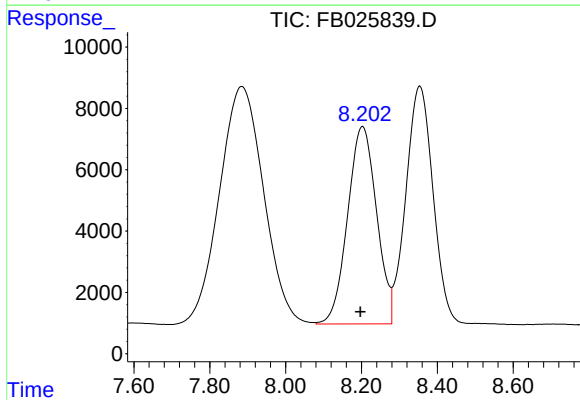


#3 n-Heptane

R.T.: 8.203 min
Delta R.T.: 0.006 min
Response: 341430
Conc: 9.34 ng/ml

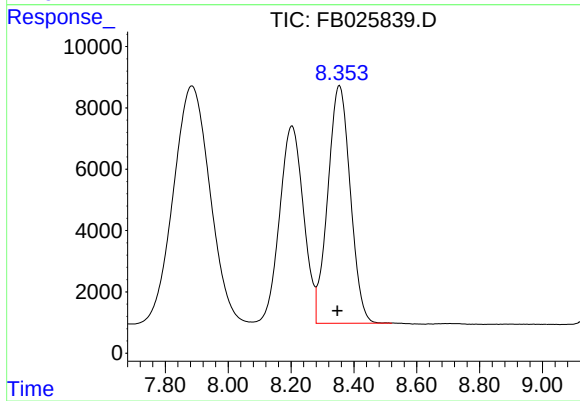

#4 Benzene


R.T.: 8.354 min
Delta R.T.: 0.006 min
Response: 385509
Conc: 8.86 ng/ml

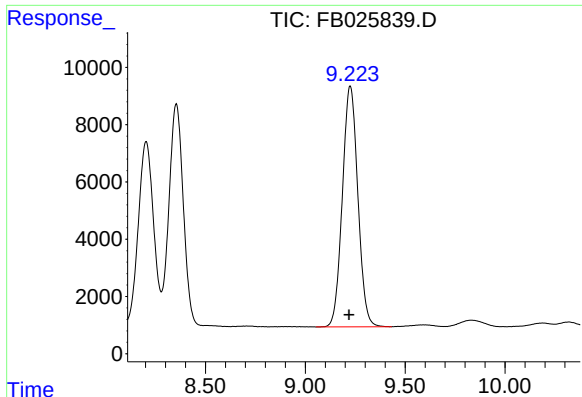

#5 AAA-TFT


R.T.: 9.225 min
Delta R.T.: 0.005 min
Response: 453222
Conc: 17.89 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0604S1

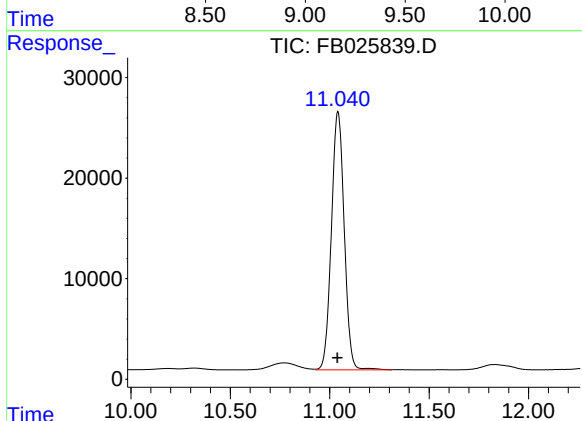


#6 Toluene

R.T.: 11.042 min
Delta R.T.: 0.004 min
Response: 1150108
Conc: 28.44 ng/ml

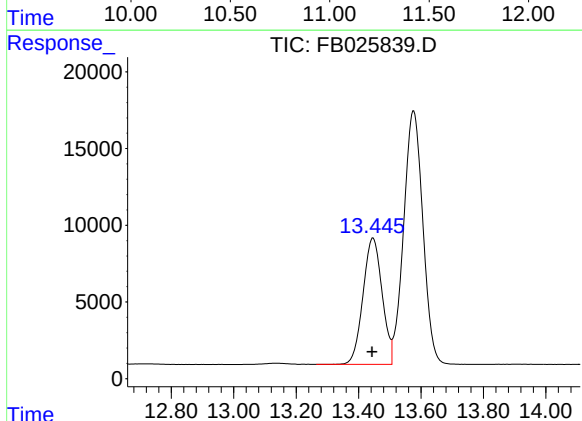


#7 Ethylbenzene

R.T.: 13.446 min
Delta R.T.: 0.004 min
Response: 349221
Conc: 9.03 ng/ml

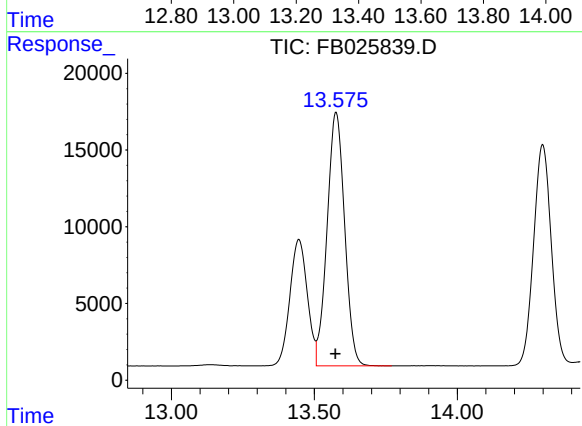

#8 m-Xylene


R.T.: 13.577 min
Delta R.T.: 0.003 min
Response: 705658
Conc: 18.55 ng/ml

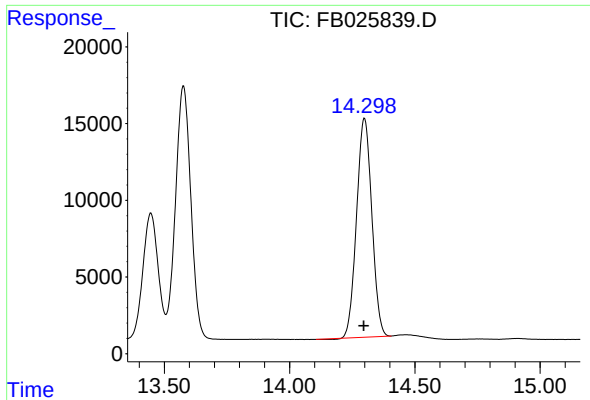

#9 O-Xylene

R.T.: 14.299 min
Delta R.T.: 0.003 min
Response: 603506
Conc: 16.88 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0604S1

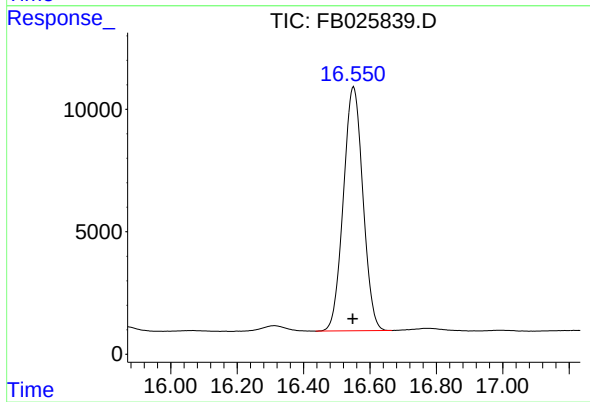

#10 1,2,4-Trimethylbenzene

R.T.: 16.551 min
Delta R.T.: 0.003 min
Response: 407371
Conc: 16.23 ng/ml