

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060421\
 Data File : FB025846.D
 Signal(s) : FID2B.CH
 Acq On : 4 Jun 2021 15:30
 Operator : DD/AJ
 Sample : M2597-01MSD
 Misc : 5.08g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 124019MSD

Integration File: Calibration.e
 Quant Time: Jun 04 22:31:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060221.M
 Quant Title :
 QLast Update : Wed Jun 02 14:44:25 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.214	440939	17.409 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.158	725175	26.000 ng/ml
2) t 2,2,4-Trimethylpentane	7.867	571984	24.300 ng/ml
3) t n-Heptane	8.186	329222	9.007 ng/ml
4) t Benzene	8.337	387310	8.904 ng/ml
6) t Toluene	11.036	1109143	27.423 ng/ml
7) t Ethylbenzene	13.444	347326	8.984 ng/ml
8) t m-Xylene	13.575	687002	18.055 ng/ml
9) t O-Xylene	14.298	600947	16.809 ng/ml
10) t 1,2,4-Trimethylbenzene	16.552	387774	15.446 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060421\
Data File : FB025846.D
Signal(s) : FID2B.CH
Acq On : 4 Jun 2021 15:30
Operator : DD/AJ
Sample : M2597-01MSD
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
124019MSD

Integration File: Calibration.e
Quant Time: Jun 04 22:31:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060221.M
Quant Title :
QLast Update : Wed Jun 02 14:44:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

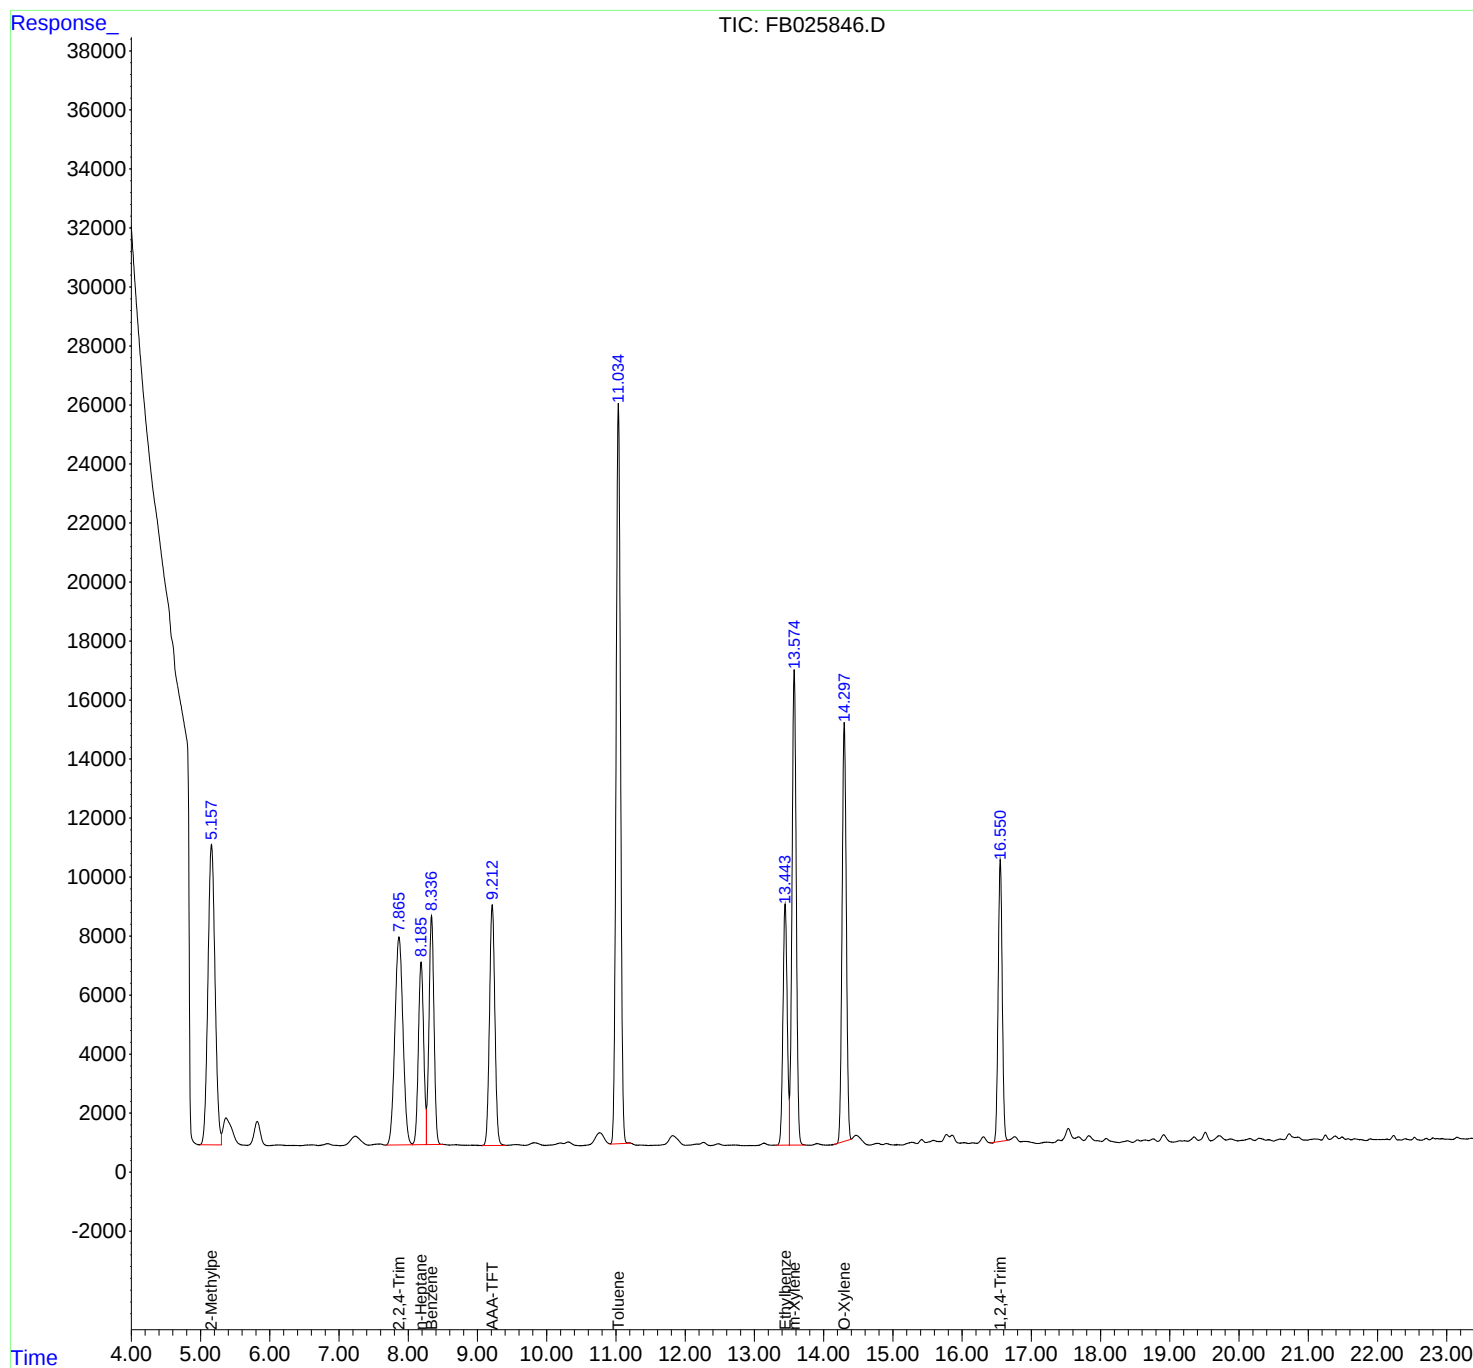


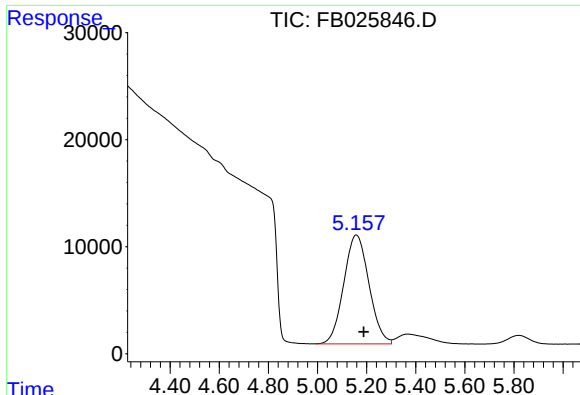

#1 2-Methylpentane


R.T.: 5.158 min
Delta R.T.: -0.031 min
Response: 725175
Conc: 26.00 ng/ml

Instrument :
FID_B
ClientSampleId :
124019MSD

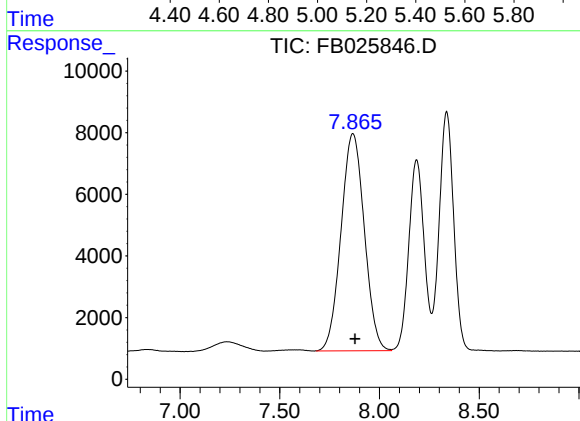


#2 2,2,4-Trimethylpentane

R.T.: 7.867 min
Delta R.T.: -0.012 min
Response: 571984
Conc: 24.30 ng/ml

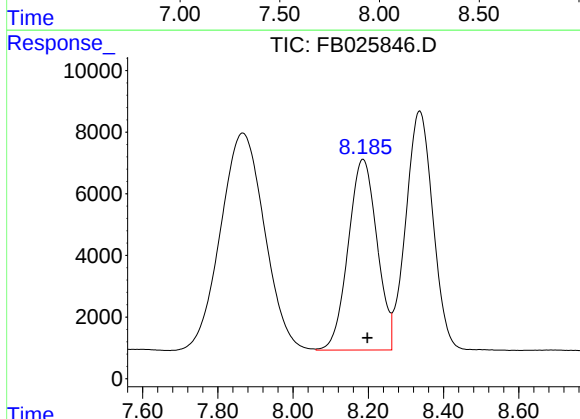


#3 n-Heptane

R.T.: 8.186 min
Delta R.T.: -0.011 min
Response: 329222
Conc: 9.01 ng/ml

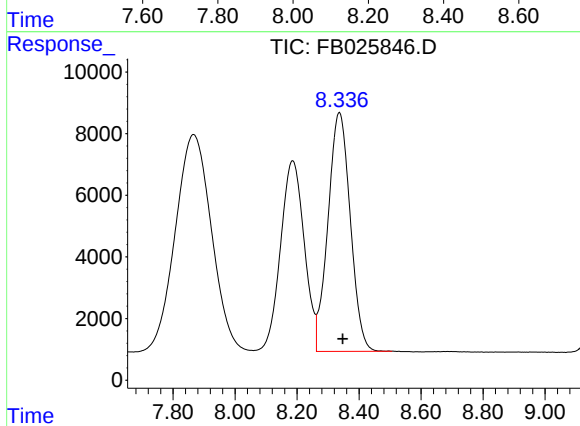

#4 Benzene


R.T.: 8.337 min
Delta R.T.: -0.011 min
Response: 387310
Conc: 8.90 ng/ml

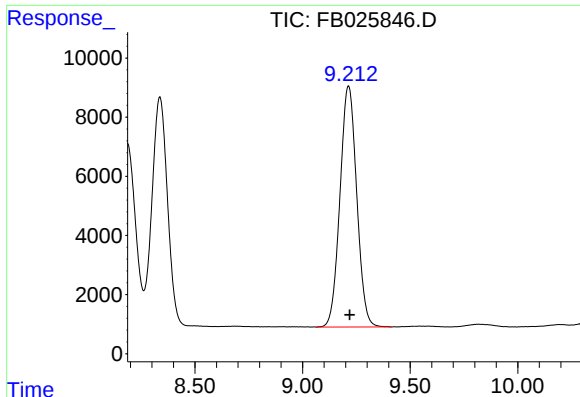

#5 AAA-TFT


R.T.: 9.214 min
Delta R.T.: -0.006 min
Response: 440939
Conc: 17.41 ng/ml

Instrument :
FID_B
ClientSampleId :
124019MSD

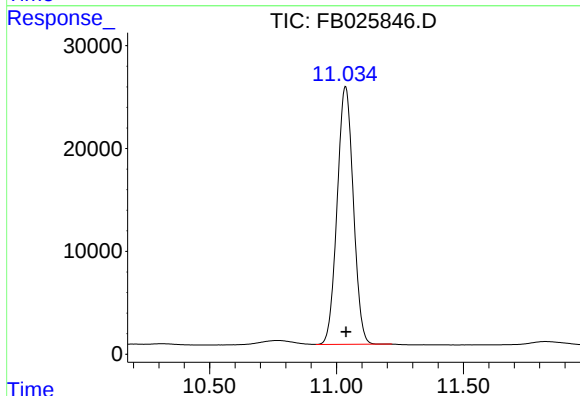


#6 Toluene

R.T.: 11.036 min
Delta R.T.: -0.002 min
Response: 1109143
Conc: 27.42 ng/ml

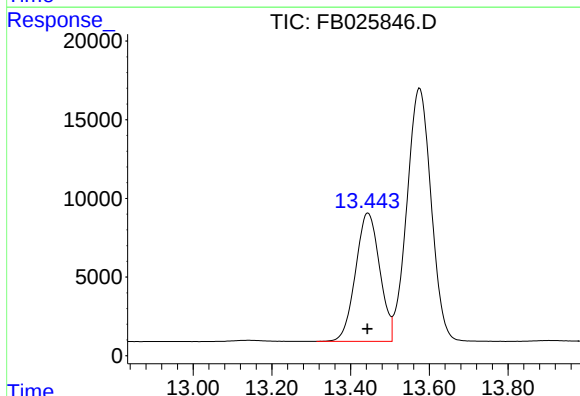


#7 Ethylbenzene

R.T.: 13.444 min
Delta R.T.: 0.002 min
Response: 347326
Conc: 8.98 ng/ml

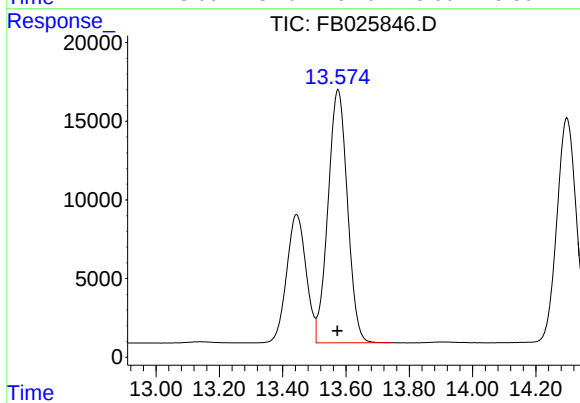

#8 m-Xylene


R.T.: 13.575 min
Delta R.T.: 0.002 min
Response: 687002
Conc: 18.05 ng/ml

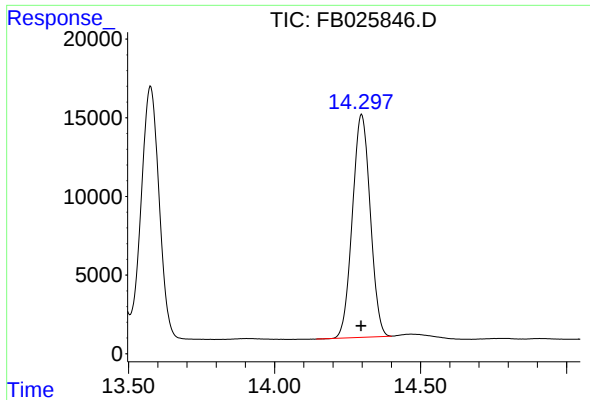

#9 O-Xylene

R.T.: 14.298 min
Delta R.T.: 0.003 min
Response: 600947
Conc: 16.81 ng/ml

Instrument :
FID_B
ClientSampleId :
124019MSD

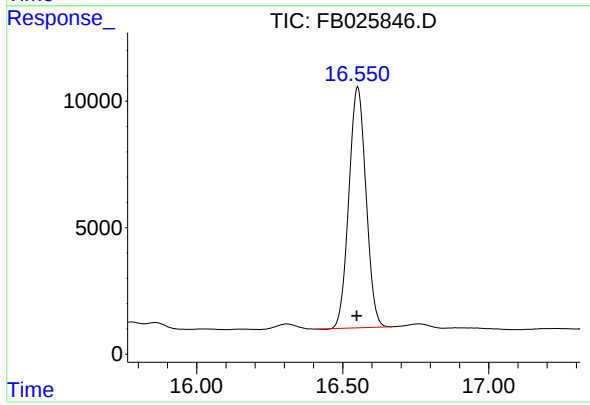

#10 1,2,4-Trimethylbenzene

R.T.: 16.552 min
Delta R.T.: 0.004 min
Response: 387774
Conc: 15.45 ng/ml