

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060523\
Data File : FB029970.D
Signal(s) : FID2B.CH
Acq On : 5 Jun 2023 15:07
Operator : YP/AJ
Sample : 03039-06 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 06 01:40:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	261544	18.799 ng/ml
Target Compounds			
8) t m-Xylene	13.180	5446	0.271 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060523\
Data File : FB029970.D
Signal(s) : FID2B.CH
Acq On : 5 Jun 2023 15:07
Operator : YP/AJ
Sample : 03039-06 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 06 01:40:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

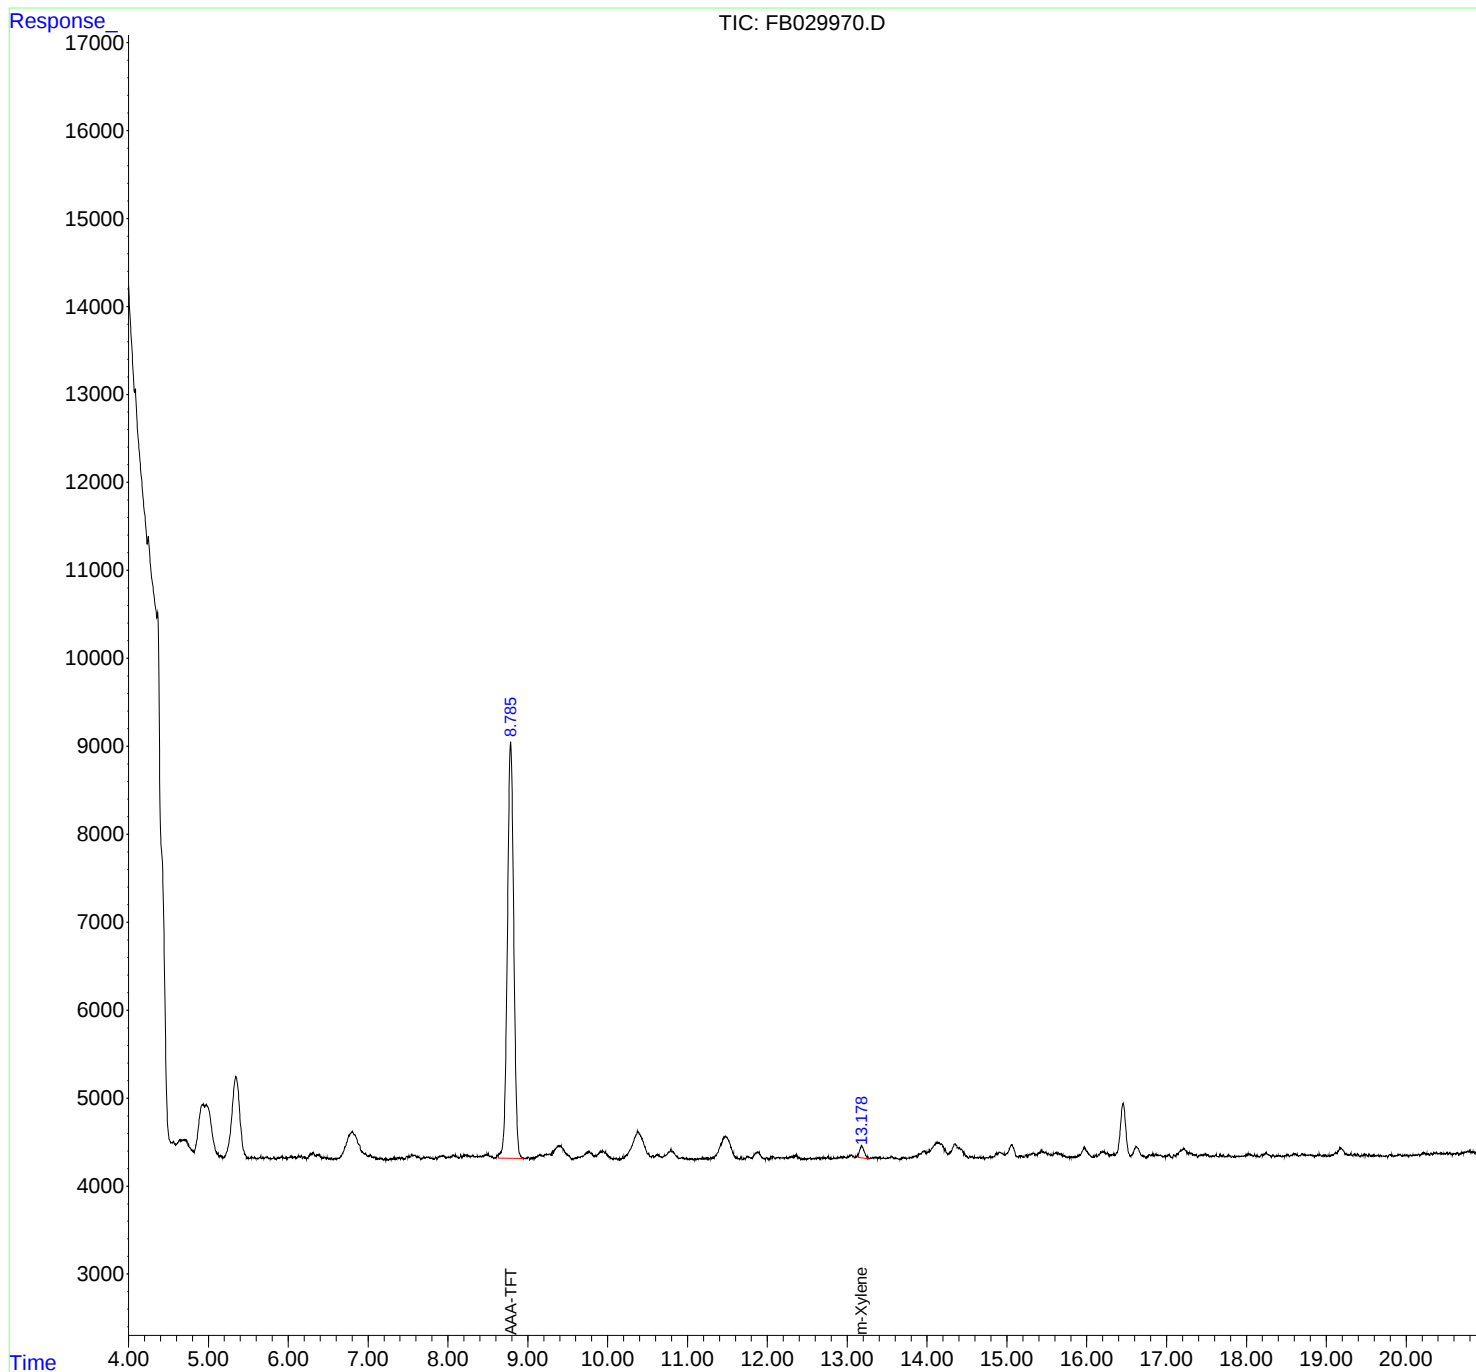


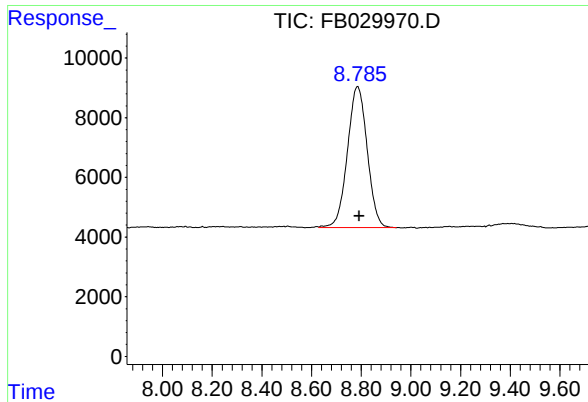

#5 AAA-TFT

R.T.: 8.786 min
Delta R.T.: -0.007 min
Response: 261544
Conc: 18.80 ng/ml

Instrument :
FID_B
ClientSampleId :

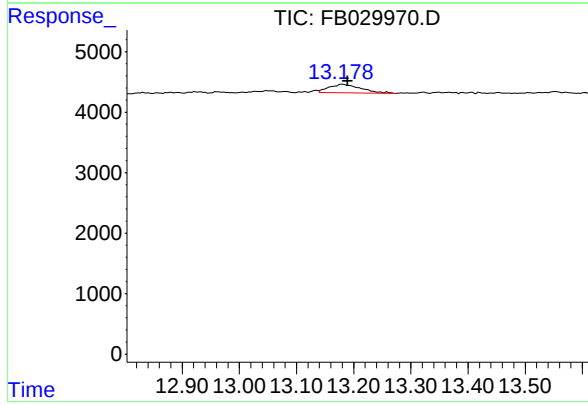

#8 m-Xylene

R.T.: 13.180 min
Delta R.T.: -0.009 min
Response: 5446
Conc: 0.27 ng/ml