

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060523\
 Data File : FB029967.D
 Signal(s) : FID2B.CH
 Acq On : 5 Jun 2023 11:59
 Operator : YP/AJ
 Sample : BSF0605S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0605S1

Integration File: Calibration.e
 Quant Time: Jun 06 01:40:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:33:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	305938	21.990 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	628827	33.282 ng/ml
2) t 2,2,4-Trimethylpentane	7.410	600889	31.845 ng/ml
3) t n-Heptane	7.744	224509	11.599 ng/ml
4) t Benzene	7.880	255259	11.404 ng/ml
6) t Toluene	10.613	744602	34.308 ng/ml
7) t Ethylbenzene	13.050	231206	11.434 ng/ml
8) t m-Xylene	13.182	453894	22.570 ng/ml
9) t O-Xylene	13.909	434361	22.286 ng/ml
10) t 1,2,4-Trimethylbenzene	16.183	419800	22.413 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060523\
Data File : FB029967.D
Signal(s) : FID2B.CH
Acq On : 5 Jun 2023 11:59
Operator : YP/AJ
Sample : BSF0605S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0605S1

Integration File: Calibration.e
Quant Time: Jun 06 01:40:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

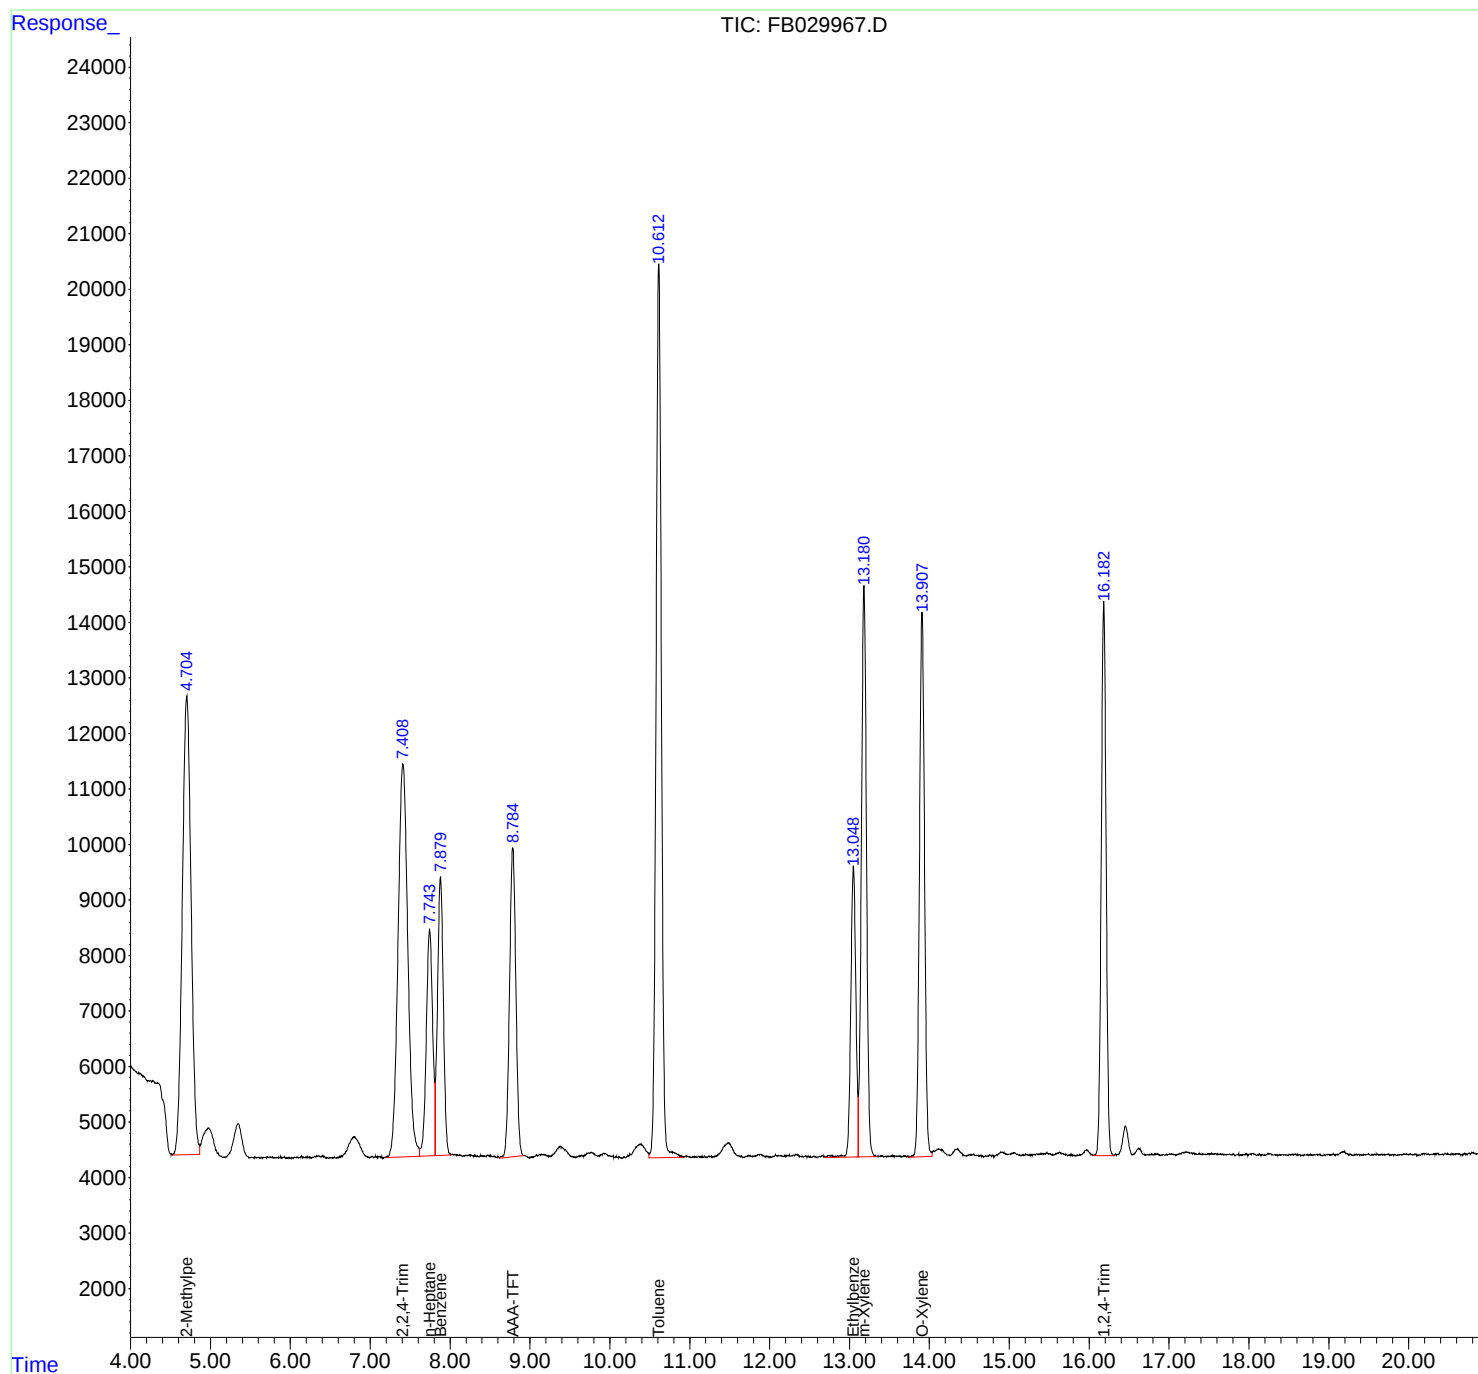


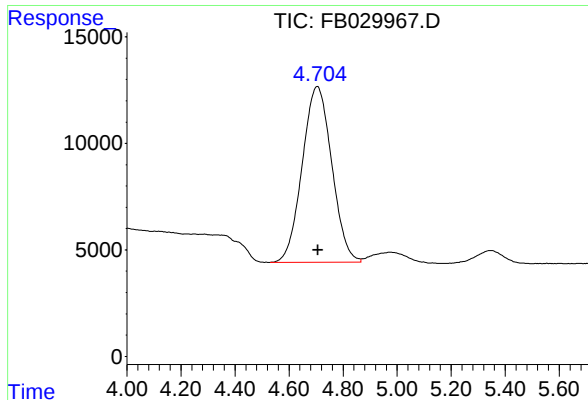

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.003 min
Response: 628827
Conc: 33.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0605S1

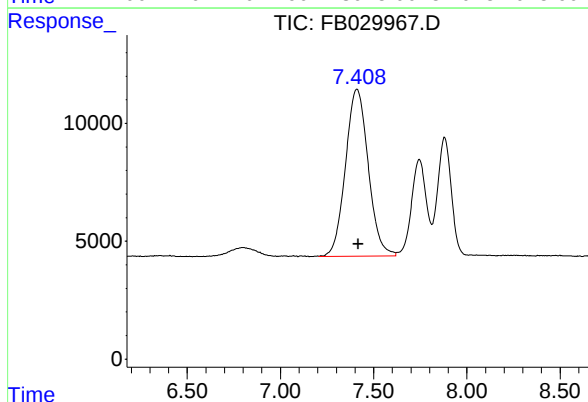


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: -0.009 min
Response: 600889
Conc: 31.85 ng/ml

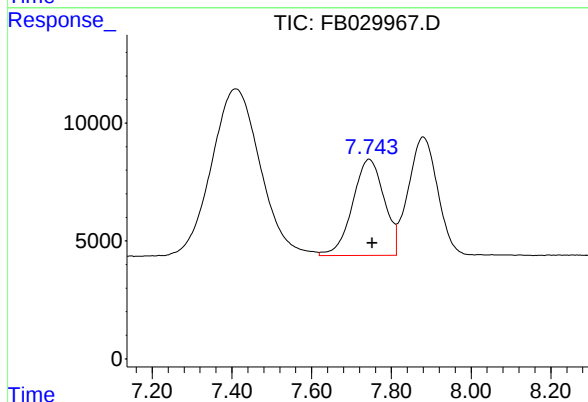


#3 n-Heptane

R.T.: 7.744 min
Delta R.T.: -0.008 min
Response: 224509
Conc: 11.60 ng/ml

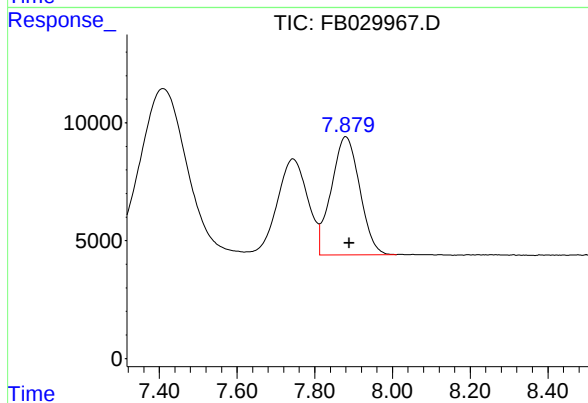

#4 Benzene


R.T.: 7.880 min
Delta R.T.: -0.008 min
Response: 255259
Conc: 11.40 ng/ml

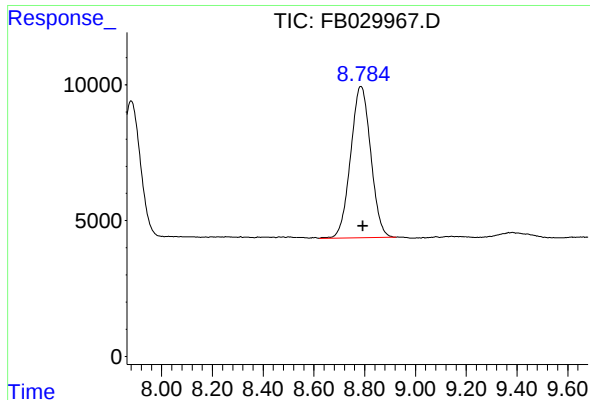

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: -0.007 min
Response: 305938
Conc: 21.99 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0605S1

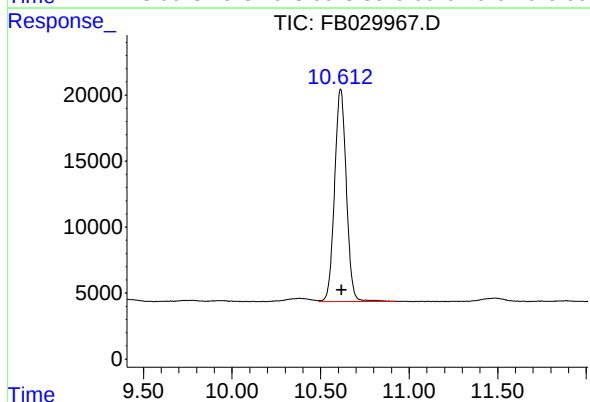


#6 Toluene

R.T.: 10.613 min
Delta R.T.: -0.007 min
Response: 744602
Conc: 34.31 ng/ml

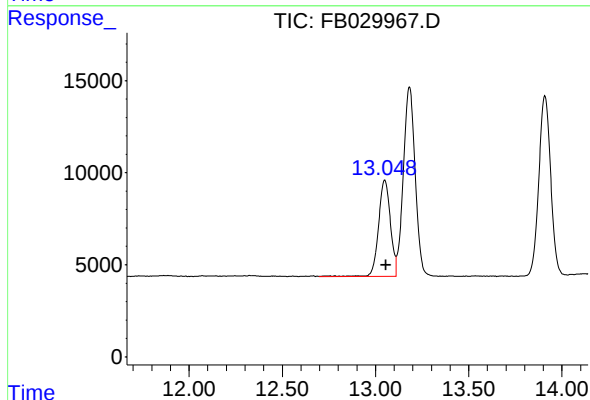


#7 Ethylbenzene

R.T.: 13.050 min
Delta R.T.: -0.007 min
Response: 231206
Conc: 11.43 ng/ml

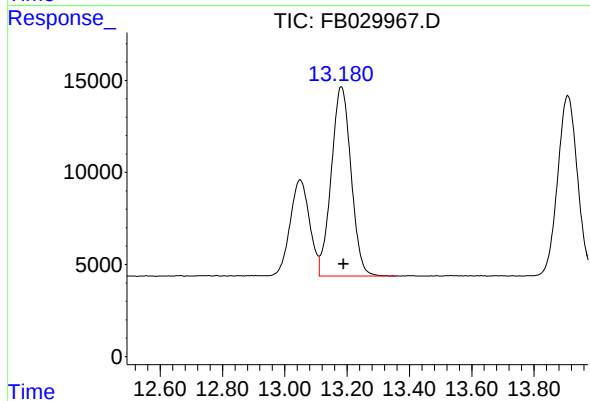

#8 m-Xylene


R.T.: 13.182 min
Delta R.T.: -0.007 min
Response: 453894
Conc: 22.57 ng/ml

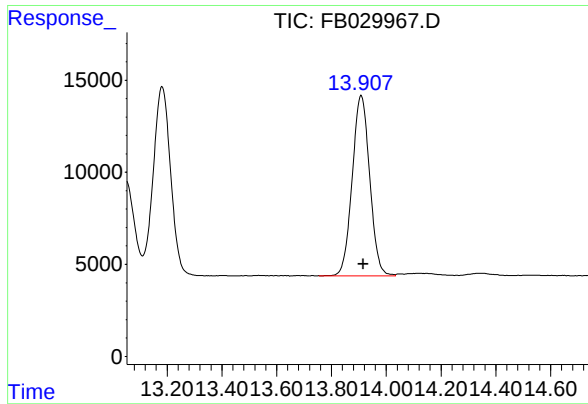

#9 O-Xylene

R.T.: 13.909 min
Delta R.T.: -0.007 min
Response: 434361
Conc: 22.29 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0605S1

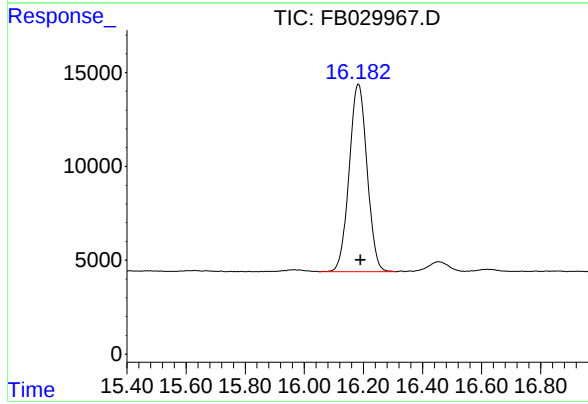

#10 1,2,4-Trimethylbenzene

R.T.: 16.183 min
Delta R.T.: -0.007 min
Response: 419800
Conc: 22.41 ng/ml