

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060523\
 Data File : FB029972.D
 Signal(s) : FID2B.CH
 Acq On : 5 Jun 2023 16:22
 Operator : YP/AJ
 Sample : 03039-06MSD 50X
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 WC31MSD

Integration File: Calibration.e
 Quant Time: Jun 06 01:40:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:33:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	253571	18.226 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.700	386881	20.477 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	438266	23.227 ng/ml
3) t n-Heptane	7.744	138976	7.180 ng/ml
4) t Benzene	7.880	194908	8.707 ng/ml
6) t Toluene	10.614	552185	25.443 ng/ml
7) t Ethylbenzene	13.052	172703	8.541 ng/ml
8) t m-Xylene	13.184	347194	17.264 ng/ml
9) t O-Xylene	13.911	347441	17.826 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	335842	17.930 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060523\
Data File : FB029972.D
Signal(s) : FID2B.CH
Acq On : 5 Jun 2023 16:22
Operator : YP/AJ
Sample : 03039-06MSD 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
WC31MSD

Integration File: Calibration.e
Quant Time: Jun 06 01:40:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

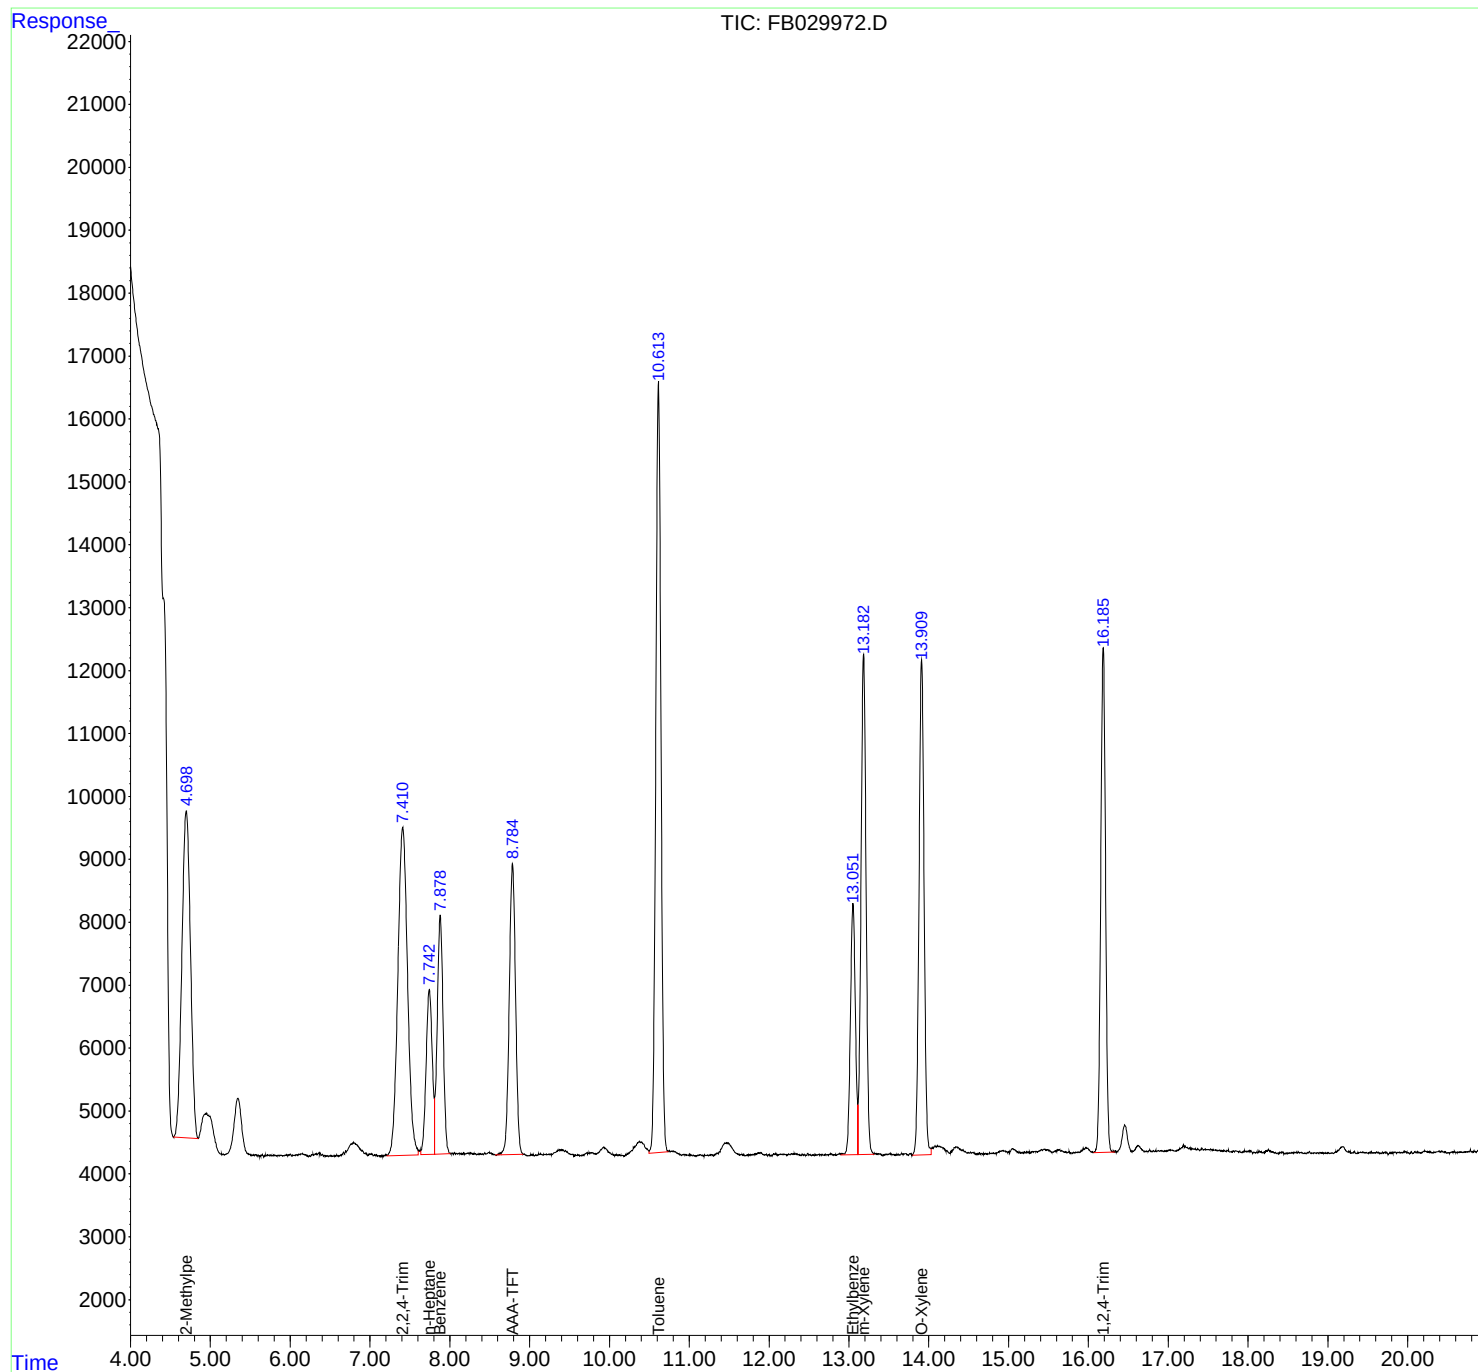


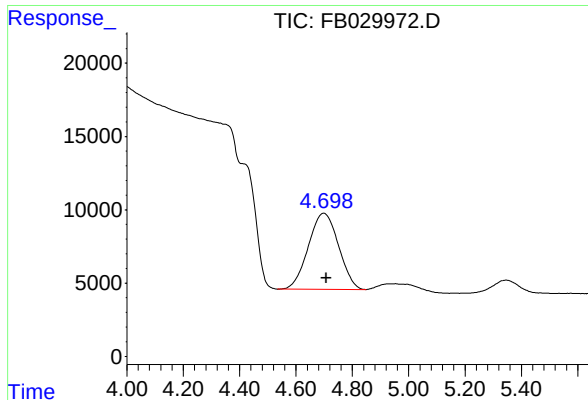

#1 2-Methylpentane


R.T.: 4.700 min
Delta R.T.: -0.008 min
Response: 386881
Conc: 20.48 ng/ml

Instrument :
FID_B
ClientSampleId :
WC31MSD

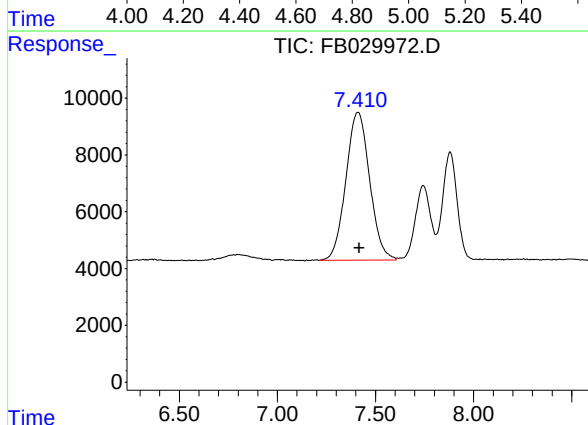


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.008 min
Response: 438266
Conc: 23.23 ng/ml

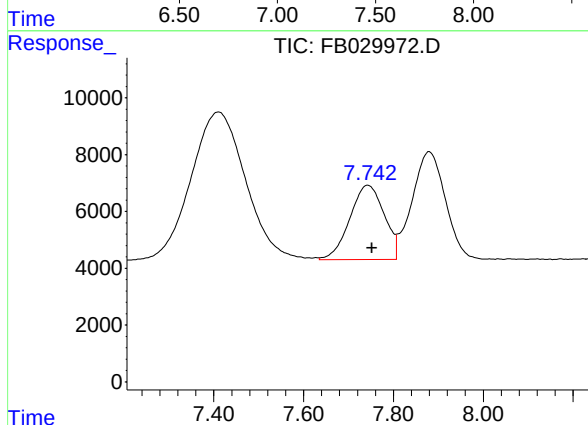


#3 n-Heptane

R.T.: 7.744 min
Delta R.T.: -0.008 min
Response: 138976
Conc: 7.18 ng/ml

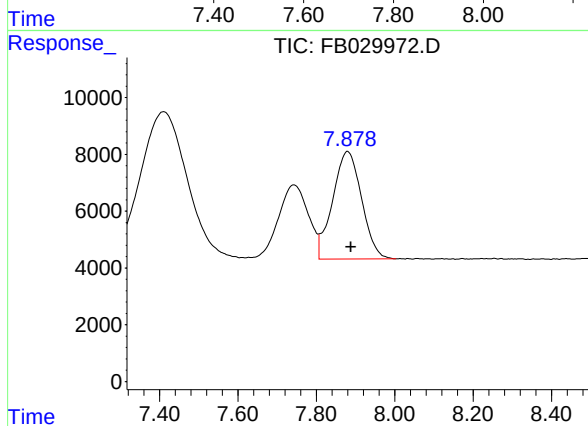

#4 Benzene


R.T.: 7.880 min
Delta R.T.: -0.009 min
Response: 194908
Conc: 8.71 ng/ml

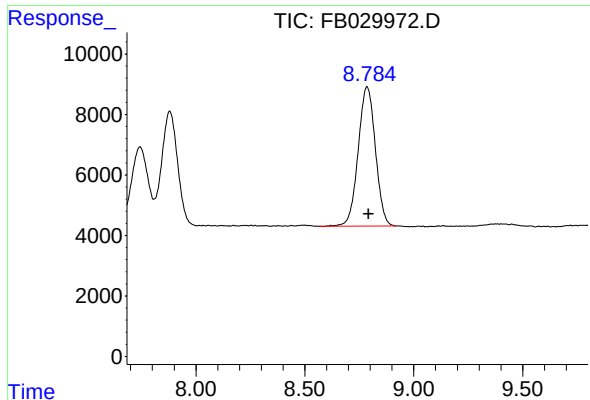

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: -0.007 min
Response: 253571
Conc: 18.23 ng/ml

Instrument :
FID_B
ClientSampleId :
WC31MSD

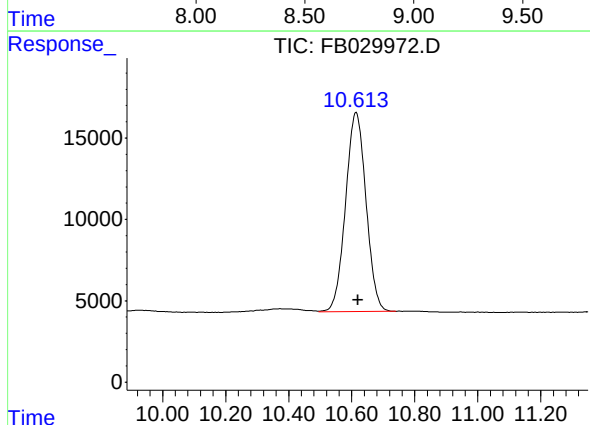


#6 Toluene

R.T.: 10.614 min
Delta R.T.: -0.006 min
Response: 552185
Conc: 25.44 ng/ml

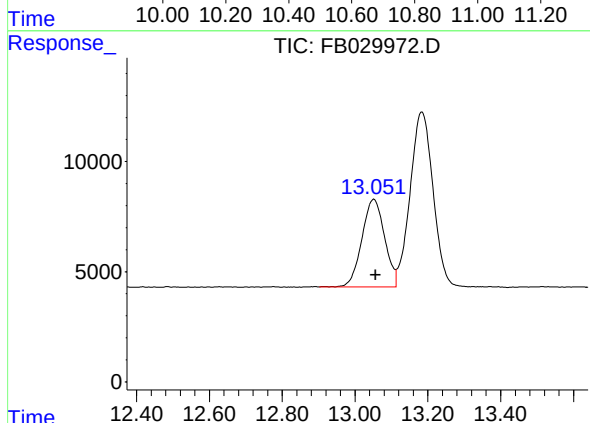


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.005 min
Response: 172703
Conc: 8.54 ng/ml

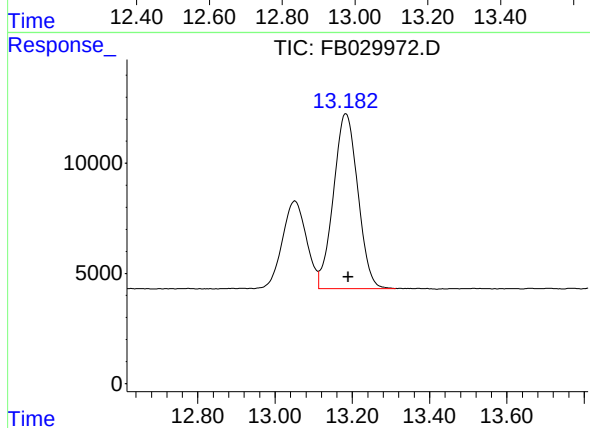

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: -0.005 min
Response: 347194
Conc: 17.26 ng/ml

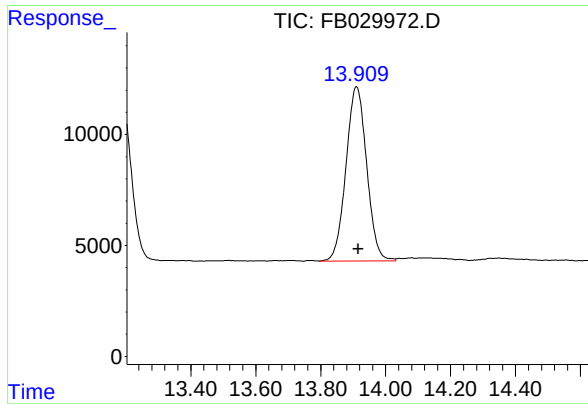

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: -0.005 min
Response: 347441
Conc: 17.83 ng/ml

Instrument :
FID_B
ClientSampleId :
WC31MSD

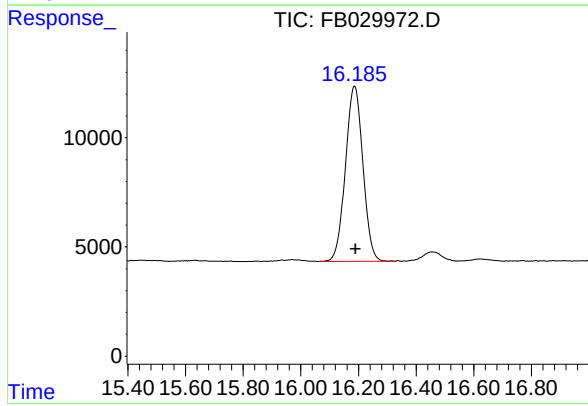

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: -0.004 min
Response: 335842
Conc: 17.93 ng/ml