

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060619\
Data File : FB021316.D
Signal(s) : FID2B.CH
Acq On : 6 Jun 2019 13:04
Operator : MJ/SJ
Sample : K2638-02MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 07 01:37:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.998	302186	20.495 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.859	968861	25.772 ng/ml
2) t	2,2,4-Trimethylpentane	7.614	790576	23.150 ng/ml
3) t	n-Heptane	7.954	235554	7.225 ng/ml
4) t	Benzene	8.091	336995	9.763 ng/ml
6) t	Toluene	10.843	694072	29.283 ng/ml
7) t	Ethylbenzene	13.294	222764	9.533 ng/ml
8) t	m-Xylene	13.427	476831	19.104 ng/ml
9) t	O-Xylene	14.158	501951	19.241 ng/ml
10) t	1,2,4-Trimethylbenzene	16.442	445030	16.571 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060619\
Data File : FB021316.D
Signal(s) : FID2B.CH
Acq On : 6 Jun 2019 13:04
Operator : MJ/SJ
Sample : K2638-02MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 07 01:37:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

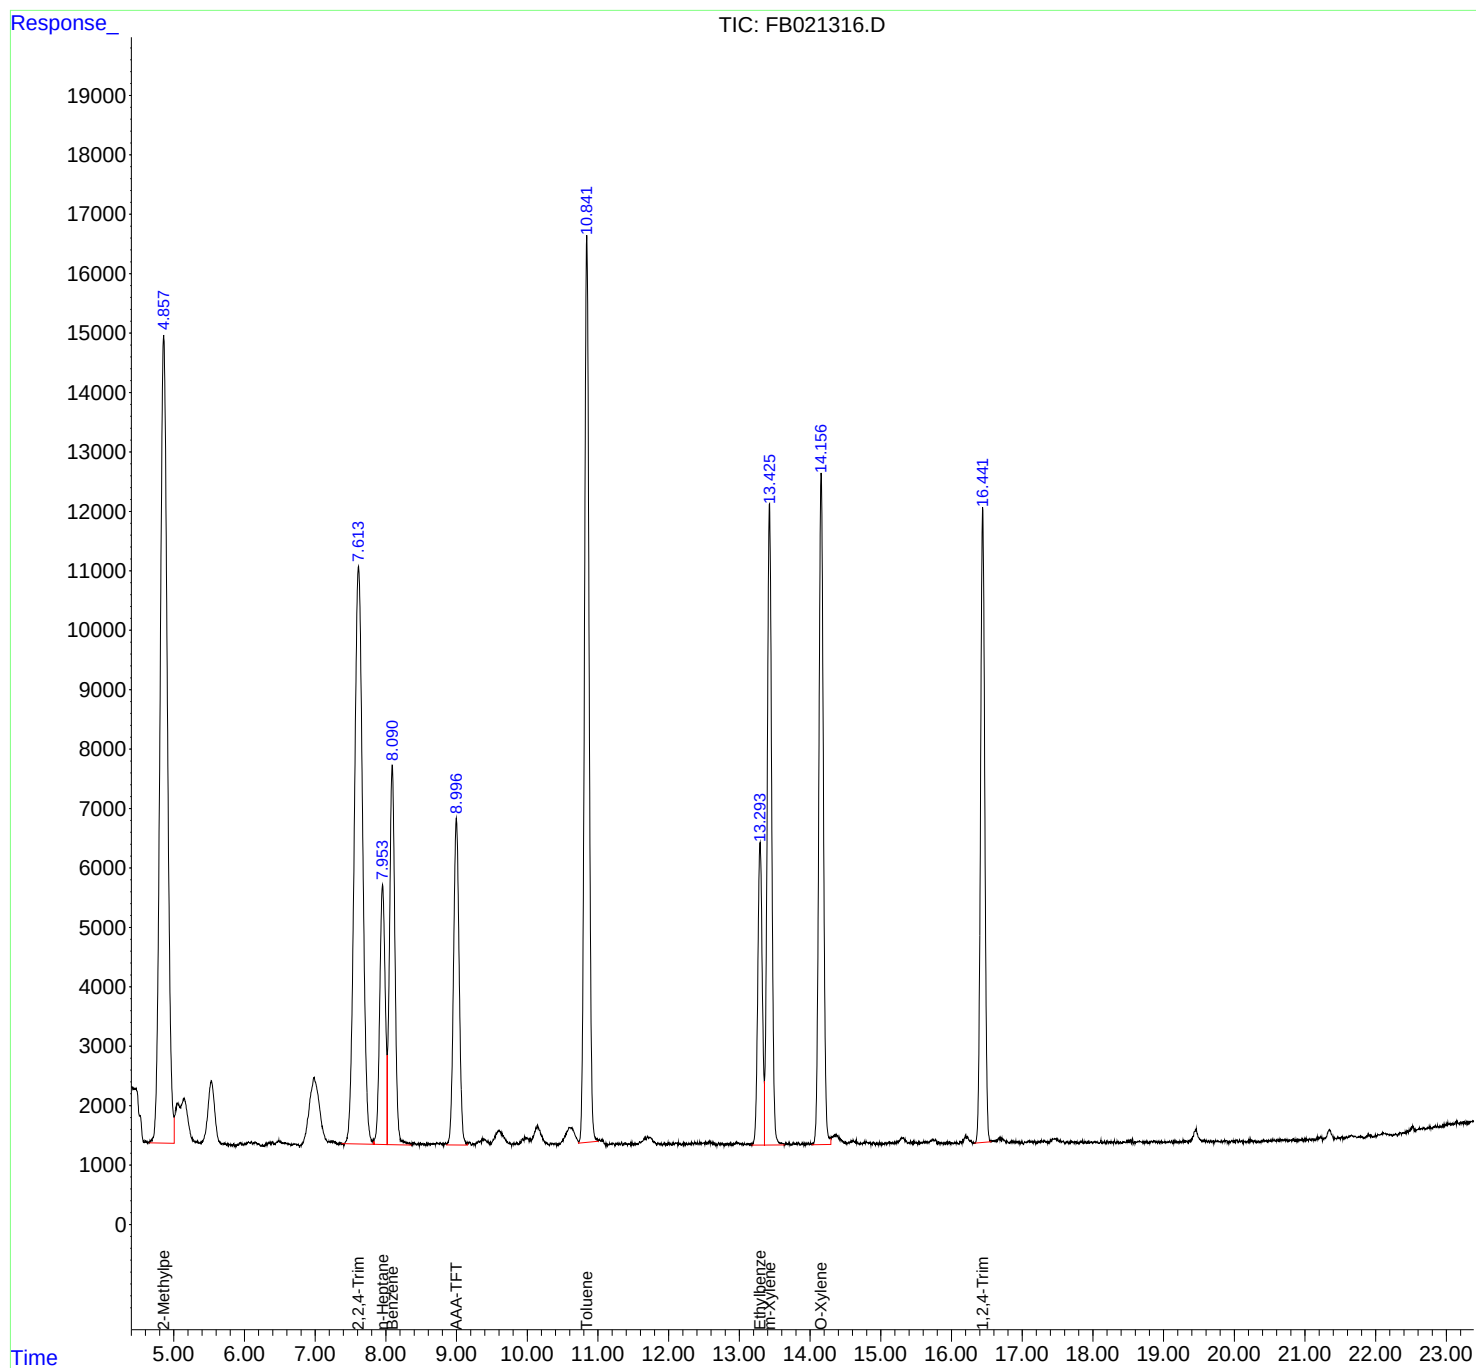

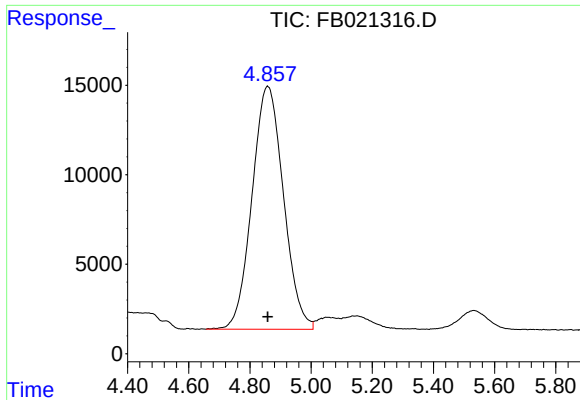


#1 2-Methylpentane

R.T.: 4.859 min

Delta R.T.: 0.000 min

Response: 968861

Conc: 25.77 ng/ml

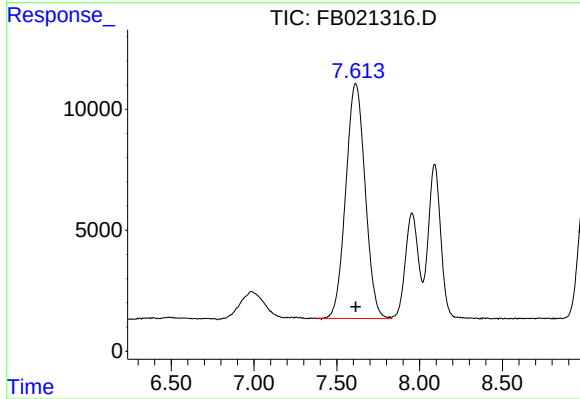


#2 2,2,4-Trimethylpentane

R.T.: 7.614 min

Delta R.T.: 0.000 min

Response: 790576

Conc: 23.15 ng/ml

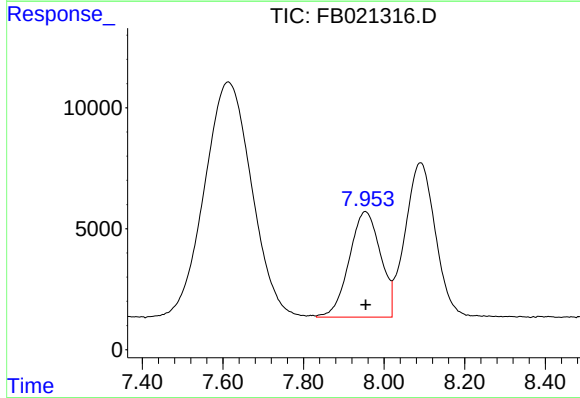


#3 n-Heptane

R.T.: 7.954 min

Delta R.T.: 0.000 min

Response: 235554

Conc: 7.23 ng/ml

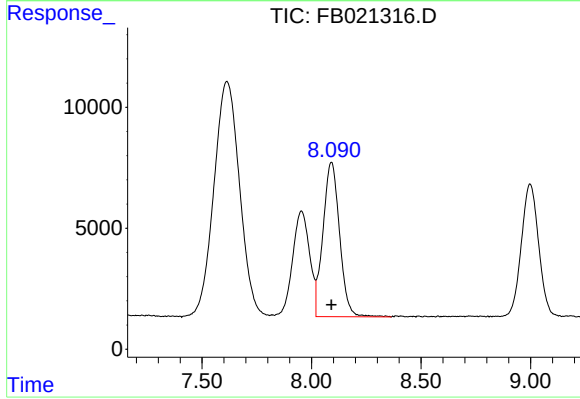


#4 Benzene

R.T.: 8.091 min

Delta R.T.: 0.000 min


Response: 336995

Conc: 9.76 ng/ml

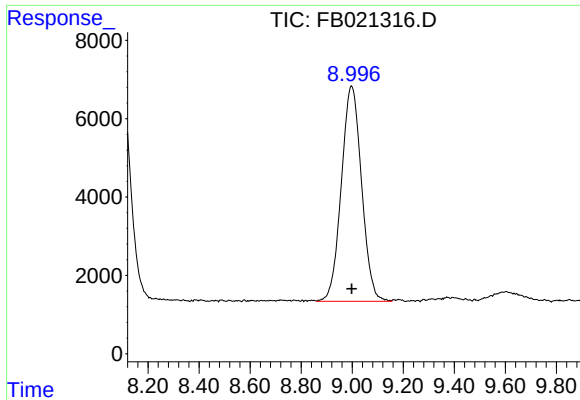


#5 AAA-TFT

R.T.: 8.998 min
 Delta R.T.: 0.000 min
 Response: 302186
 Conc: 20.50 ng/ml

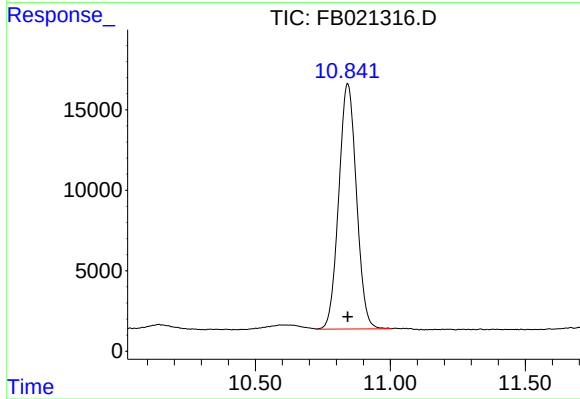


#6 Toluene

R.T.: 10.843 min
 Delta R.T.: 0.000 min
 Response: 694072
 Conc: 29.28 ng/ml

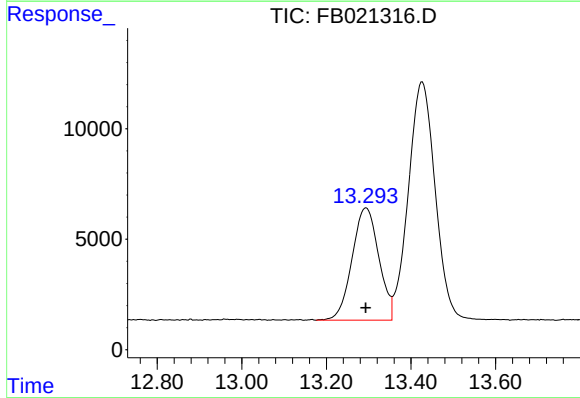


#7 Ethylbenzene

R.T.: 13.294 min
 Delta R.T.: 0.000 min
 Response: 222764
 Conc: 9.53 ng/ml

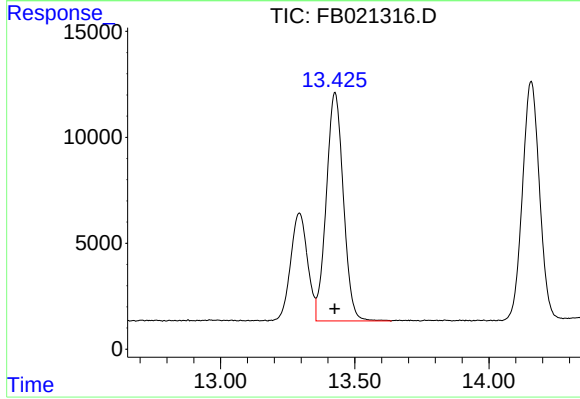


#8 m-Xylene

R.T.: 13.427 min
 Delta R.T.: 0.000 min
 Response: 476831
 Conc: 19.10 ng/ml

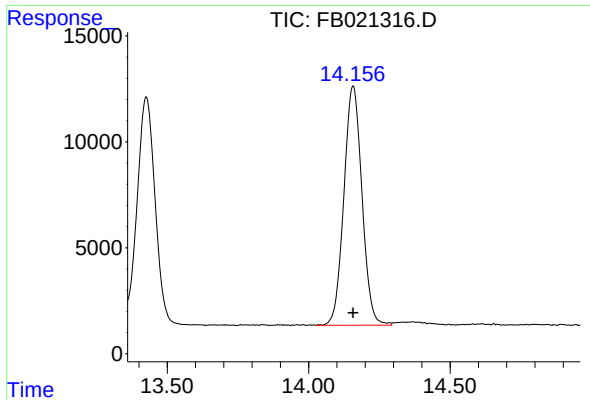

#9 O-Xylene

R.T.: 14.158 min
Delta R.T.: 0.000 min
Response: 501951
Conc: 19.24 ng/ml

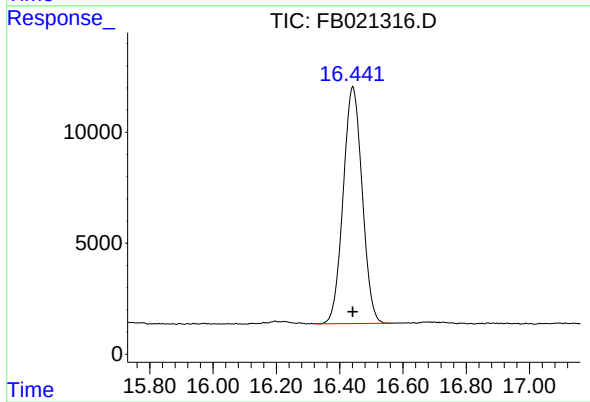

#10 1,2,4-Trimethylbenzene

R.T.: 16.442 min
Delta R.T.: 0.001 min
Response: 445030
Conc: 16.57 ng/ml