

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060619\
 Data File : FB021317.D
 Signal(s) : FID2B.CH
 Acq On : 6 Jun 2019 13:35
 Operator : MJ/SJ
 Sample : K2638-02MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 07 01:37:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.997	326444	22.141 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.856	993781	26.435 ng/ml
2) t 2,2,4-Trimethylpentane	7.612	832076	24.365 ng/ml
3) t n-Heptane	7.953	240538	7.378 ng/ml
4) t Benzene	8.090	329833	9.556 ng/ml
6) t Toluene	10.842	702088	29.621 ng/ml
7) t Ethylbenzene	13.293	225193	9.637 ng/ml
8) t m-Xylene	13.426	478904	19.187 ng/ml
9) t O-Xylene	14.157	507862	19.468 ng/ml
10) t 1,2,4-Trimethylbenzene	16.442	477458	17.779 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060619\
Data File : FB021317.D
Signal(s) : FID2B.CH
Acq On : 6 Jun 2019 13:35
Operator : MJ/SJ
Sample : K2638-02MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 07 01:37:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

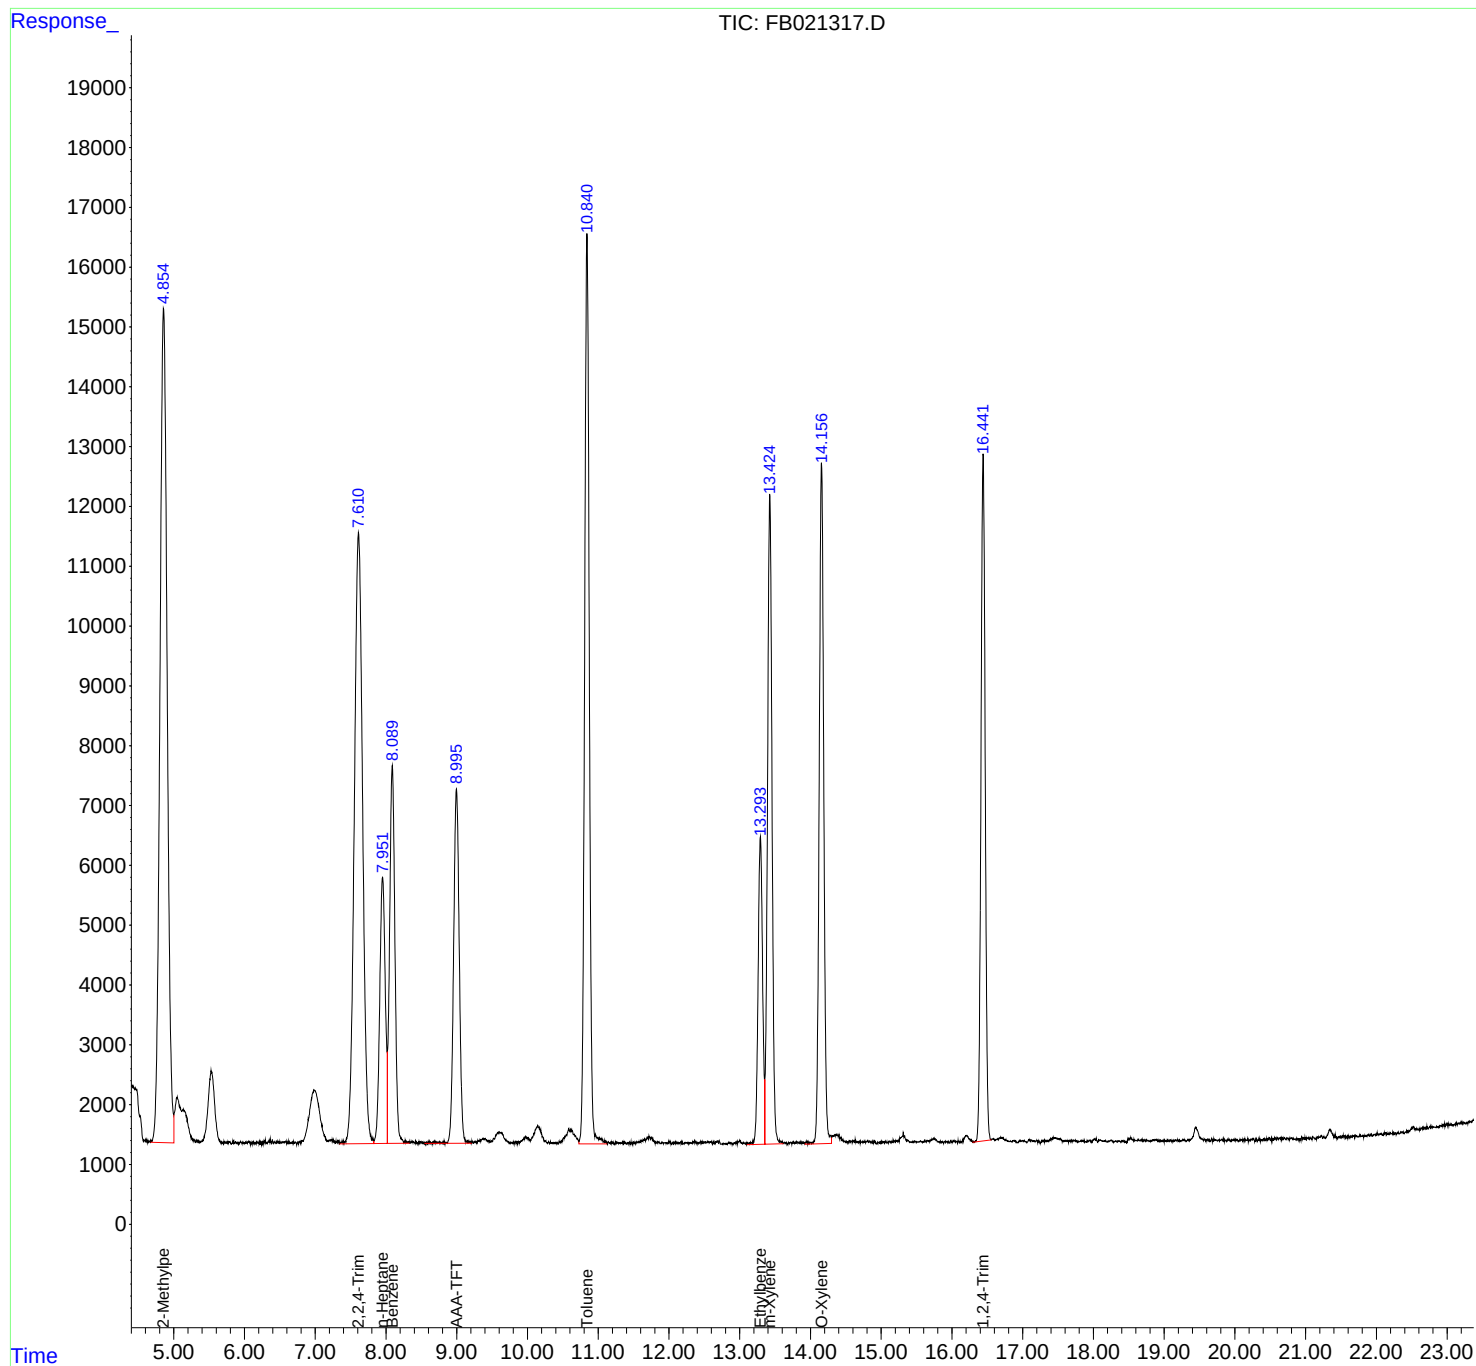

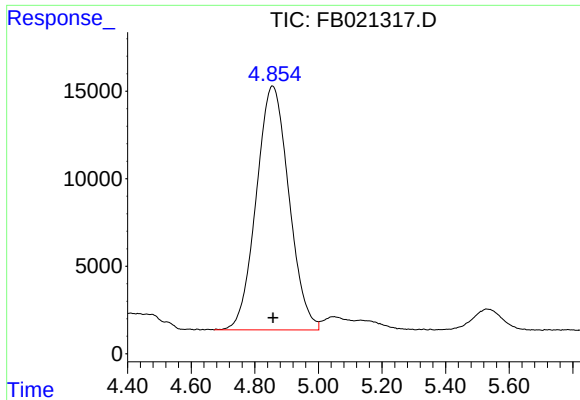


#1 2-Methylpentane

R.T.: 4.856 min
Delta R.T.: -0.002 min
Response: 993781
Conc: 26.43 ng/ml

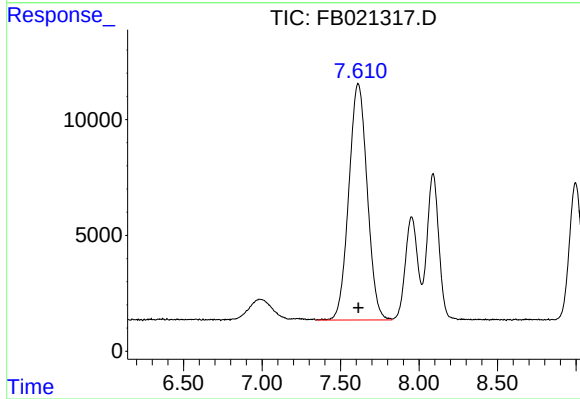


#2 2,2,4-Trimethylpentane

R.T.: 7.612 min
Delta R.T.: -0.002 min
Response: 832076
Conc: 24.37 ng/ml

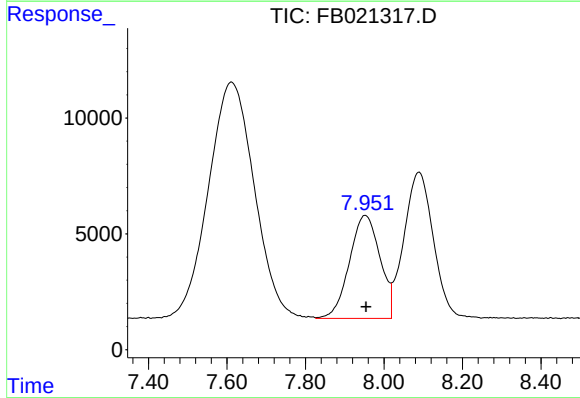


#3 n-Heptane

R.T.: 7.953 min
Delta R.T.: -0.001 min
Response: 240538
Conc: 7.38 ng/ml

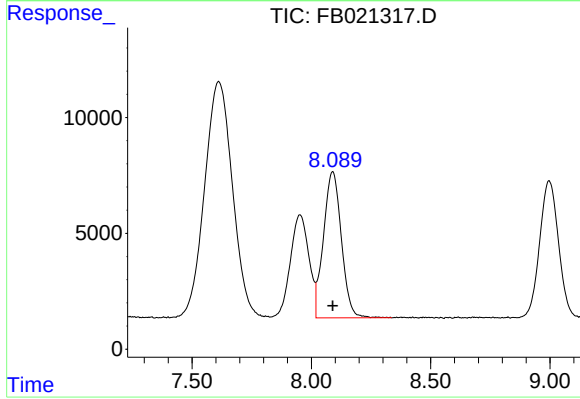


#4 Benzene

R.T.: 8.090 min
Delta R.T.: 0.000 min
Response: 329833
Conc: 9.56 ng/ml

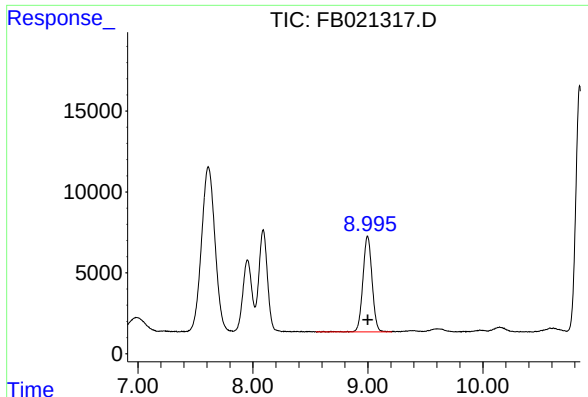


#5 AAA-TFT

R.T.: 8.997 min
Delta R.T.: -0.001 min
Response: 326444
Conc: 22.14 ng/ml

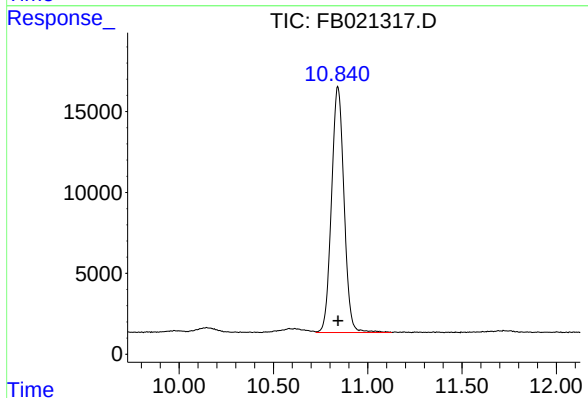


#6 Toluene

R.T.: 10.842 min
Delta R.T.: 0.000 min
Response: 702088
Conc: 29.62 ng/ml

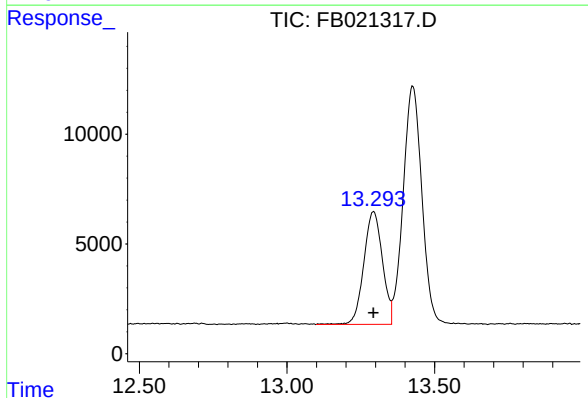


#7 Ethylbenzene

R.T.: 13.293 min
Delta R.T.: 0.000 min
Response: 225193
Conc: 9.64 ng/ml

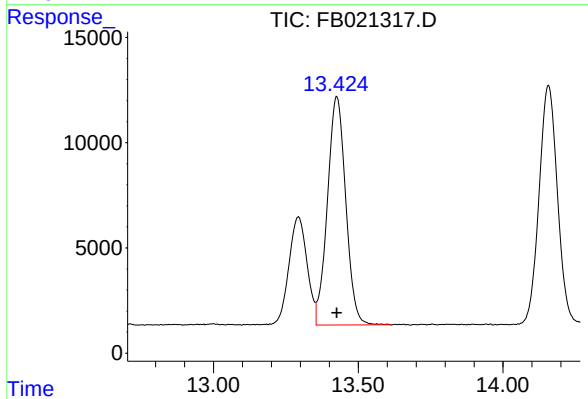


#8 m-Xylene

R.T.: 13.426 min
Delta R.T.: 0.000 min
Response: 478904
Conc: 19.19 ng/ml

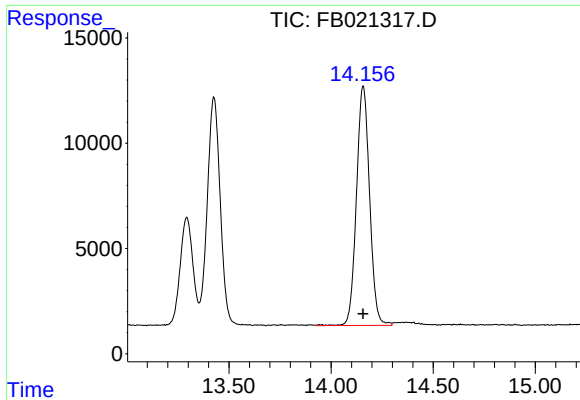

#9 O-Xylene

R.T.: 14.157 min
Delta R.T.: 0.000 min
Response: 507862
Conc: 19.47 ng/ml

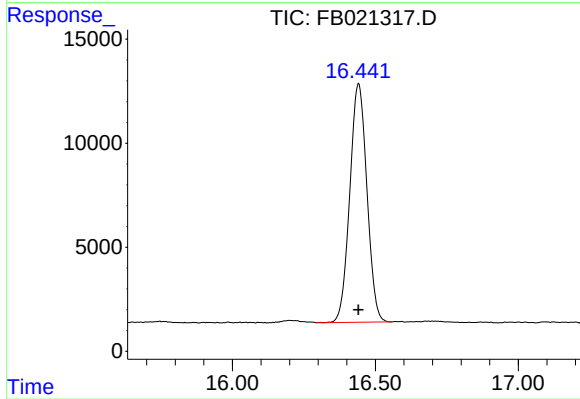

#10 1,2,4-Trimethylbenzene

R.T.: 16.442 min
Delta R.T.: 0.000 min
Response: 477458
Conc: 17.78 ng/ml