

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB060623\  
 Data File : FB029994.D  
 Signal(s) : FID2B.CH  
 Acq On : 7 Jun 2023 00:05  
 Operator : YP/AJ  
 Sample : 03044-16MS 50X  
 Misc : 5.09G/5.00 ML MEOH  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Jun 07 01:42:38 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB060323.M  
 Quant Title :  
 QLast Update : Mon Jun 05 04:33:00 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

|                             | Compound               | R.T.   | Response | Conc Units   |
|-----------------------------|------------------------|--------|----------|--------------|
| -----                       |                        |        |          |              |
| System Monitoring Compounds |                        |        |          |              |
| 5) s                        | AAA-TFT                | 8.788  | 215992   | 15.525 ng/ml |
| Target Compounds            |                        |        |          |              |
| 1) t                        | 2-Methylpentane        | 4.702  | 375452   | 19.872 ng/ml |
| 2) t                        | 2,2,4-Trimethylpentane | 7.413  | 383974   | 20.349 ng/ml |
| 3) t                        | n-Heptane              | 7.745  | 139915   | 7.228 ng/ml  |
| 4) t                        | Benzene                | 7.882  | 172451   | 7.704 ng/ml  |
| 6) t                        | Toluene                | 10.616 | 501807   | 23.121 ng/ml |
| 7) t                        | Ethylbenzene           | 13.053 | 158388   | 7.833 ng/ml  |
| 8) t                        | m-Xylene               | 13.185 | 304977   | 15.165 ng/ml |
| 9) t                        | O-Xylene               | 13.912 | 291938   | 14.978 ng/ml |
| 10) t                       | 1,2,4-Trimethylbenzene | 16.187 | 272305   | 14.538 ng/ml |
| -----                       |                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB060623\  
Data File : FB029994.D  
Signal(s) : FID2B.CH  
Acq On : 7 Jun 2023 00:05  
Operator : YP/AJ  
Sample : 03044-16MS 50X  
Misc : 5.09G/5.00 ML MEOH  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Jun 07 01:42:38 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB060323.M  
Quant Title :  
QLast Update : Mon Jun 05 04:33:00 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

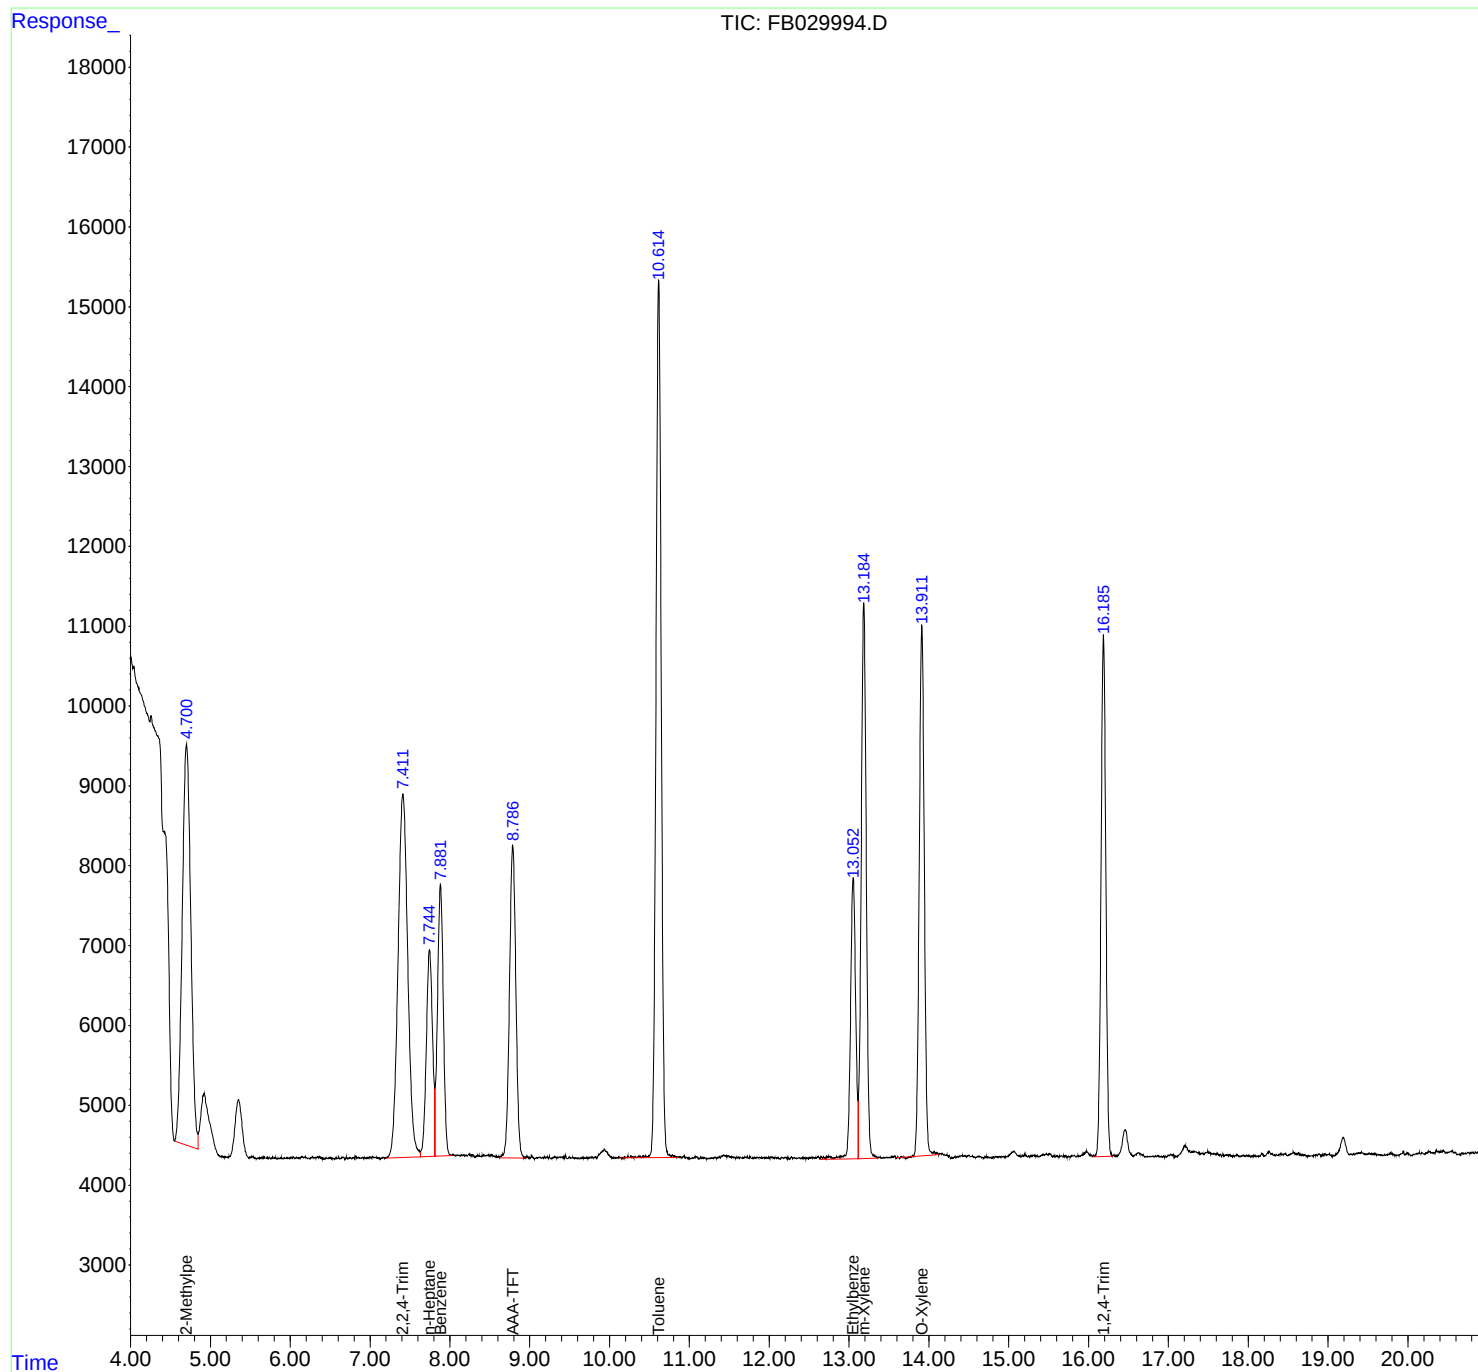

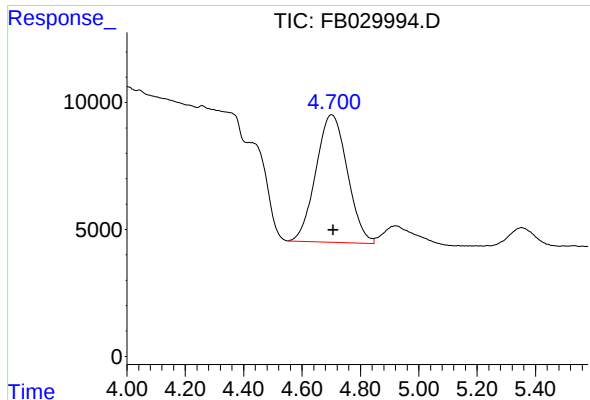


#1 2-Methylpentane

R.T.: 4.702 min  
Delta R.T.: -0.006 min  
Response: 375452  
Conc: 19.87 ng/ml


Instrument : FID\_B

ClientSampleId :

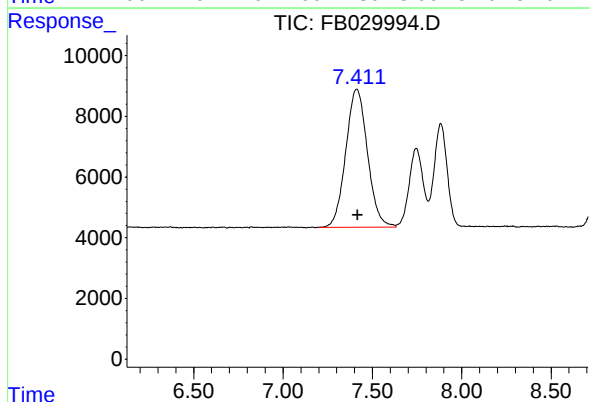


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min  
Delta R.T.: -0.006 min  
Response: 383974  
Conc: 20.35 ng/ml

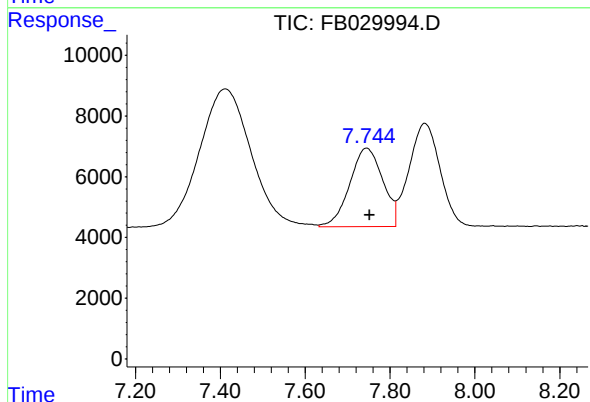


#3 n-Heptane

R.T.: 7.745 min  
Delta R.T.: -0.007 min  
Response: 139915  
Conc: 7.23 ng/ml

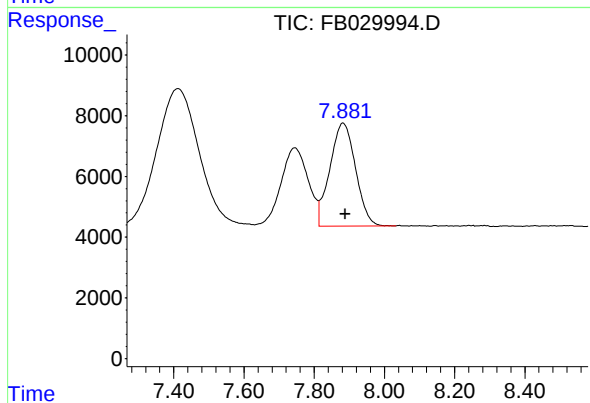

#4 Benzene


R.T.: 7.882 min  
Delta R.T.: -0.006 min  
Response: 172451  
Conc: 7.70 ng/ml

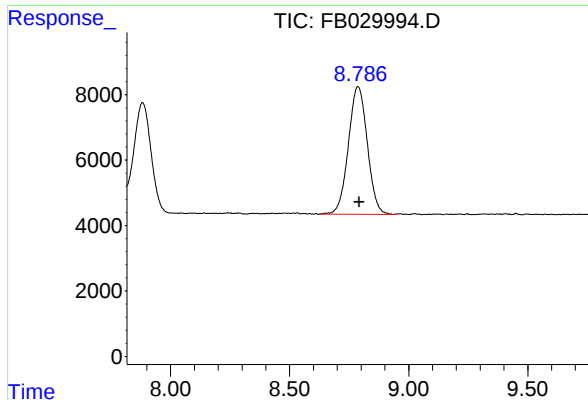

#5 AAA-TFT


R.T.: 8.788 min  
Delta R.T.: -0.005 min  
Response: 215992  
Conc: 15.52 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

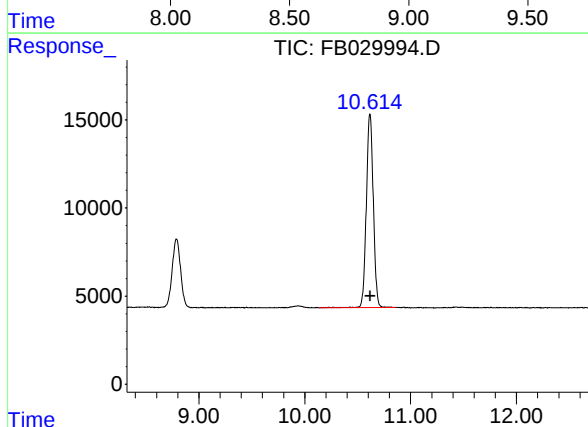


#6 Toluene

R.T.: 10.616 min  
Delta R.T.: -0.004 min  
Response: 501807  
Conc: 23.12 ng/ml

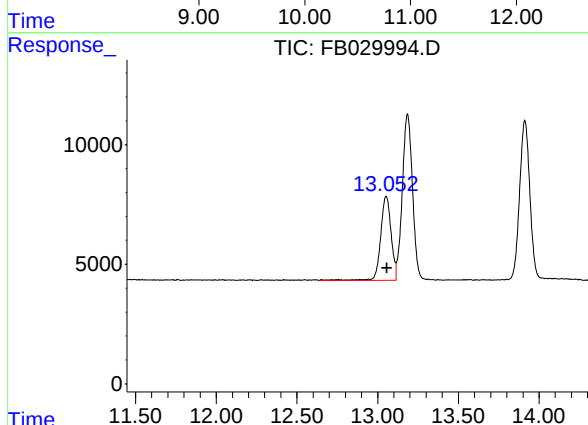


#7 Ethylbenzene

R.T.: 13.053 min  
Delta R.T.: -0.004 min  
Response: 158388  
Conc: 7.83 ng/ml

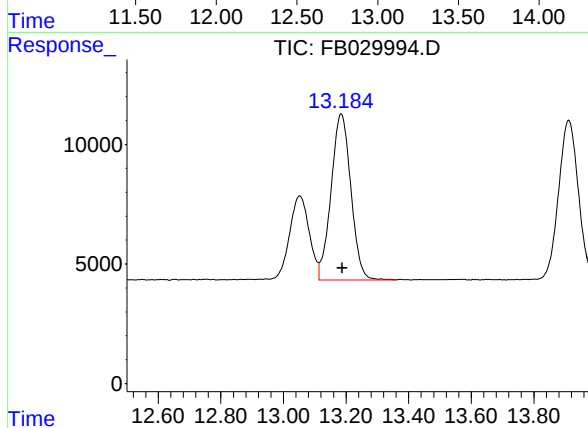

#8 m-Xylene


R.T.: 13.185 min  
Delta R.T.: -0.004 min  
Response: 304977  
Conc: 15.17 ng/ml

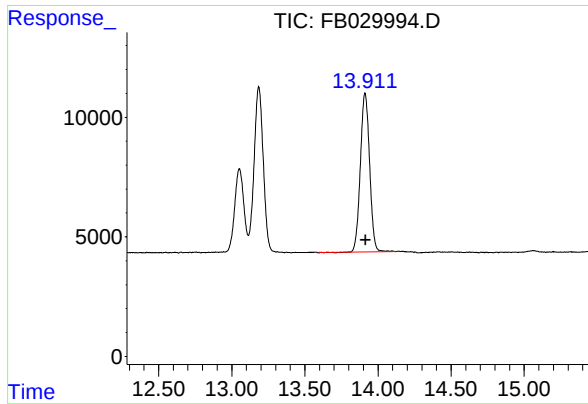

#9 O-Xylene

R.T.: 13.912 min  
Delta R.T.: -0.004 min  
Response: 291938  
Conc: 14.98 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

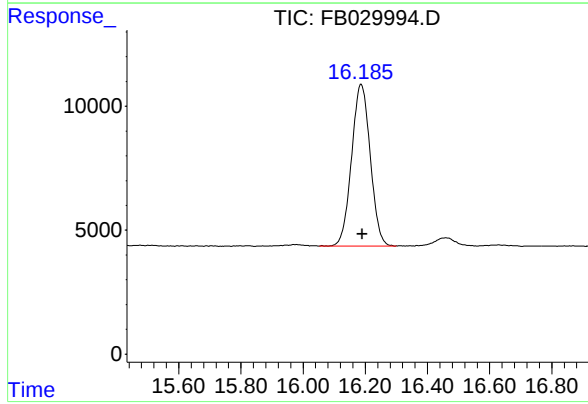

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min  
Delta R.T.: -0.003 min  
Response: 272305  
Conc: 14.54 ng/ml