

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060719\
 Data File : FB021337.D
 Signal(s) : FID2B.CH
 Acq On : 7 Jun 2019 13:27
 Operator : MJ/SJ
 Sample : K3158-01MSD
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 07 21:20:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.996	263662	17.883 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.857	831301	22.113 ng/ml
2) t 2,2,4-Trimethylpentane	7.612	691564	20.251 ng/ml
3) t n-Heptane	7.952	168445	5.167 ng/ml
4) t Benzene	8.088	296458	8.589 ng/ml
6) t Toluene	10.840	597511	25.209 ng/ml
7) t Ethylbenzene	13.291	186832	7.996 ng/ml
8) t m-Xylene	13.424	369857	14.818 ng/ml
9) t O-Xylene	14.155	405153	15.531 ng/ml
10) t 1,2,4-Trimethylbenzene	16.440	298112	11.101 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060719\
Data File : FB021337.D
Signal(s) : FID2B.CH
Acq On : 7 Jun 2019 13:27
Operator : MJ/SJ
Sample : K3158-01MSD
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 07 21:20:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

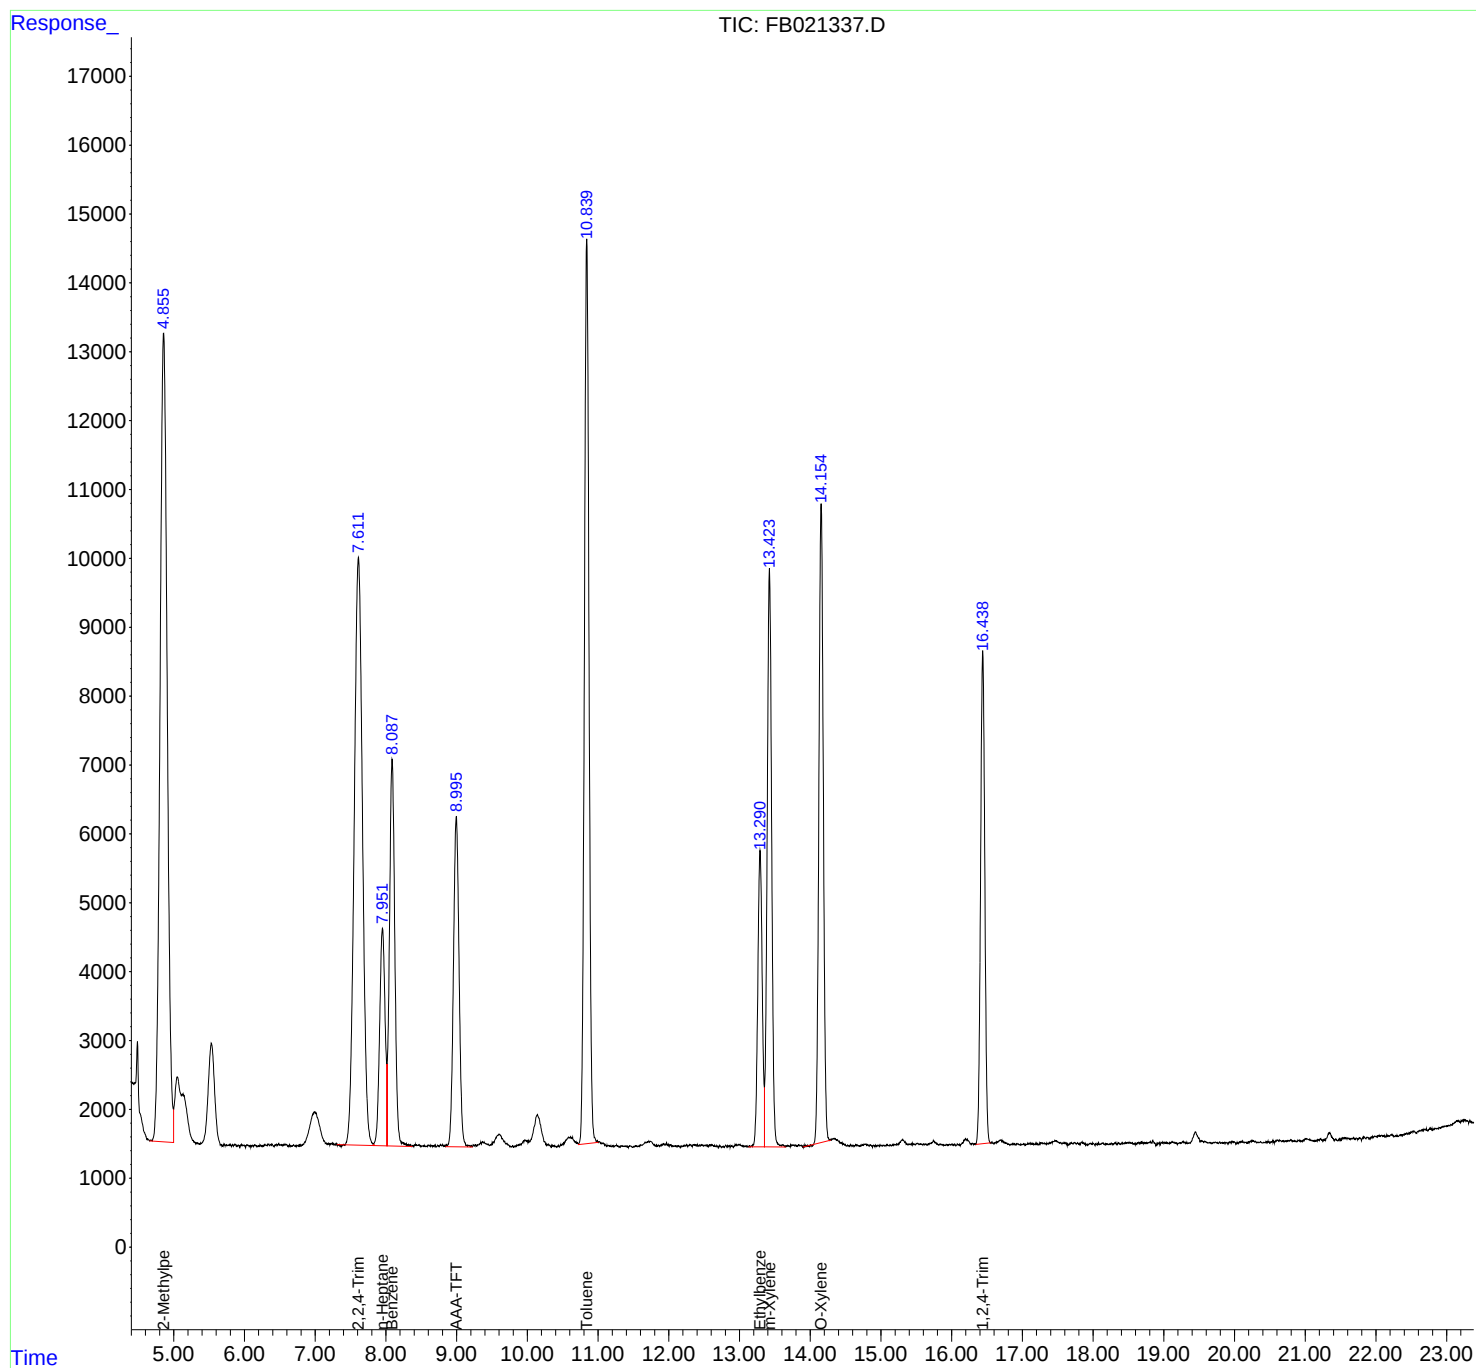

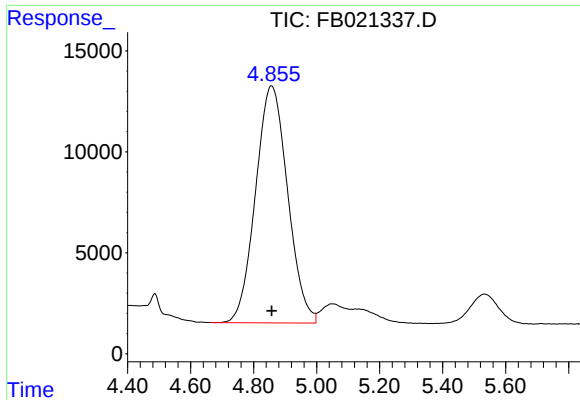


#1 2-Methylpentane

R.T.: 4.857 min
Delta R.T.: 0.000 min
Response: 831301
Conc: 22.11 ng/ml

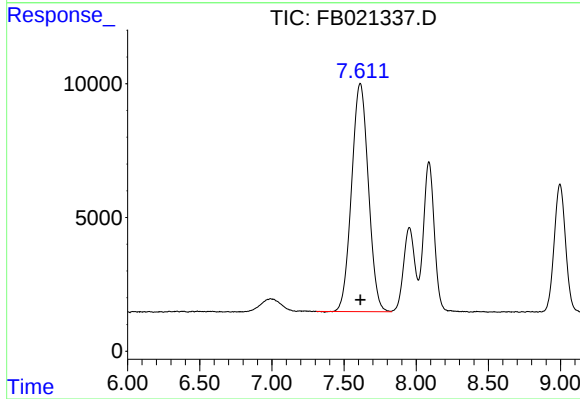


#2 2,2,4-Trimethylpentane

R.T.: 7.612 min
Delta R.T.: -0.002 min
Response: 691564
Conc: 20.25 ng/ml

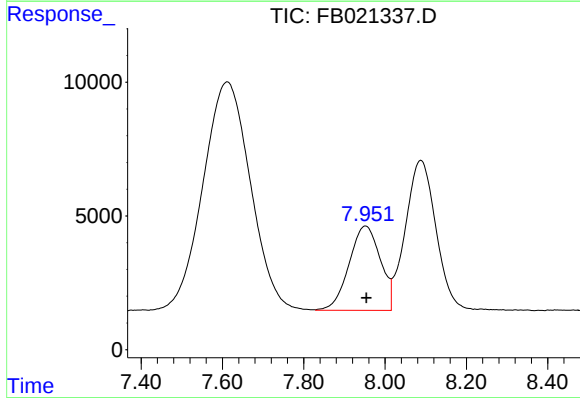


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: -0.002 min
Response: 168445
Conc: 5.17 ng/ml

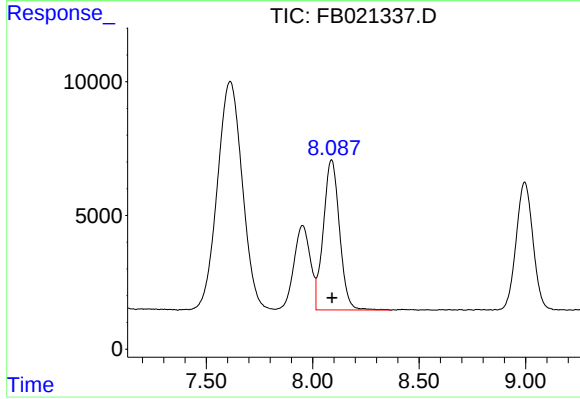


#4 Benzene

R.T.: 8.088 min
Delta R.T.: -0.002 min
Response: 296458
Conc: 8.59 ng/ml

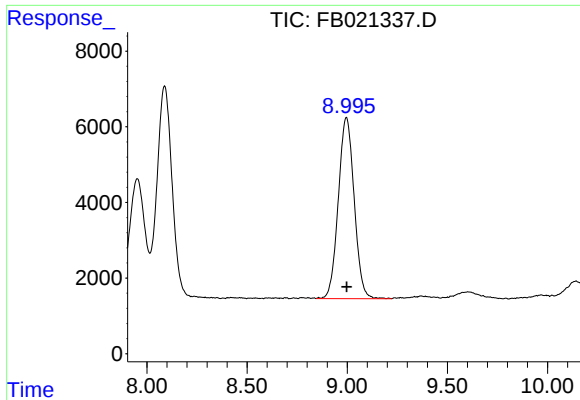


#5 AAA-TFT

R.T.: 8.996 min
 Delta R.T.: -0.002 min
 Response: 263662
 Conc: 17.88 ng/ml

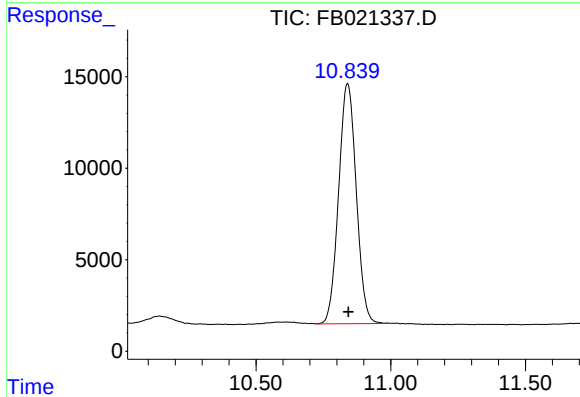


#6 Toluene

R.T.: 10.840 min
 Delta R.T.: -0.002 min
 Response: 597511
 Conc: 25.21 ng/ml

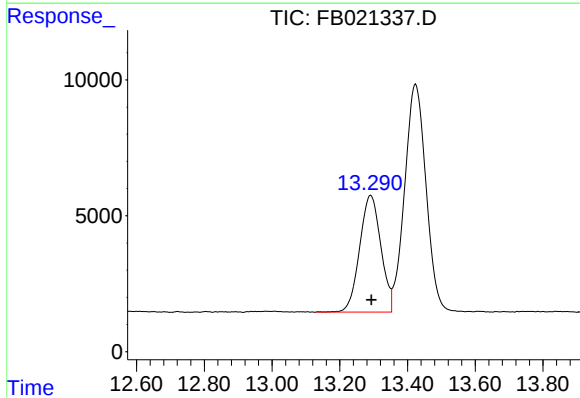


#7 Ethylbenzene

R.T.: 13.291 min
 Delta R.T.: -0.002 min
 Response: 186832
 Conc: 8.00 ng/ml

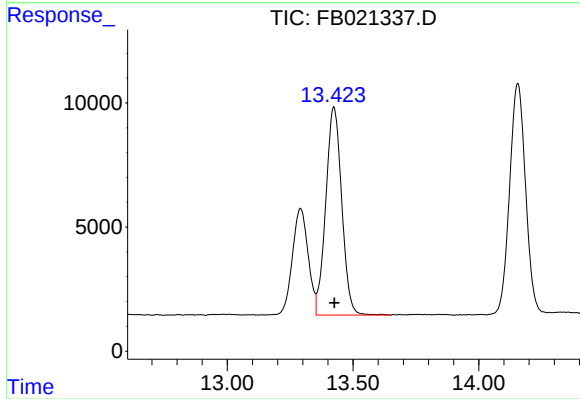


#8 m-Xylene

R.T.: 13.424 min
 Delta R.T.: -0.002 min
 Response: 369857
 Conc: 14.82 ng/ml

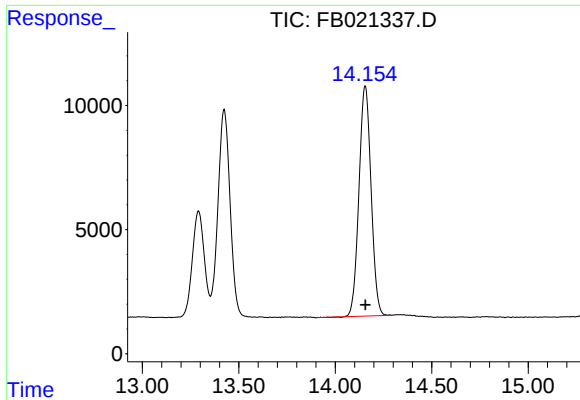

#9 O-Xylene

R.T.: 14.155 min
Delta R.T.: -0.001 min
Response: 405153
Conc: 15.53 ng/ml

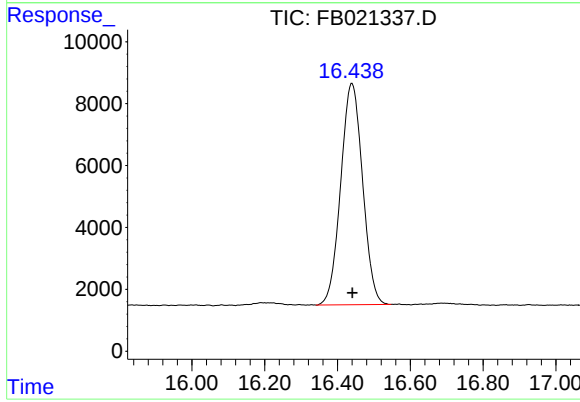

#10 1,2,4-Trimethylbenzene

R.T.: 16.440 min
Delta R.T.: 0.000 min
Response: 298112
Conc: 11.10 ng/ml