

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060719\
 Data File : FB021330.D
 Signal(s) : FID2B.CH
 Acq On : 7 Jun 2019 9:31
 Operator : MJ/SJ
 Sample : BSF0607S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 07 21:19:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.995	321994	21.839 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.856	1068225	28.415 ng/ml
2) t 2,2,4-Trimethylpentane	7.610	1043043	30.543 ng/ml
3) t n-Heptane	7.951	328264	10.069 ng/ml
4) t Benzene	8.087	333262	9.655 ng/ml
6) t Toluene	10.839	727496	30.693 ng/ml
7) t Ethylbenzene	13.289	239803	10.263 ng/ml
8) t m-Xylene	13.423	514643	20.619 ng/ml
9) t O-Xylene	14.153	534473	20.488 ng/ml
10) t 1,2,4-Trimethylbenzene	16.439	553848	20.623 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060719\
Data File : FB021330.D
Signal(s) : FID2B.CH
Acq On : 7 Jun 2019 9:31
Operator : MJ/SJ
Sample : BSF0607S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 07 21:19:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

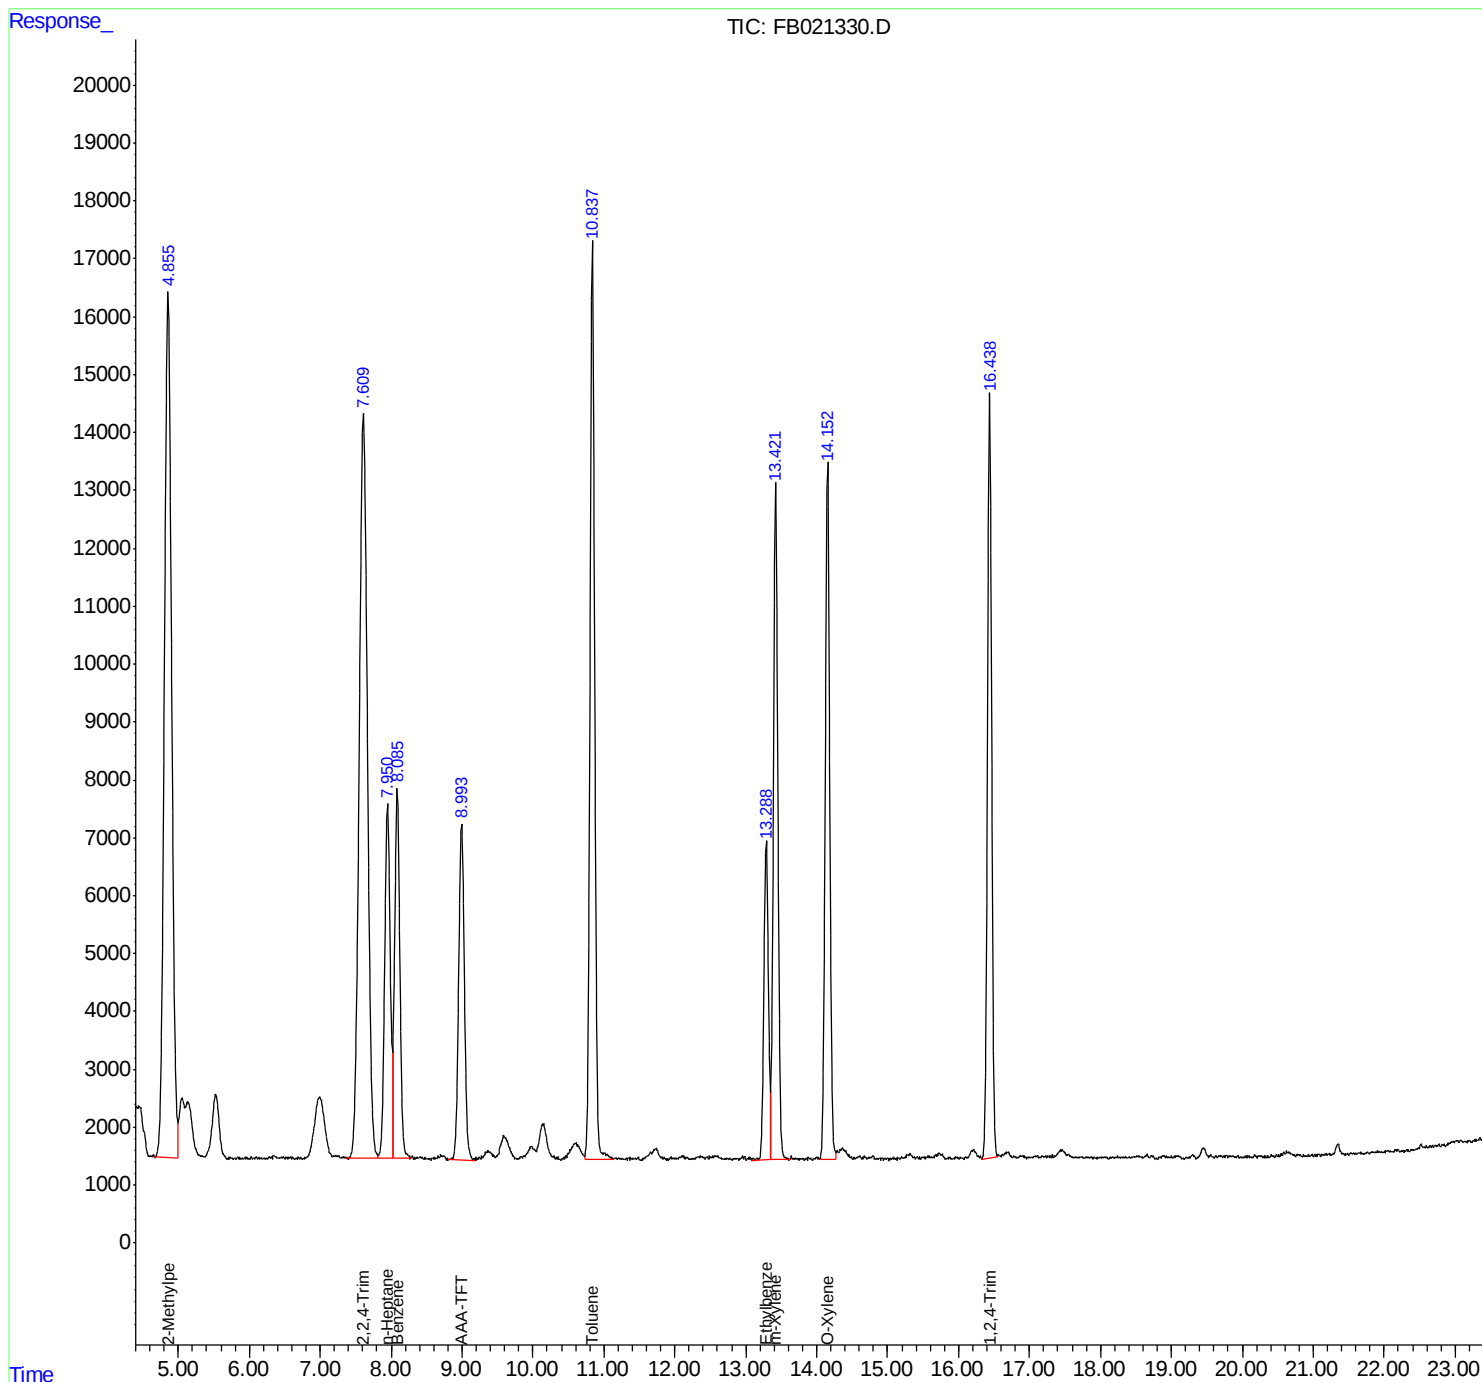

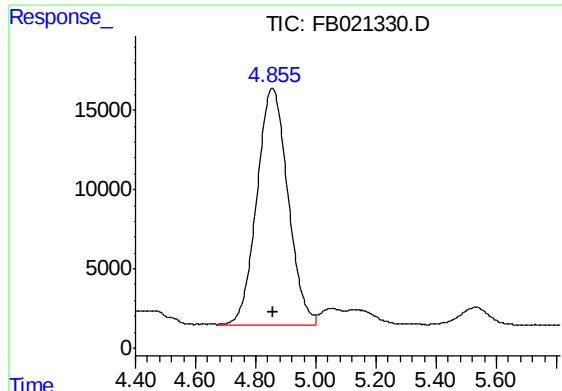


#1 2-Methylpentane

R.T.: 4.856 min
Delta R.T.: -0.002 min
Response: 1068225
Conc: 28.42 ng/ml

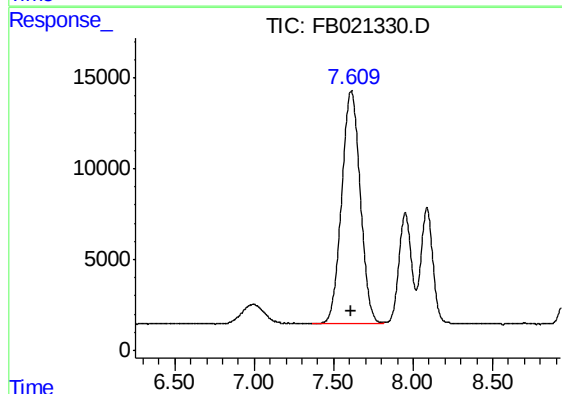


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: -0.004 min
Response: 1043043
Conc: 30.54 ng/ml

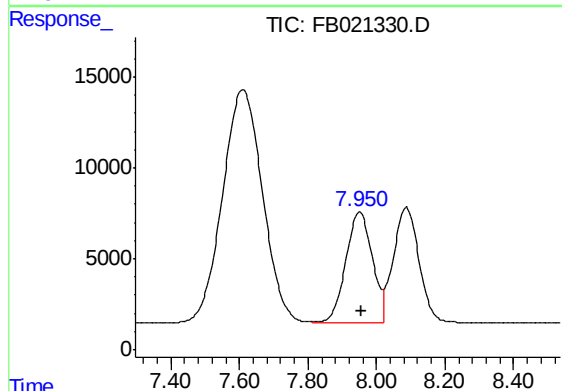


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: -0.003 min
Response: 328264
Conc: 10.07 ng/ml

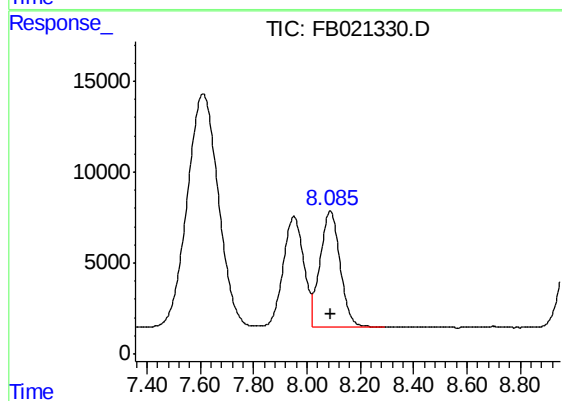


#4 Benzene

R.T.: 8.087 min
Delta R.T.: -0.003 min
Response: 333262
Conc: 9.66 ng/ml

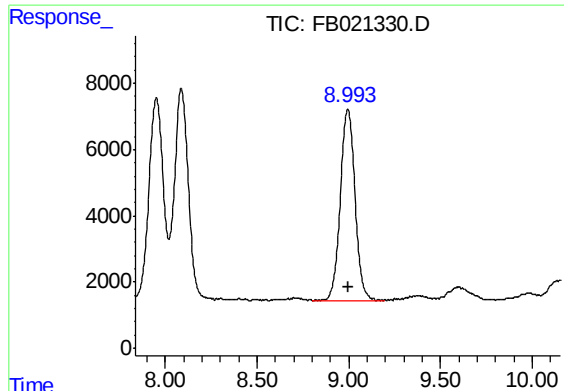


#5 AAA-TFT

R.T.: 8.995 min
Delta R.T.: -0.004 min
Response: 321994
Conc: 21.84 ng/ml

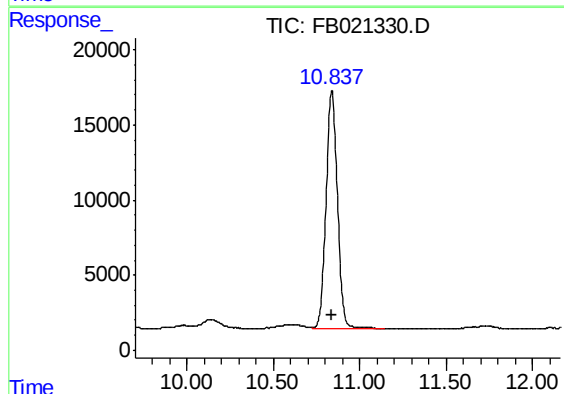


#6 Toluene

R.T.: 10.839 min
Delta R.T.: -0.004 min
Response: 727496
Conc: 30.69 ng/ml

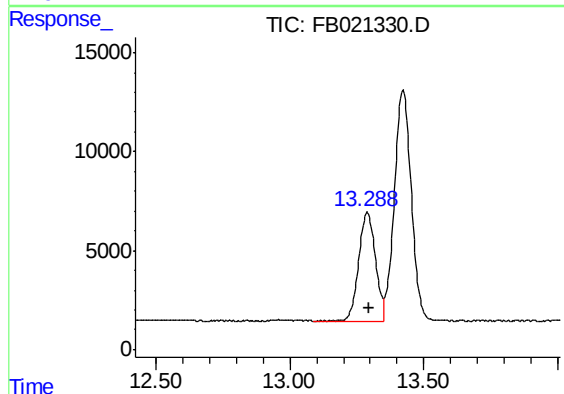


#7 Ethylbenzene

R.T.: 13.289 min
Delta R.T.: -0.004 min
Response: 239803
Conc: 10.26 ng/ml

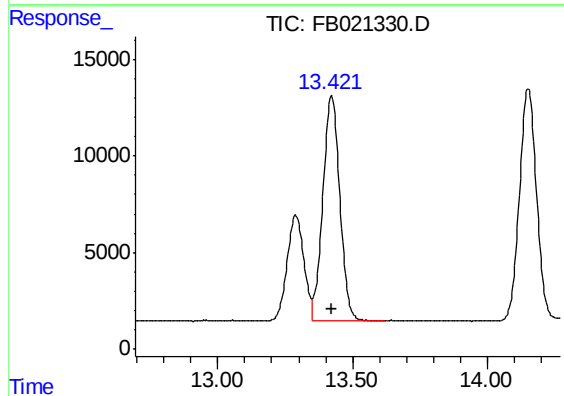


#8 m-Xylene

R.T.: 13.423 min
Delta R.T.: -0.003 min
Response: 514643
Conc: 20.62 ng/ml

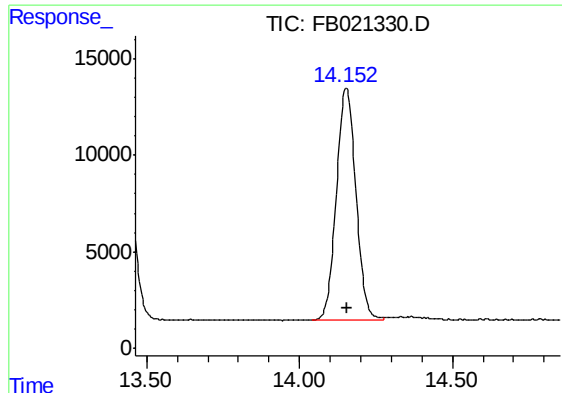

#9 O-Xylene

R.T.: 14.153 min
Delta R.T.: -0.003 min
Response: 534473
Conc: 20.49 ng/ml

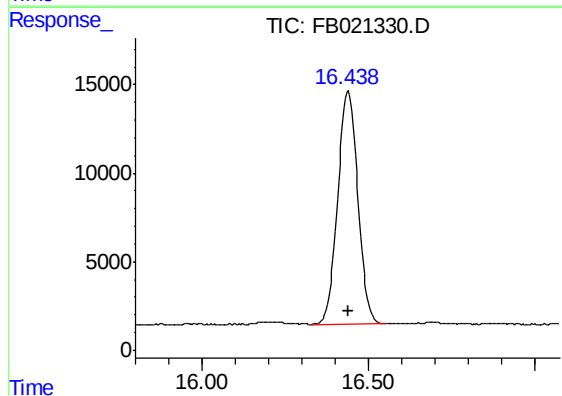

#10 1,2,4-Trimethylbenzene

R.T.: 16.439 min
Delta R.T.: -0.002 min
Response: 553848
Conc: 20.62 ng/ml