

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060722\
Data File : FB027334.D
Signal(s) : FID2B.CH
Acq On : 7 Jun 2022 12:58
Operator : AJ/MA
Sample : VBF0607S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 08 04:30:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	250394	23.853 ng/ml
Target Compounds			
6) t Toluene	10.626	5117	0.288 ng/ml
8) t m-Xylene	13.181	6903	0.420 ng/ml
10) t 1,2,4-Trimethylbenzene	16.182	2318	0.139 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060722\
Data File : FB027334.D
Signal(s) : FID2B.CH
Acq On : 7 Jun 2022 12:58
Operator : AJ/MA
Sample : VBF0607S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 08 04:30:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

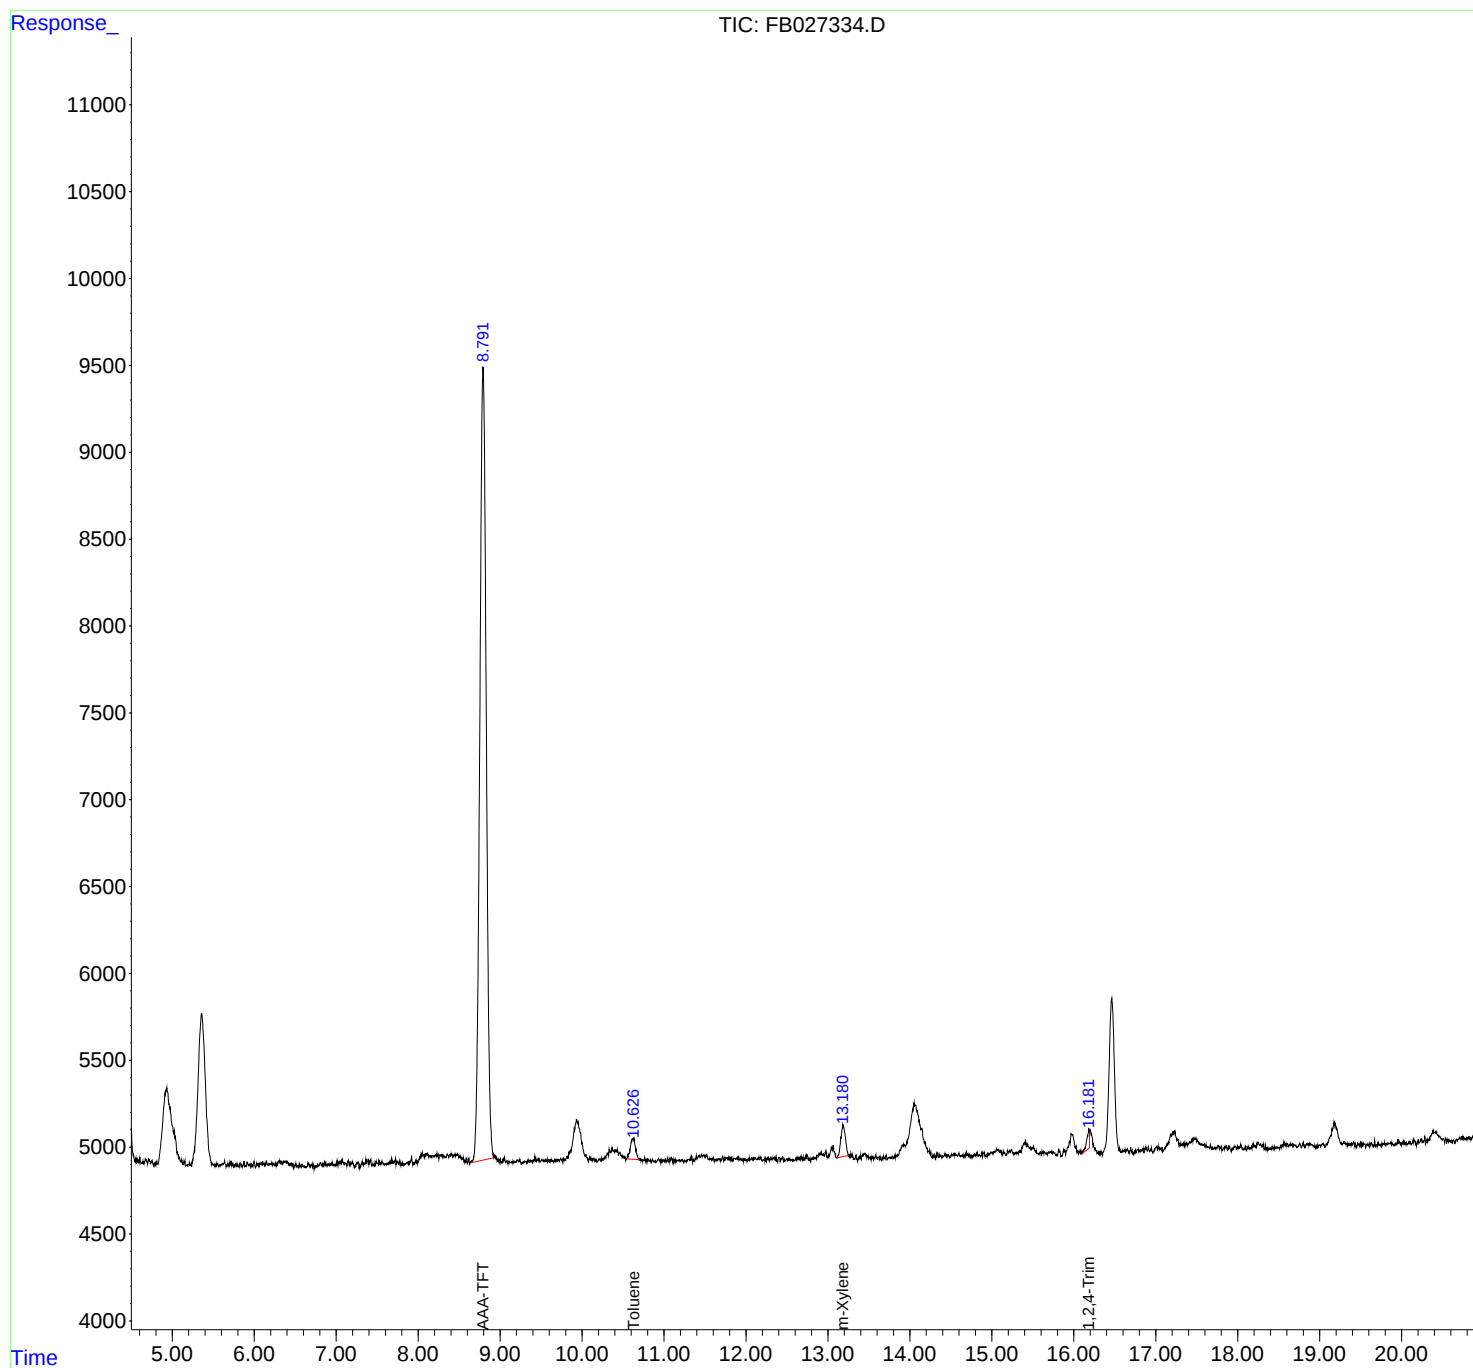


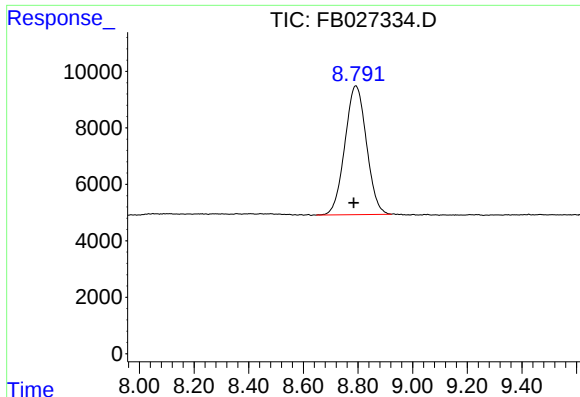

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.008 min
Response: 250394
Conc: 23.85 ng/ml

Instrument :
FID_B
ClientSampleId :

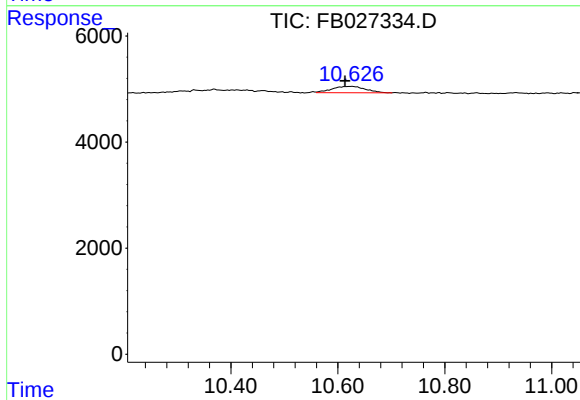


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.013 min
Response: 5117
Conc: 0.29 ng/ml

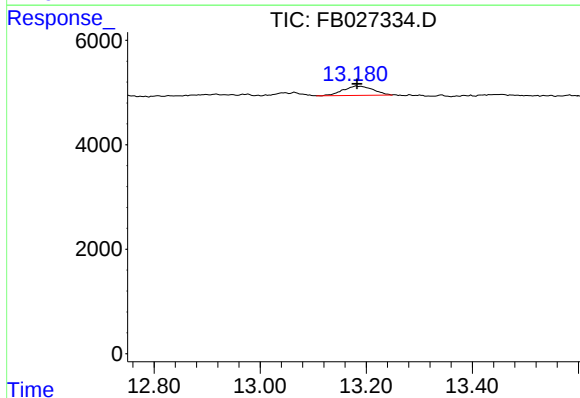

#8 m-Xylene

R.T.: 13.181 min
Delta R.T.: -0.002 min
Response: 6903
Conc: 0.42 ng/ml

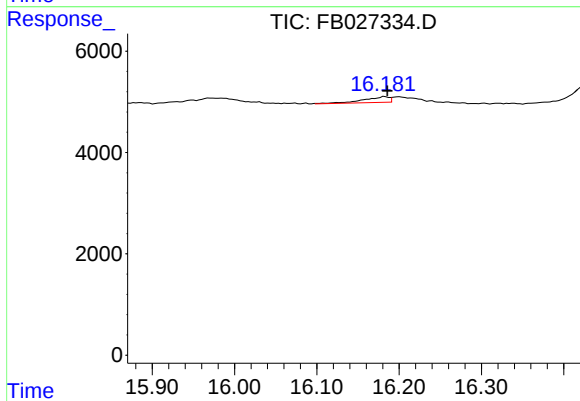

#10 1,2,4-Trimethylbenzene

R.T.: 16.182 min
Delta R.T.: -0.003 min
Response: 2318
Conc: 0.14 ng/ml