

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060722\
 Data File : FB027336.D
 Signal(s) : FID2B.CH
 Acq On : 7 Jun 2022 14:11
 Operator : AJ/MA
 Sample : BSF0607S1
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0607S1

Integration File: Calibration.e
 Quant Time: Jun 08 04:30:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
 Quant Title :
 QLast Update : Tue May 10 13:42:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	200500	19.100 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	376059	23.631 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	435952	27.021 ng/ml
3) t n-Heptane	7.750	123927	7.584 ng/ml
4) t Benzene	7.889	176783	9.533 ng/ml
6) t Toluene	10.621	518007	29.177 ng/ml
7) t Ethylbenzene	13.058	162509	9.841 ng/ml
8) t m-Xylene	13.191	320832	19.498 ng/ml
9) t O-Xylene	13.918	317072	19.330 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	320380	19.190 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060722\
Data File : FB027336.D
Signal(s) : FID2B.CH
Acq On : 7 Jun 2022 14:11
Operator : AJ/MA
Sample : BSF0607S1
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0607S1

Integration File: Calibration.e
Quant Time: Jun 08 04:30:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

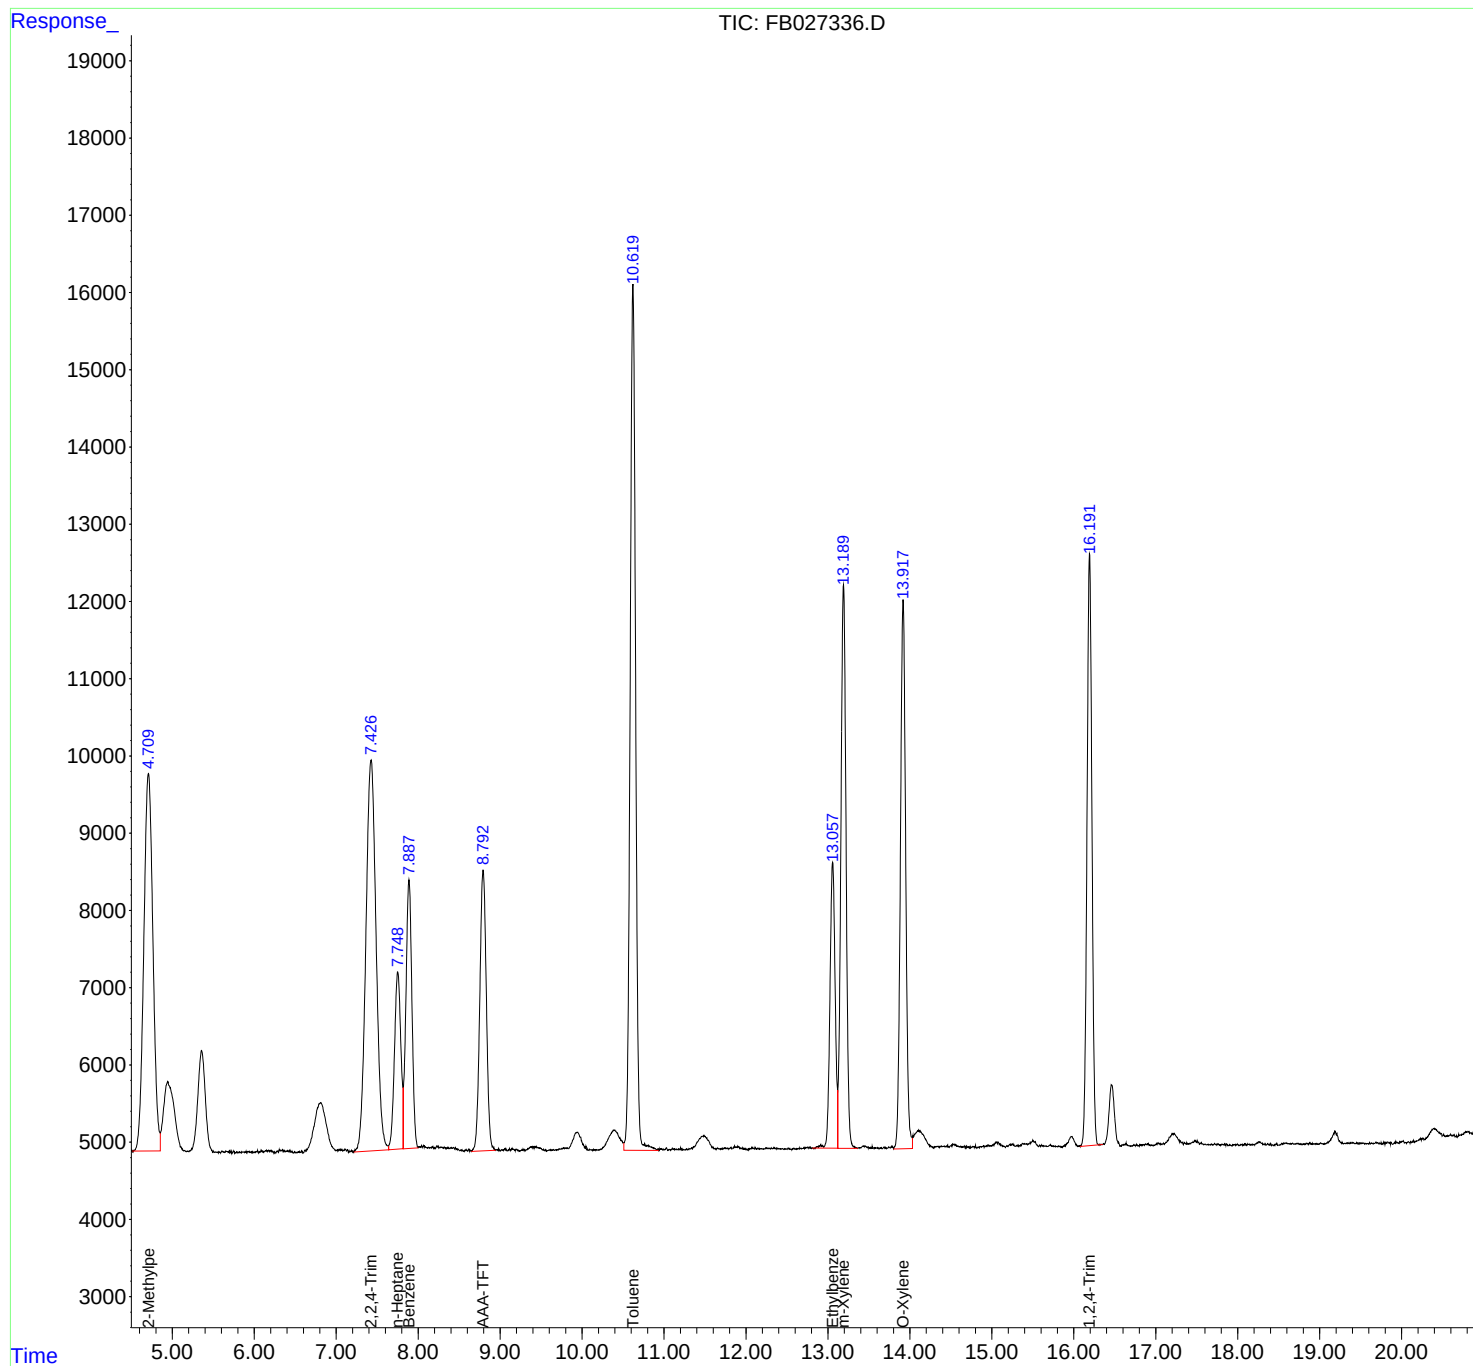


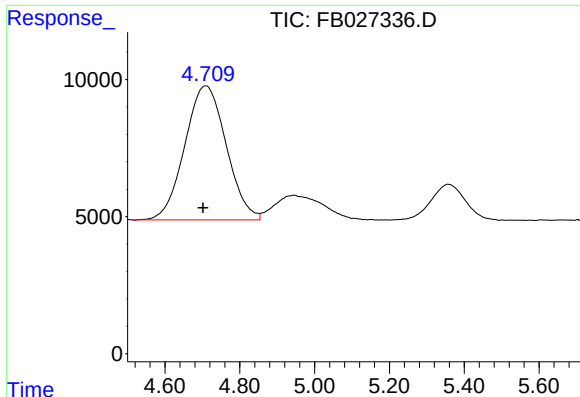

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.008 min
Response: 376059
Conc: 23.63 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0607S1

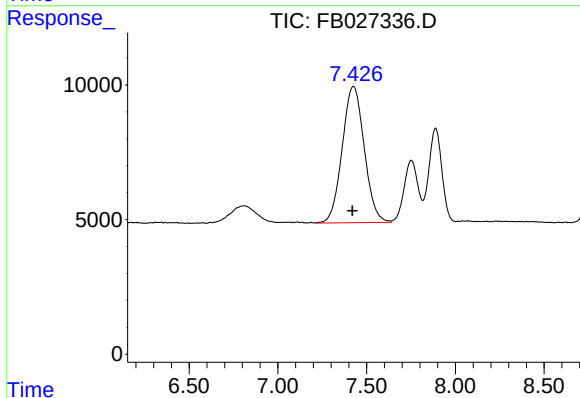


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.007 min
Response: 435952
Conc: 27.02 ng/ml

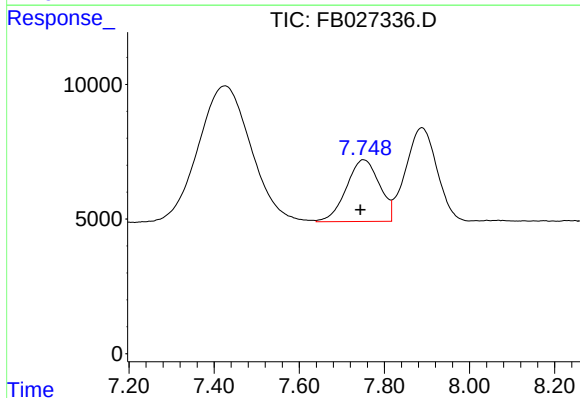


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.007 min
Response: 123927
Conc: 7.58 ng/ml

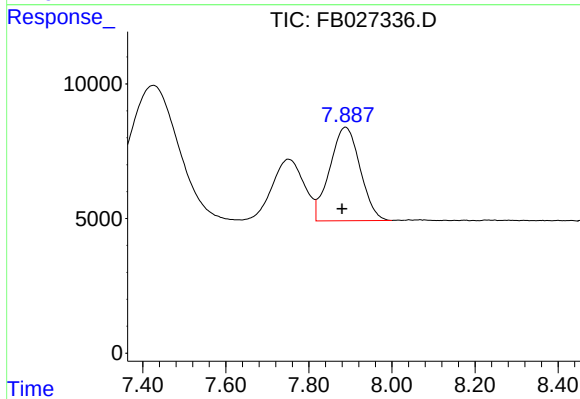

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.008 min
Response: 176783
Conc: 9.53 ng/ml

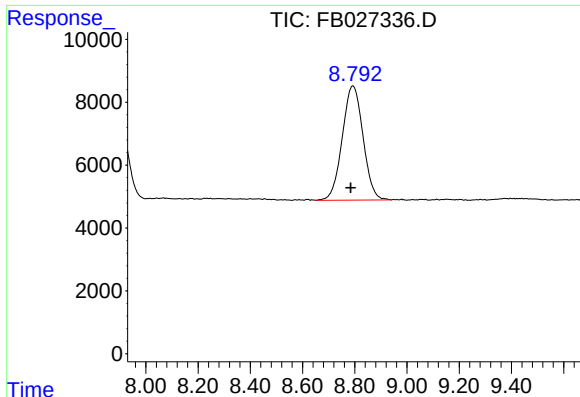

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.008 min
Response: 200500
Conc: 19.10 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0607S1

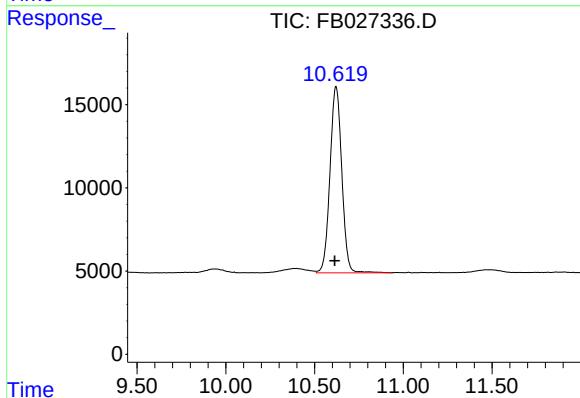


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.008 min
Response: 518007
Conc: 29.18 ng/ml

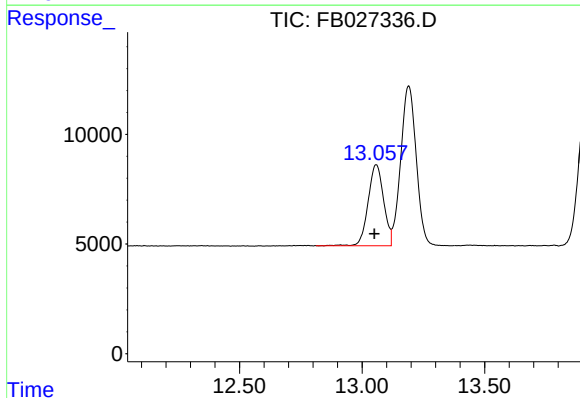


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.008 min
Response: 162509
Conc: 9.84 ng/ml

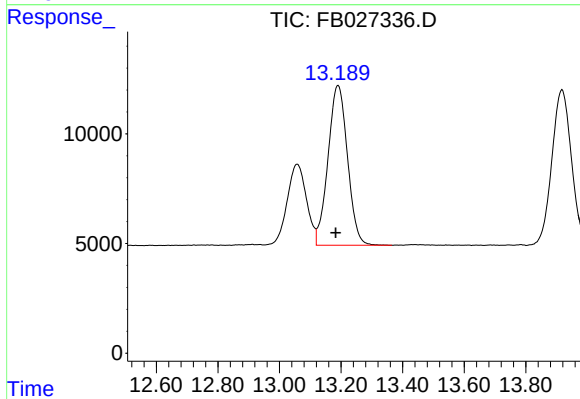

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.008 min
Response: 320832
Conc: 19.50 ng/ml

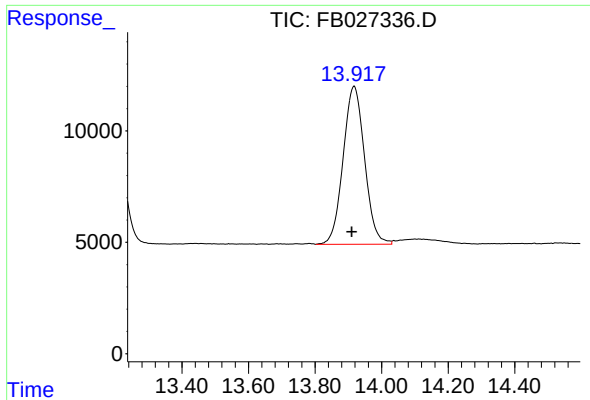

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.008 min
Response: 317072
Conc: 19.33 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0607S1

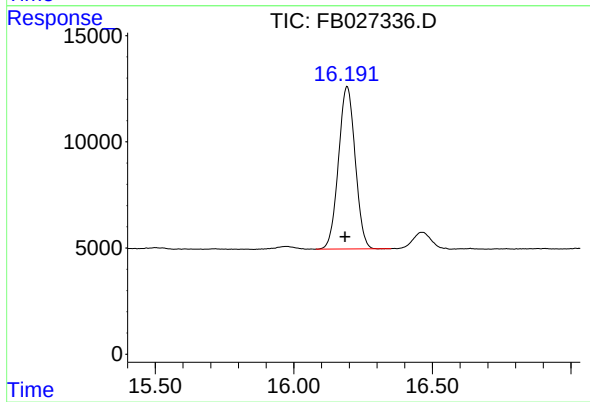

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.007 min
Response: 320380
Conc: 19.19 ng/ml