

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060722\
Data File : FB027353.D
Signal(s) : FID2B.CH
Acq On : 8 Jun 2022 1:13
Operator : AJ/MA
Sample : N3194-11
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TPH-2-TP-3

Integration File: Calibration.e
Quant Time: Jun 08 04:32:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	46006	4.383 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060722\
Data File : FB027353.D
Signal(s) : FID2B.CH
Acq On : 8 Jun 2022 1:13
Operator : AJ/MA
Sample : N3194-11
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TPH-2-TP-3

Integration File: Calibration.e
Quant Time: Jun 08 04:32:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

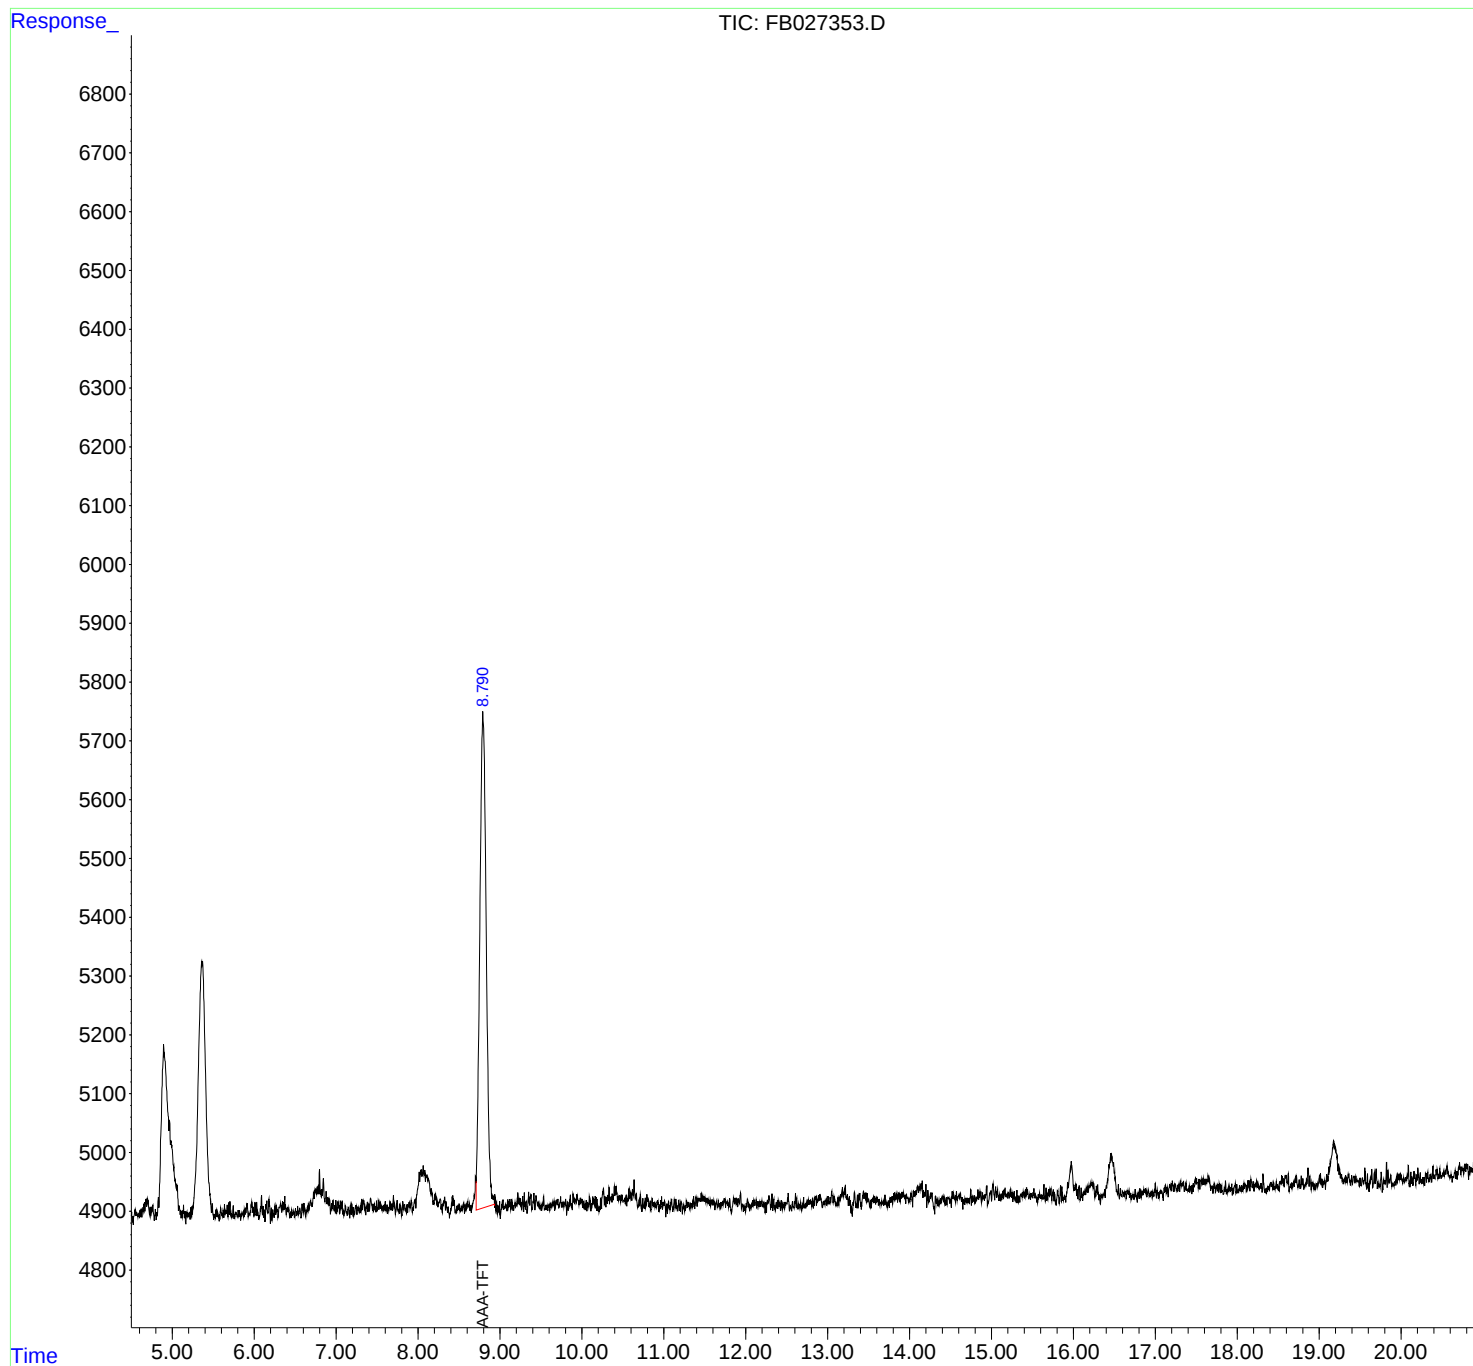

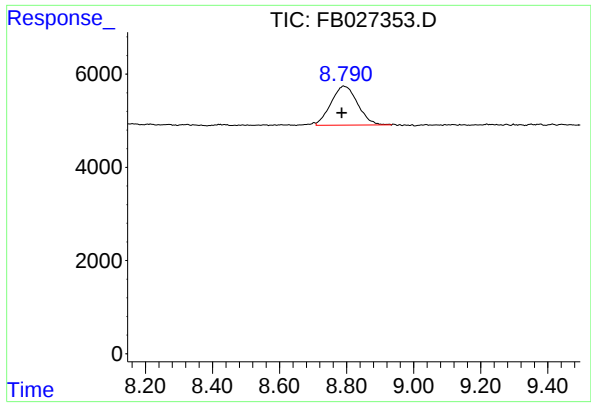

#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.006 min
Response: 46006
Conc: 4.38 ng/ml

Instrument :
FID_B
ClientSampleId :
TPH-2-TP-3