

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060722\
Data File : FB027354.D
Signal(s) : FID2B.CH
Acq On : 8 Jun 2022 1:50
Operator : AJ/MA
Sample : N3194-12
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TPH-3-TP-3

Integration File: Calibration.e
Quant Time: Jun 08 04:33:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	8748	0.833 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060722\
Data File : FB027354.D
Signal(s) : FID2B.CH
Acq On : 8 Jun 2022 1:50
Operator : AJ/MA
Sample : N3194-12
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TPH-3-TP-3

Integration File: Calibration.e
Quant Time: Jun 08 04:33:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

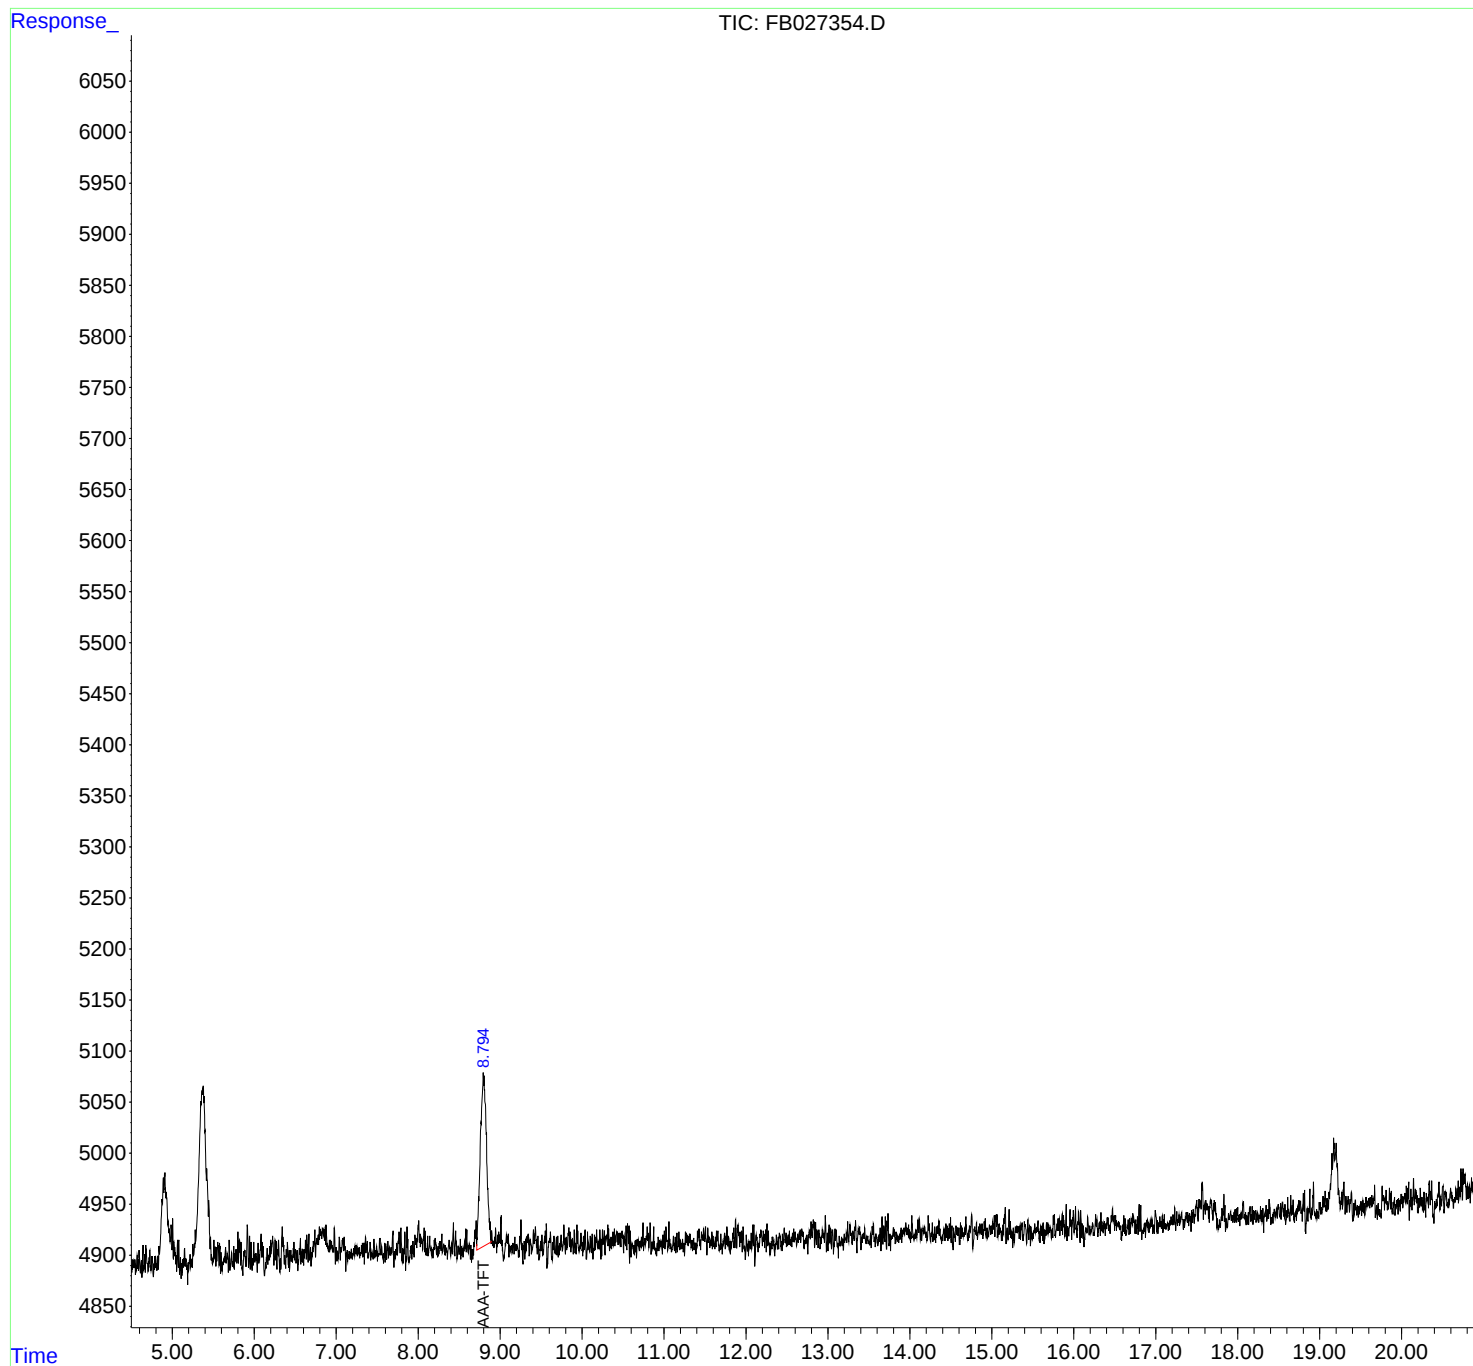

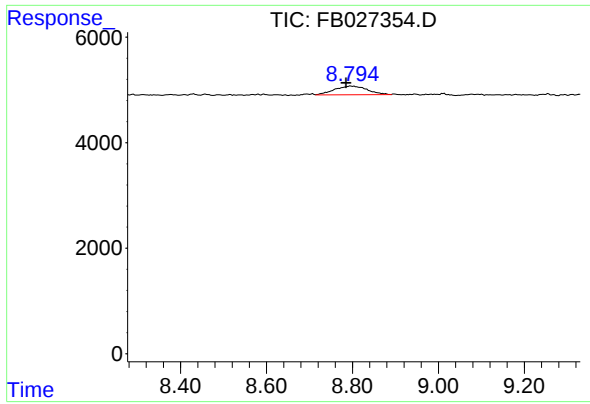

#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: 0.010 min
Response: 8748
Conc: 0.83 ng/ml

Instrument :
FID_B
ClientSampleId :
TPH-3-TP-3