

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060722\
 Data File : FB027356.D
 Signal(s) : FID2B.CH
 Acq On : 8 Jun 2022 3:03
 Operator : AJ/MA
 Sample : BSF0607S3
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0607S3

Integration File: Calibration.e
 Quant Time: Jun 08 04:33:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
 Quant Title :
 QLast Update : Tue May 10 13:42:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	203062	19.344 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	396672	24.927 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	455962	28.261 ng/ml
3) t n-Heptane	7.752	119224	7.296 ng/ml
4) t Benzene	7.889	182995	9.868 ng/ml
6) t Toluene	10.621	526845	29.674 ng/ml
7) t Ethylbenzene	13.058	168591	10.209 ng/ml
8) t m-Xylene	13.191	330416	20.081 ng/ml
9) t O-Xylene	13.918	326995	19.935 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	331253	19.841 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060722\
Data File : FB027356.D
Signal(s) : FID2B.CH
Acq On : 8 Jun 2022 3:03
Operator : AJ/MA
Sample : BSF0607S3
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0607S3

Integration File: Calibration.e
Quant Time: Jun 08 04:33:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

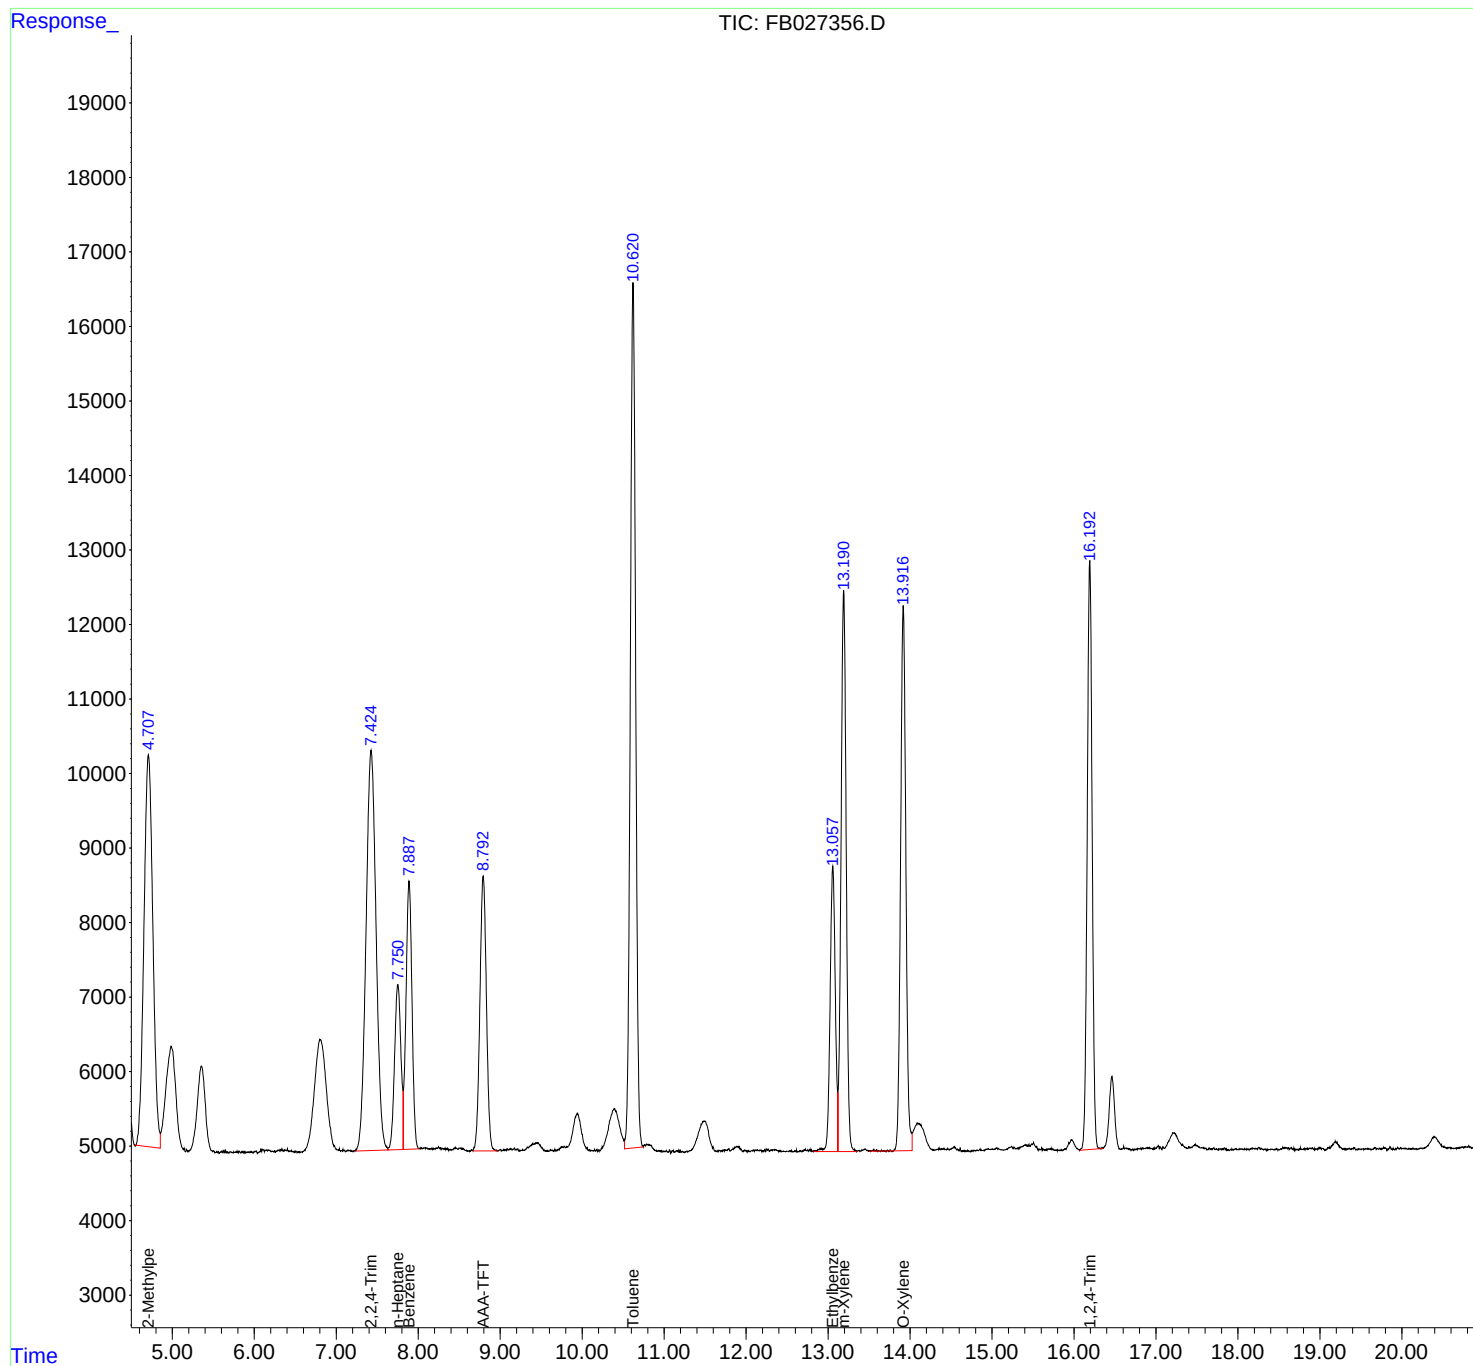


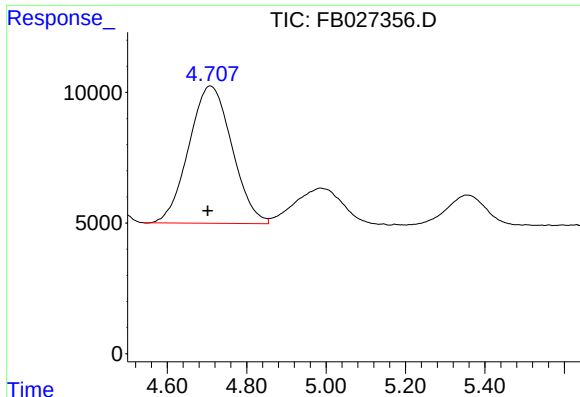

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.007 min
Response: 396672
Conc: 24.93 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0607S3

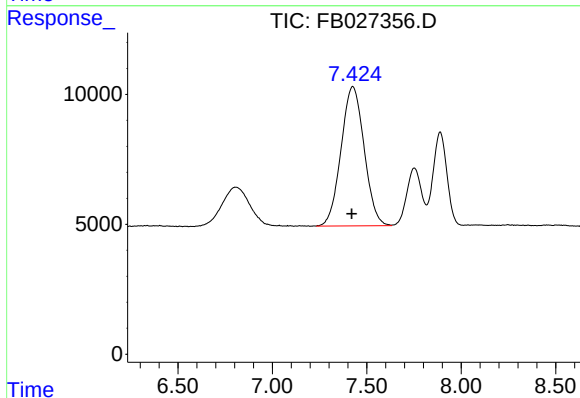


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: 0.005 min
Response: 455962
Conc: 28.26 ng/ml

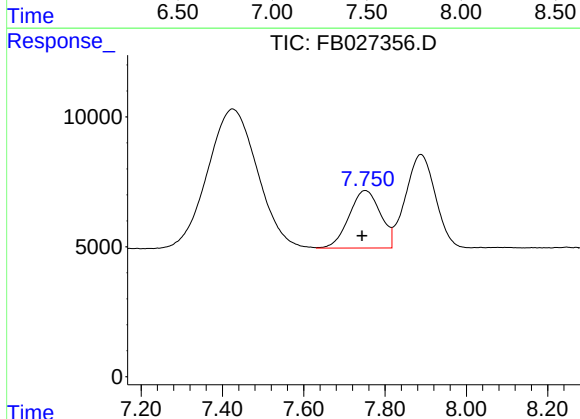


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.008 min
Response: 119224
Conc: 7.30 ng/ml

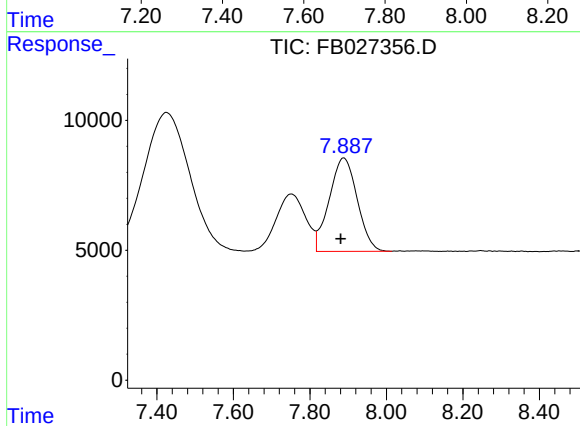

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.008 min
Response: 182995
Conc: 9.87 ng/ml

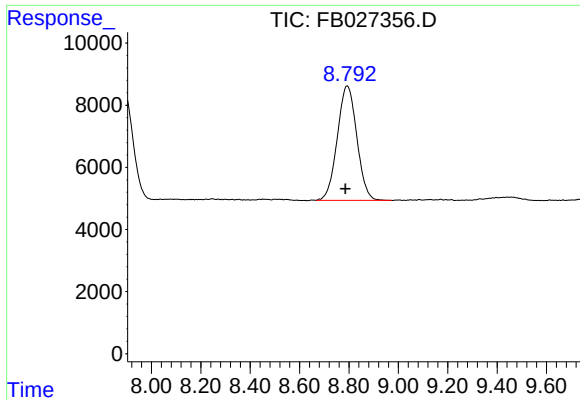

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.008 min
Response: 203062
Conc: 19.34 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0607S3

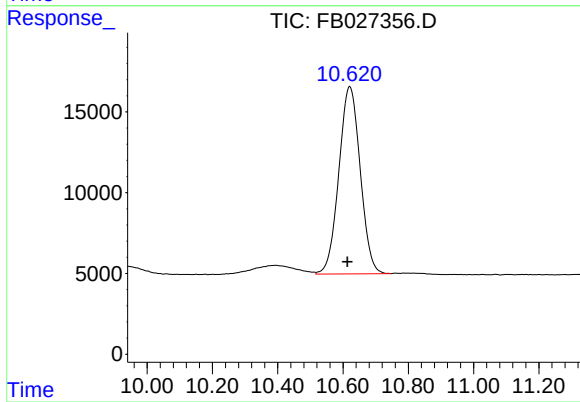


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.008 min
Response: 526845
Conc: 29.67 ng/ml

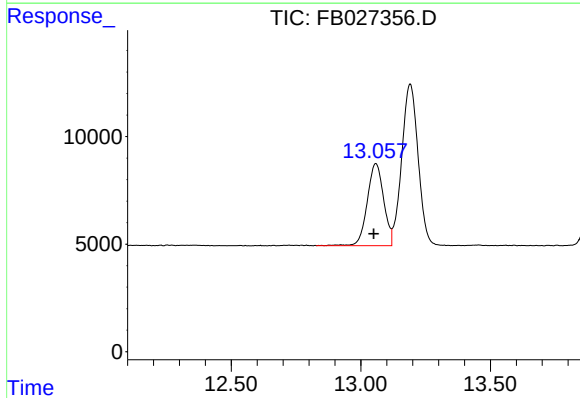


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.008 min
Response: 168591
Conc: 10.21 ng/ml

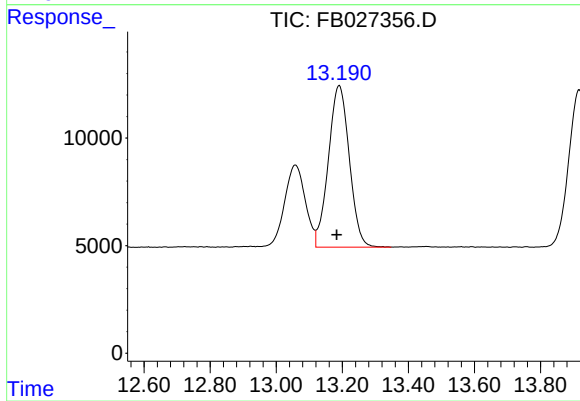

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.008 min
Response: 330416
Conc: 20.08 ng/ml

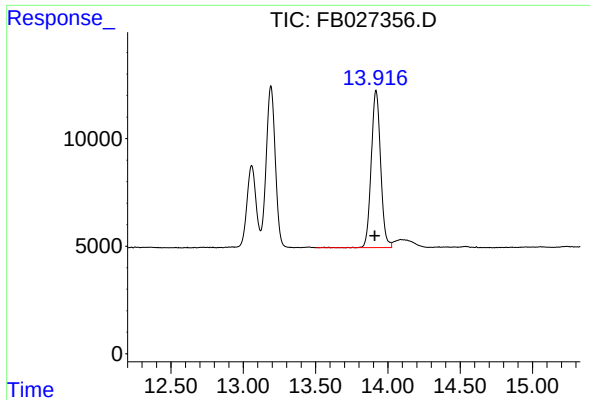

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.008 min
Response: 326995
Conc: 19.94 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0607S3

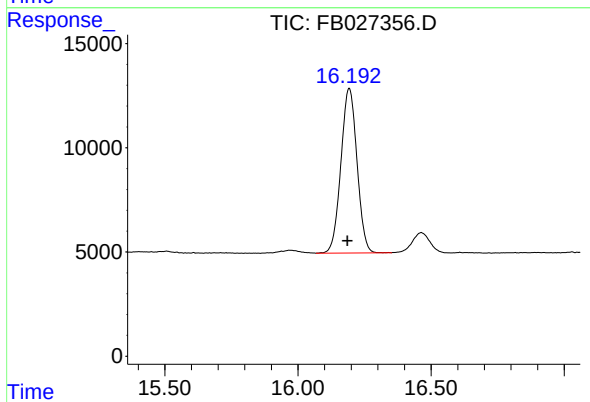

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.007 min
Response: 331253
Conc: 19.84 ng/ml