

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060723\
 Data File : FB030000.D
 Signal(s) : FID2B.CH
 Acq On : 7 Jun 2023 11:37
 Operator : YP/AJ
 Sample : BSF0607S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0607S1

Integration File: Calibration.e
 Quant Time: Jun 08 01:16:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:33:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	282130	20.279 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	578952	30.642 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	540563	28.648 ng/ml
3) t n-Heptane	7.747	207783	10.735 ng/ml
4) t Benzene	7.883	243635	10.884 ng/ml
6) t Toluene	10.616	696165	32.077 ng/ml
7) t Ethylbenzene	13.052	215847	10.675 ng/ml
8) t m-Xylene	13.184	429999	21.382 ng/ml
9) t O-Xylene	13.911	411695	21.123 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	386331	20.626 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060723\
Data File : FB030000.D
Signal(s) : FID2B.CH
Acq On : 7 Jun 2023 11:37
Operator : YP/AJ
Sample : BSF0607S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0607S1

Integration File: Calibration.e
Quant Time: Jun 08 01:16:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

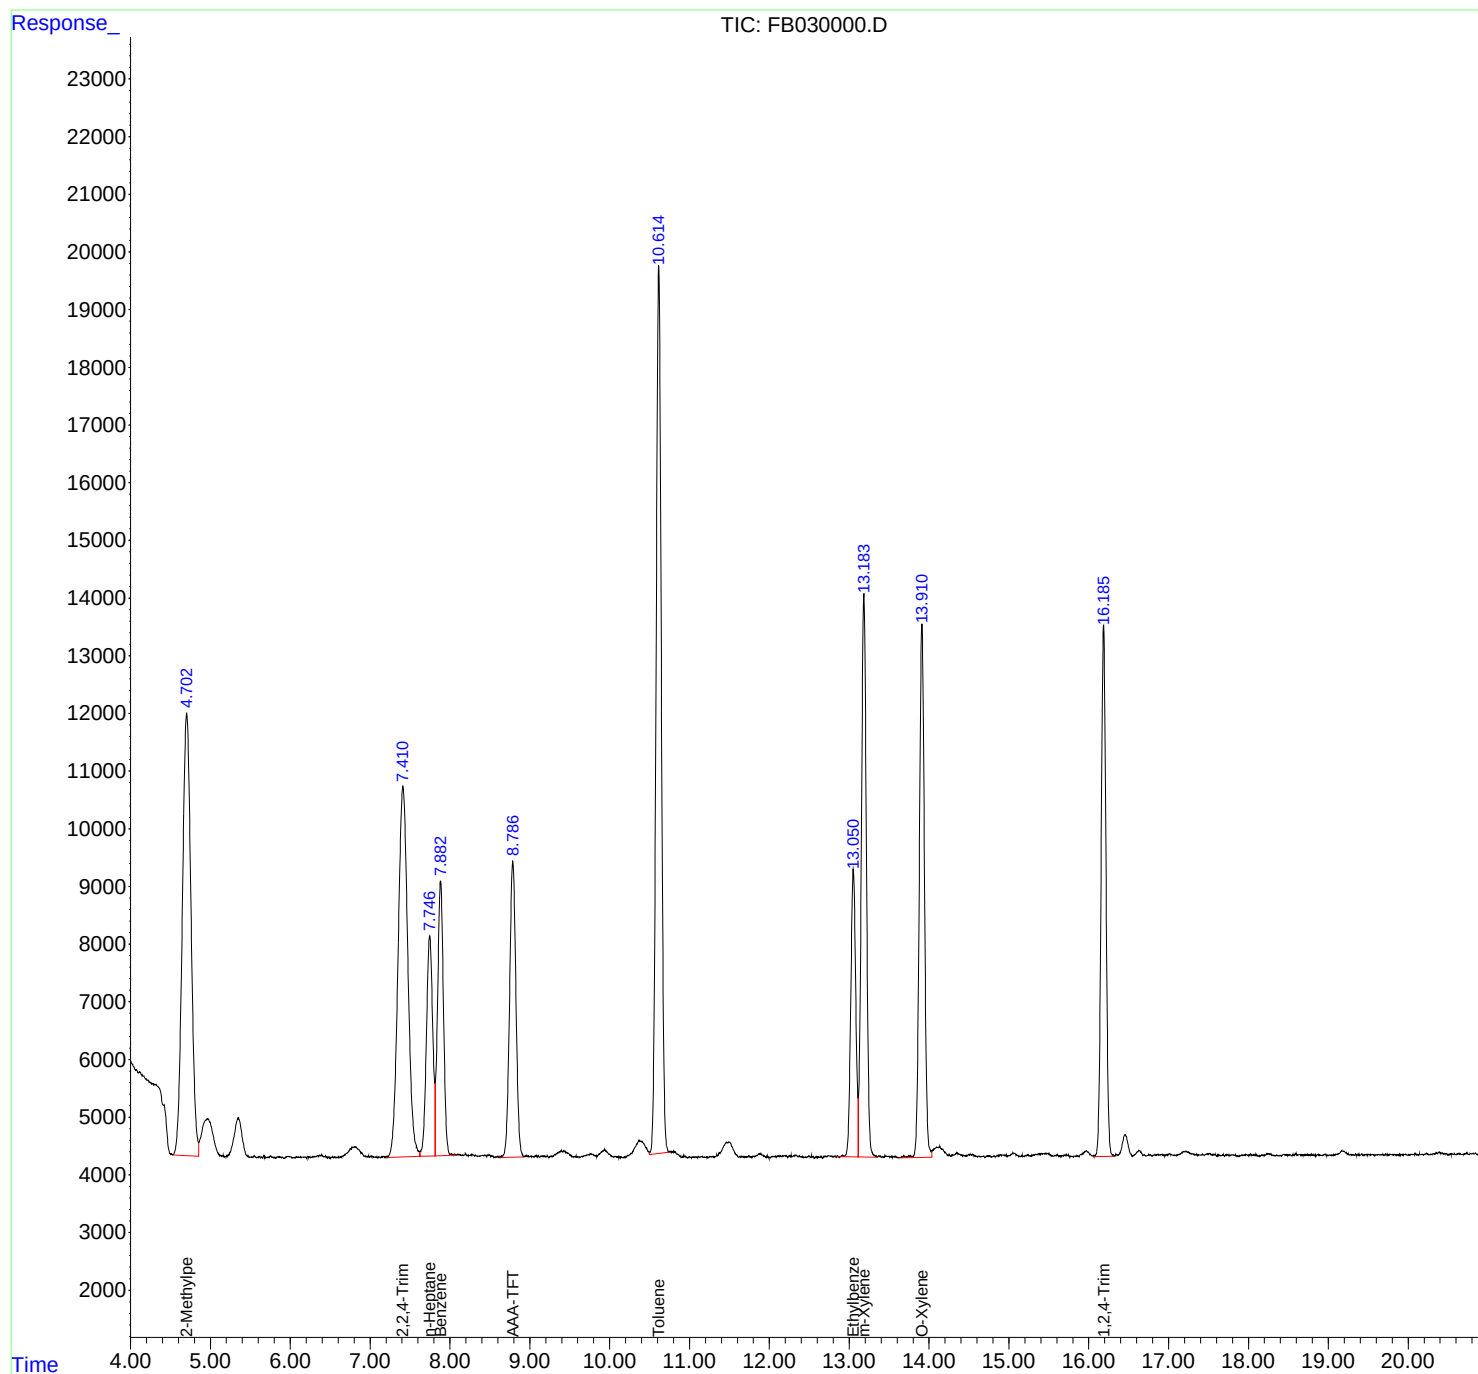


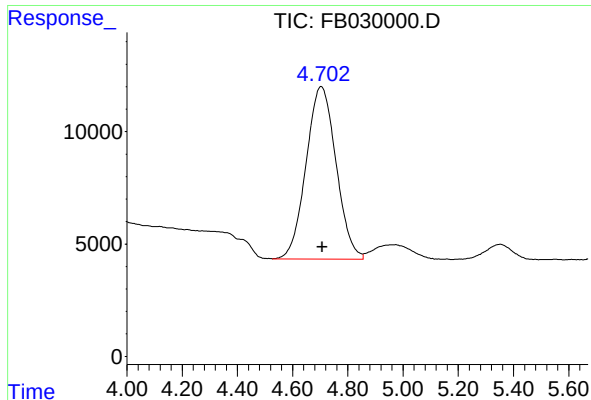

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: -0.004 min
Response: 578952
Conc: 30.64 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0607S1

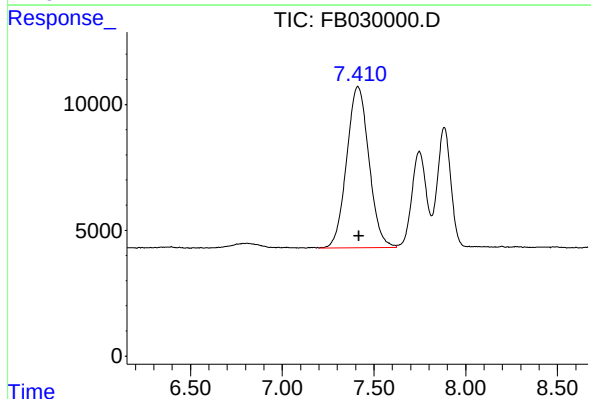


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.007 min
Response: 540563
Conc: 28.65 ng/ml

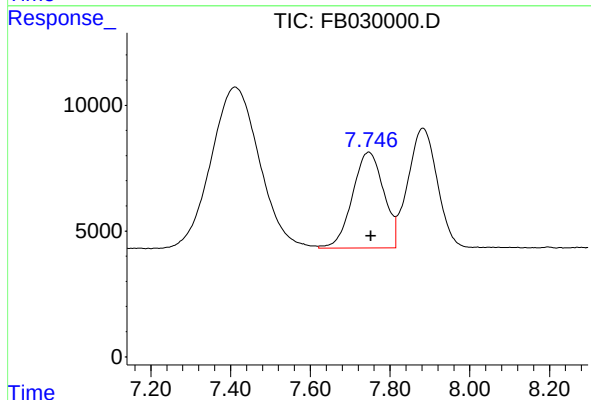


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.005 min
Response: 207783
Conc: 10.73 ng/ml

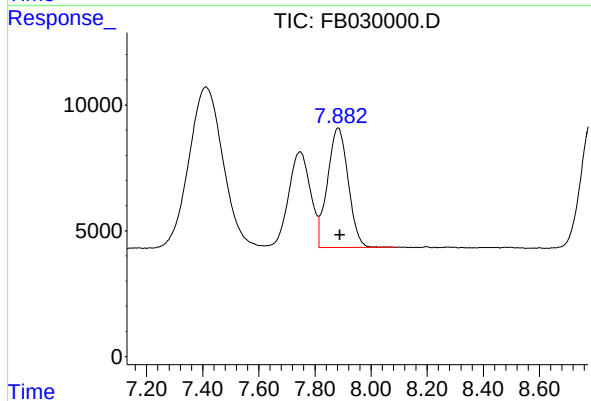

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.006 min
Response: 243635
Conc: 10.88 ng/ml

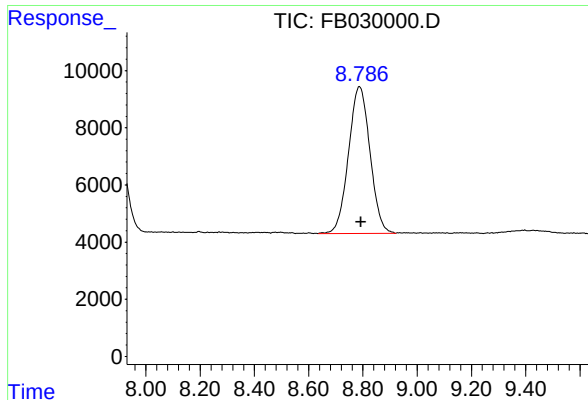

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: -0.005 min
Response: 282130
Conc: 20.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0607S1

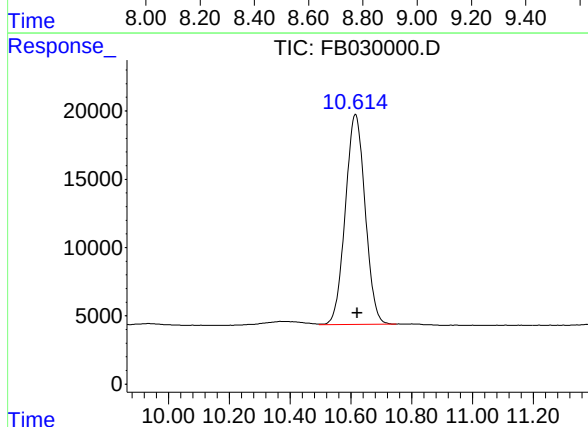


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.005 min
Response: 696165
Conc: 32.08 ng/ml

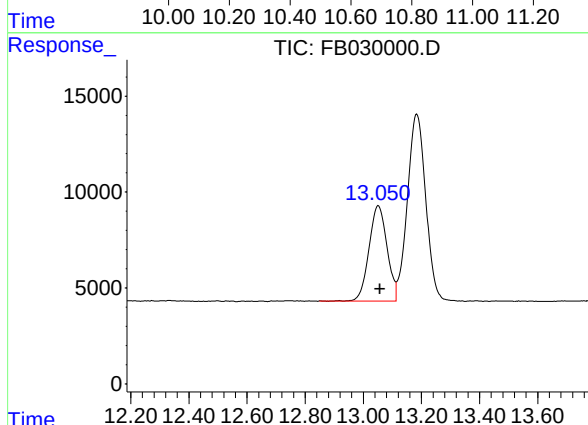


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.005 min
Response: 215847
Conc: 10.67 ng/ml

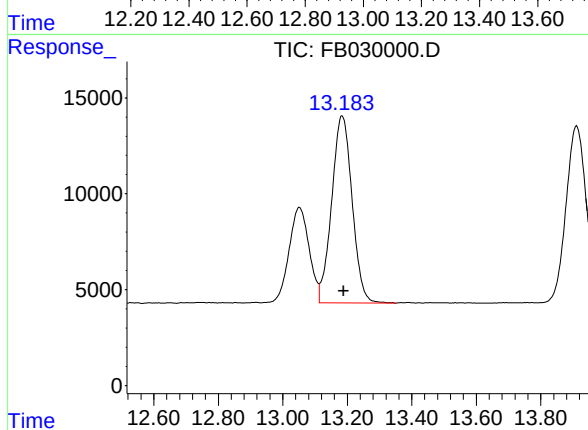

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: -0.005 min
Response: 429999
Conc: 21.38 ng/ml

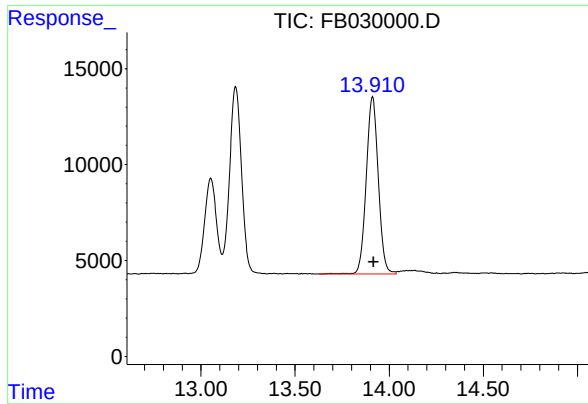

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: -0.005 min
Response: 411695
Conc: 21.12 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0607S1

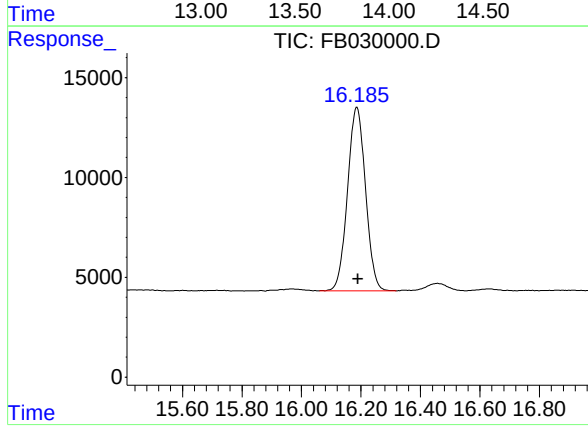

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: -0.004 min
Response: 386331
Conc: 20.63 ng/ml