

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060822\
 Data File : PS019660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2022 01:45
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 03:44:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.200	6.783	1031.6E6	414.7E6	429.979	535.200
Target Compounds							
1) T	Dalapon	3.008	0.000	653914	0	<MDL	N.D. #
3) T	4-Nitroph...	0.000	6.389	0	813248	N.D.	1.900
7) T	MCPA	7.661	0.000	1706320	0	<MDL	N.D. #
9) T	2,4-D	0.000	7.845	0	335960	N.D.	<MDL
10) T	Pentachlo...	8.621	8.287	1474303	1338241	<MDL	<MDL #
11) T	2,4,5-TP ...	9.183	8.653	2136561	582017	<MDL	<MDL #
12) T	2,4,5-T	9.422	9.055	50484662	800740	2.683	<MDL #
13) T	2,4-DB	0.000	9.565	0	403378	N.D.	<MDL
14) T	DINOSEB	0.000	9.855	0	448905	N.D.	<MDL
15) T	Picloram	10.981	10.877	1749350	40786974	<MDL	6.341 #
16) T	DCPA	11.426	10.780	5113448	1241212	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060822\
Data File : PS019660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2022 01:45
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 03:44:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

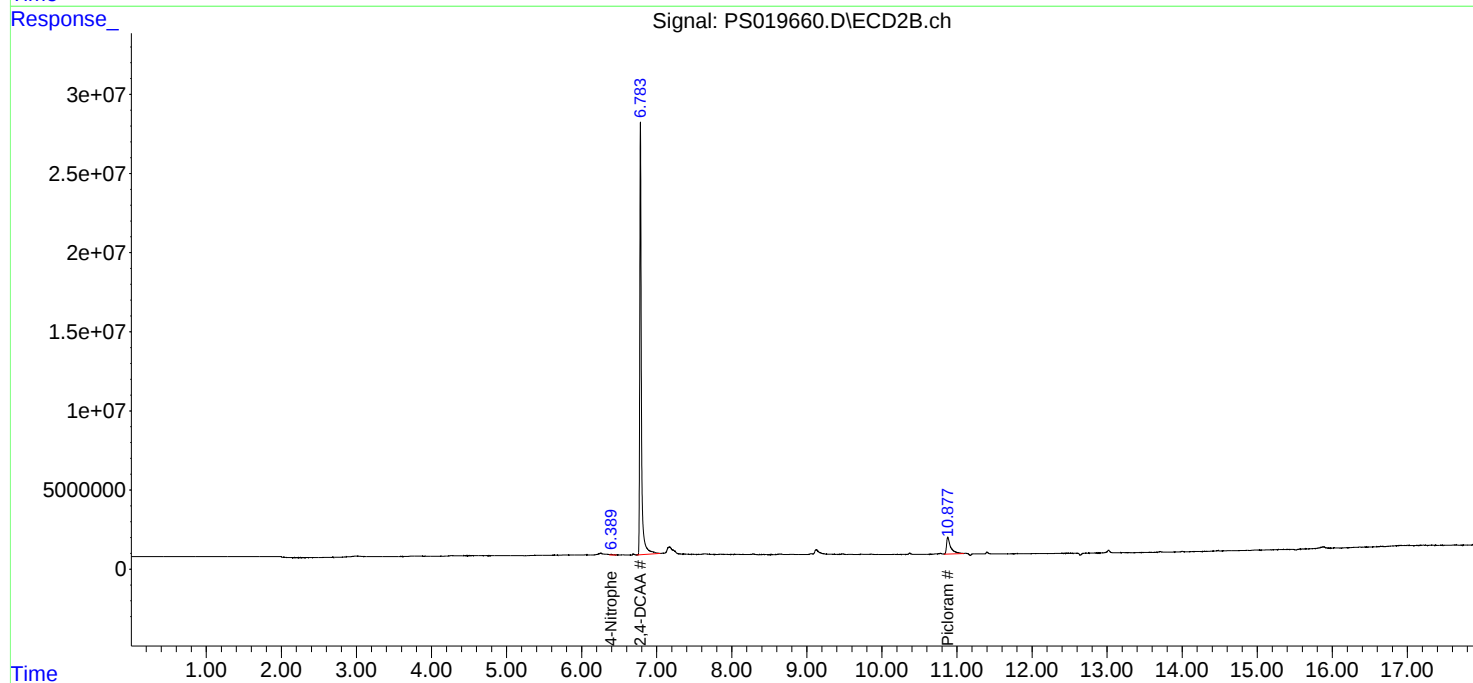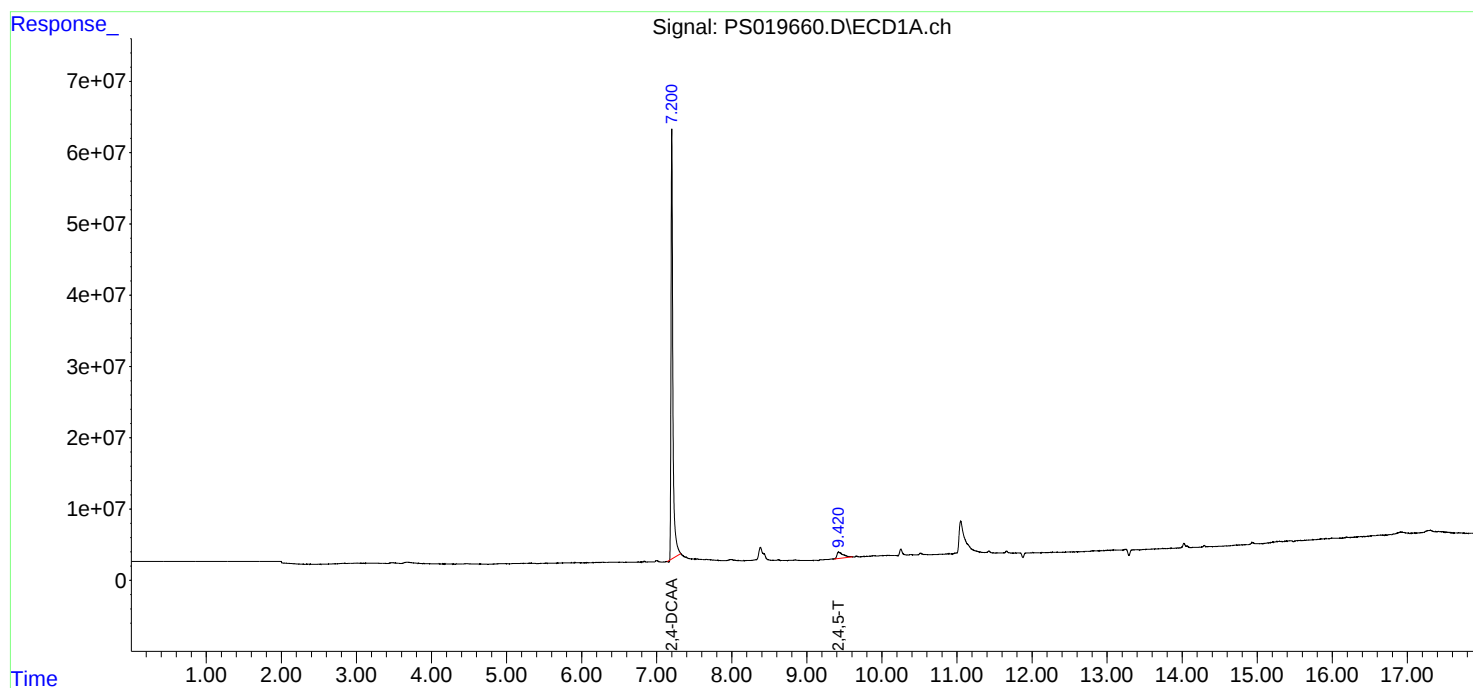


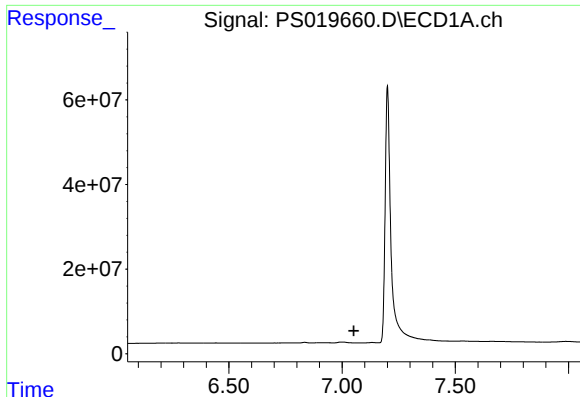

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.052 min
Response: 0
Conc: N.D.

Instrument :
FID_B
ClientSampleId :

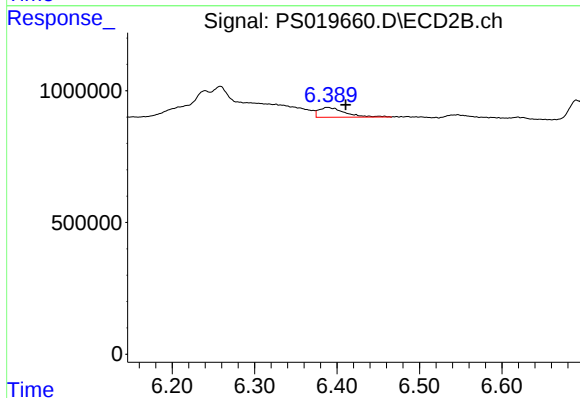


#3 4-Nitrophenol

R.T.: 6.389 min
Delta R.T.: -0.022 min
Response: 813248
Conc: 1.90 ng/ml

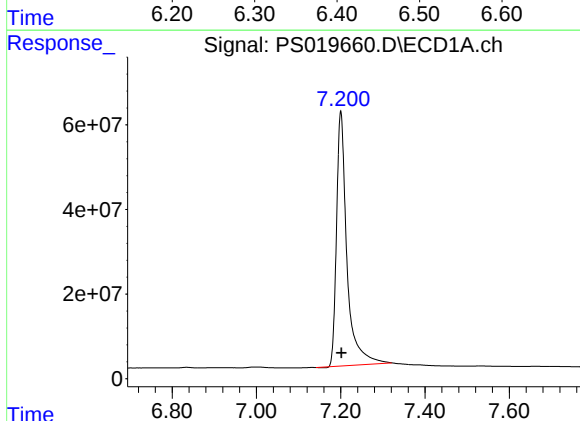


#4 2,4-DCAA

R.T.: 7.200 min
Delta R.T.: -0.002 min
Response: 1031592548
Conc: 429.98 ng/ml

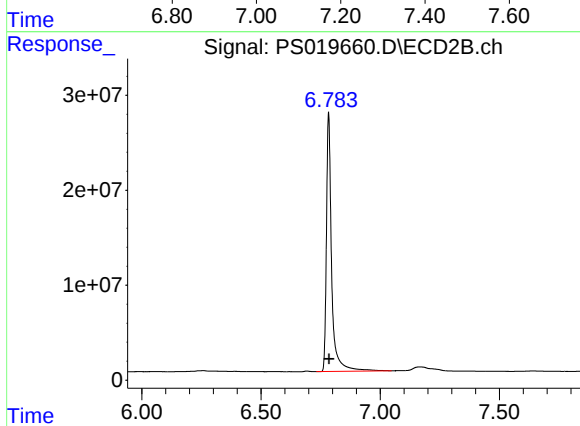

#4 2,4-DCAA


R.T.: 6.783 min
Delta R.T.: -0.001 min
Response: 414710552
Conc: 535.20 ng/ml

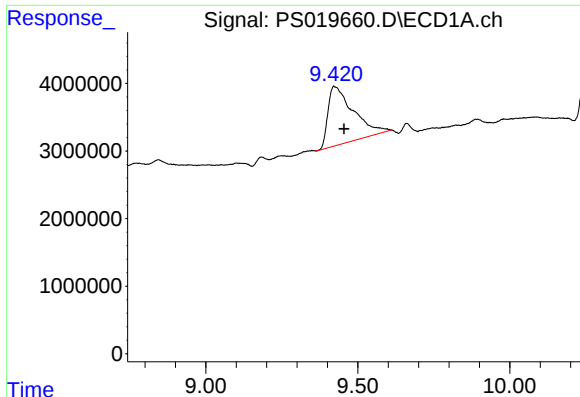

#12 2,4,5-T


R.T.: 9.422 min
Delta R.T.: -0.033 min
Response: 50484662
Conc: 2.68 ng/ml

Instrument :
FID_B
ClientSampleId :

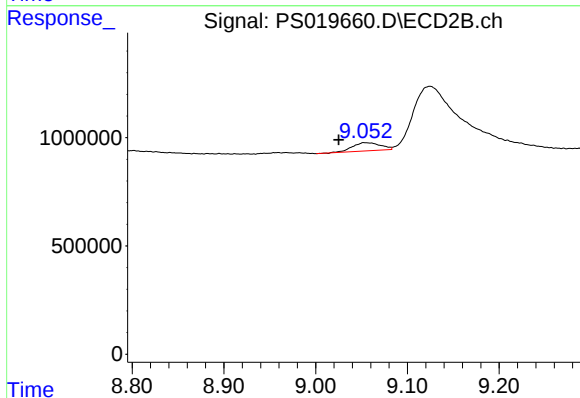


#12 2,4,5-T

R.T.: 9.055 min
Delta R.T.: 0.030 min
Response: 800740
Conc: N.D.

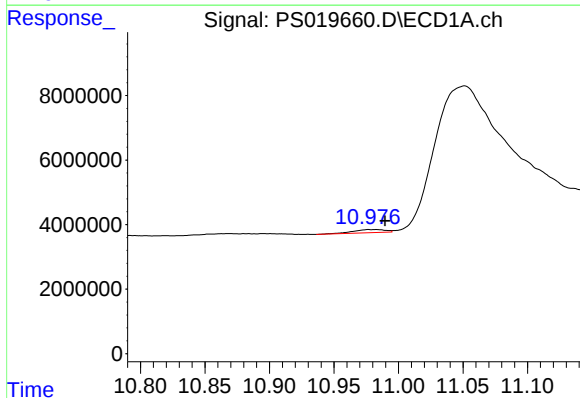

#15 Picloram

R.T.: 10.981 min
Delta R.T.: -0.009 min
Response: 1749350
Conc: N.D.

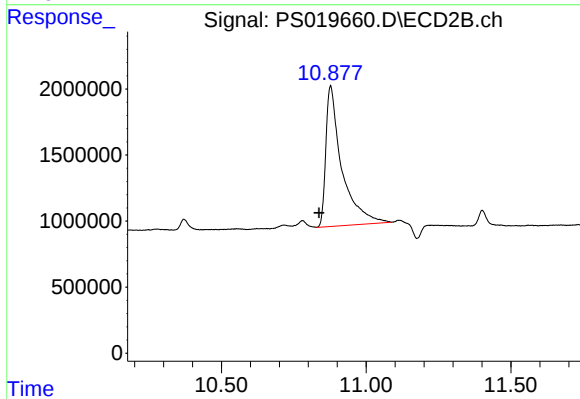

#15 Picloram

R.T.: 10.877 min
Delta R.T.: 0.039 min
Response: 40786974
Conc: 6.34 ng/ml