

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060822\
 Data File : FB027361.D
 Signal(s) : FID2B.CH
 Acq On : 8 Jun 2022 10:38
 Operator : AJ/MA
 Sample : BSF0608S1
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0608S1

Integration File: Calibration.e
 Quant Time: Jun 09 02:30:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
 Quant Title :
 QLast Update : Tue May 10 13:42:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	210604	20.063 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	365045	22.939 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	430069	26.656 ng/ml
3) t n-Heptane	7.751	114660	7.017 ng/ml
4) t Benzene	7.888	176461	9.516 ng/ml
6) t Toluene	10.621	510292	28.742 ng/ml
7) t Ethylbenzene	13.058	160717	9.732 ng/ml
8) t m-Xylene	13.191	320576	19.483 ng/ml
9) t O-Xylene	13.918	315564	19.238 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	324103	19.413 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060822\
Data File : FB027361.D
Signal(s) : FID2B.CH
Acq On : 8 Jun 2022 10:38
Operator : AJ/MA
Sample : BSF0608S1
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0608S1

Integration File: Calibration.e
Quant Time: Jun 09 02:30:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

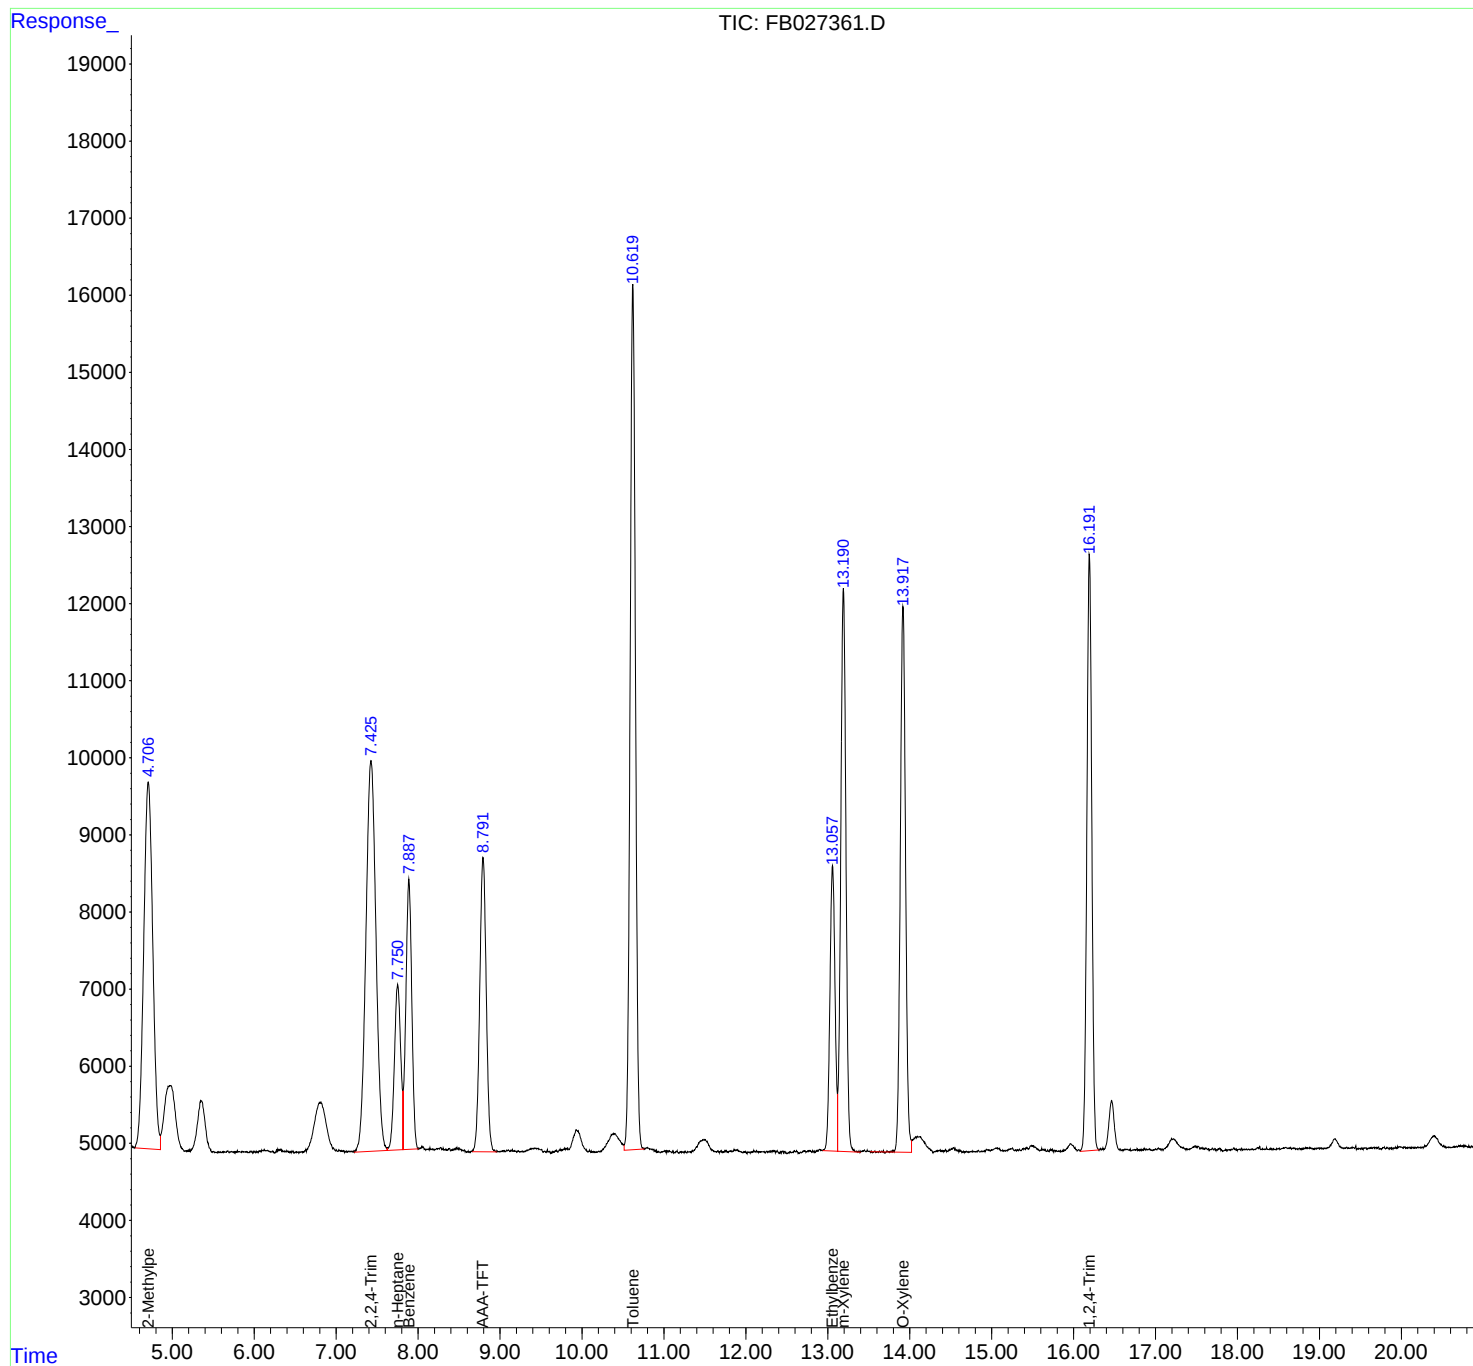


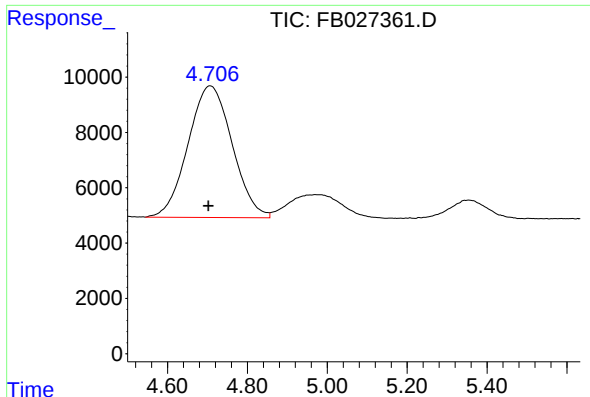

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: 0.005 min
Response: 365045
Conc: 22.94 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0608S1

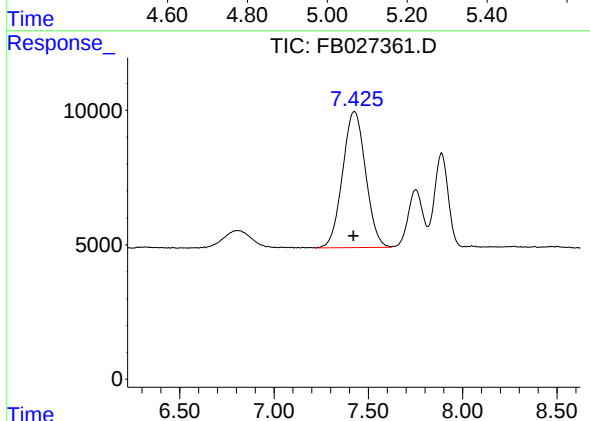


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: 0.006 min
Response: 430069
Conc: 26.66 ng/ml

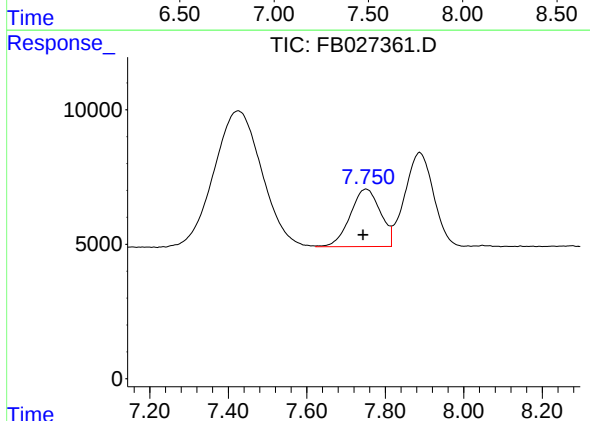


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.008 min
Response: 114660
Conc: 7.02 ng/ml

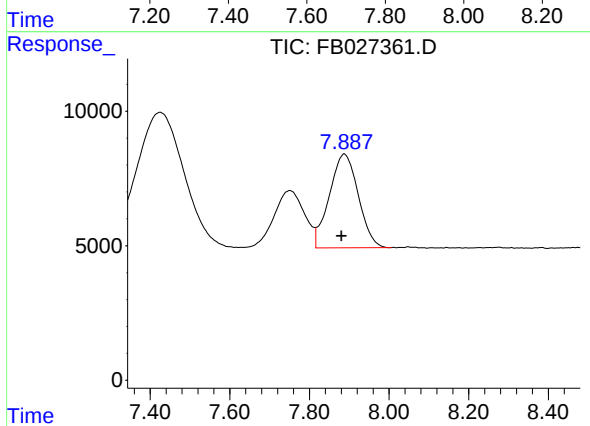

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.008 min
Response: 176461
Conc: 9.52 ng/ml

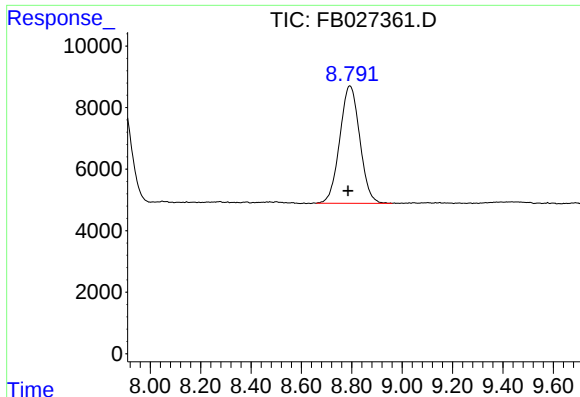

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.008 min
Response: 210604
Conc: 20.06 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0608S1

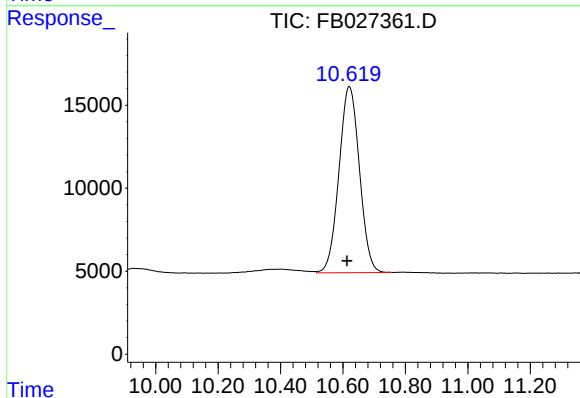


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.008 min
Response: 510292
Conc: 28.74 ng/ml

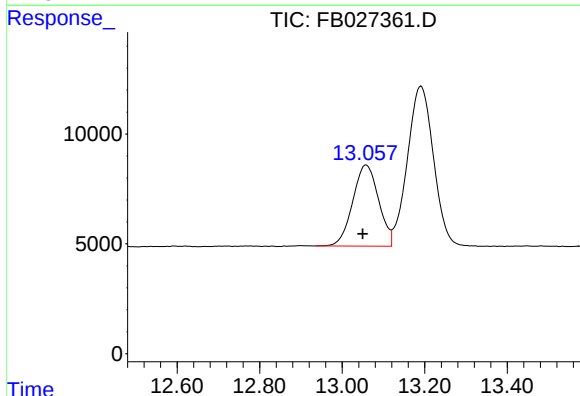


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.008 min
Response: 160717
Conc: 9.73 ng/ml

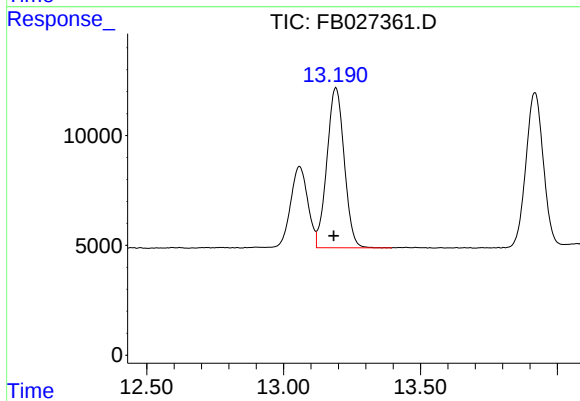

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.008 min
Response: 320576
Conc: 19.48 ng/ml

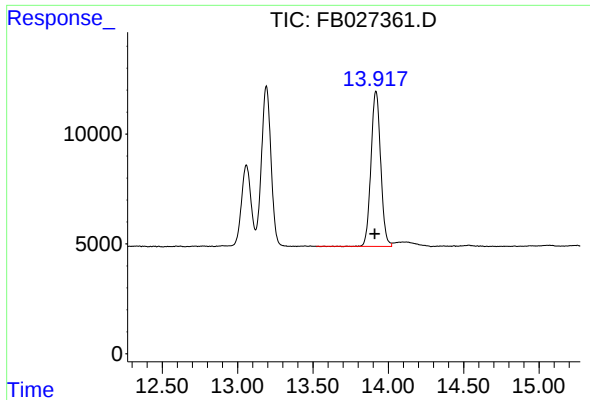

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.008 min
Response: 315564
Conc: 19.24 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0608S1

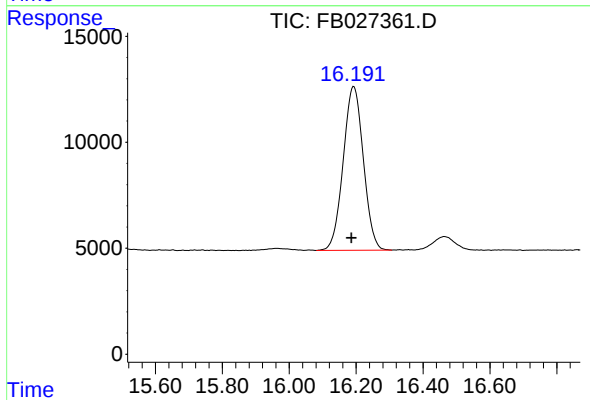

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.007 min
Response: 324103
Conc: 19.41 ng/ml