

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060920\
 Data File : FB024437.D
 Signal(s) : FID2B.CH
 Acq On : 9 Jun 2020 15:43
 Operator : DD/AJ
 Sample : L2815-02
 Misc : 5.01gm/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 10 01:35:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	488232	20.180 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.695	3595	0.112 ng/ml
2) t 2,2,4-Trimethylpentane	7.404	5313	0.158 ng/ml
3) t n-Heptane	7.750	1550	0.046 ng/ml
4) t Benzene	7.887	4430	0.110 ng/ml
6) t Toluene	10.633	89897	2.288 ng/ml
7) t Ethylbenzene	13.065	2812	0.080 ng/ml
8) t m-Xylene	13.204	4106	0.120 ng/ml
9) t O-Xylene	13.935	3421	0.102 ng/ml
10) t 1,2,4-Trimethylbenzene	16.222	3582	0.129 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060920\
Data File : FB024437.D
Signal(s) : FID2B.CH
Acq On : 9 Jun 2020 15:43
Operator : DD/AJ
Sample : L2815-02
Misc : 5.01gm/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 10 01:35:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

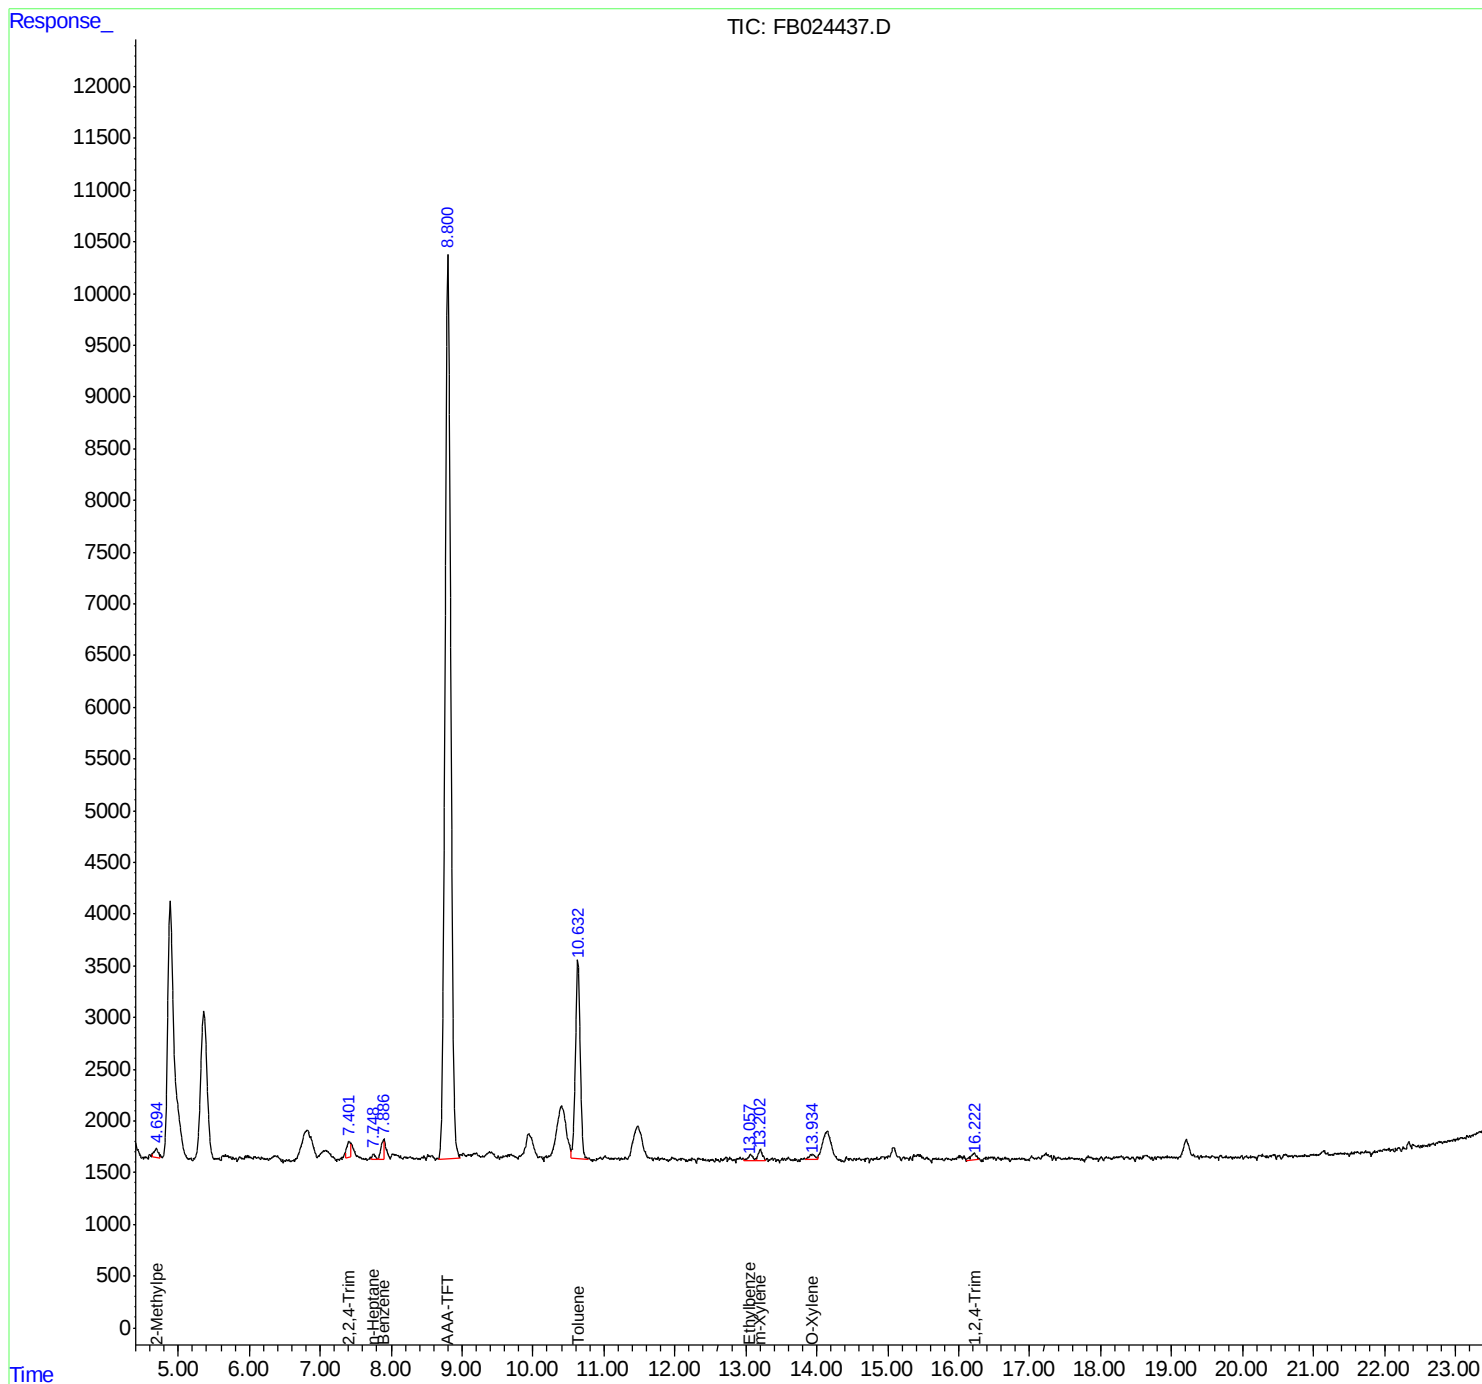

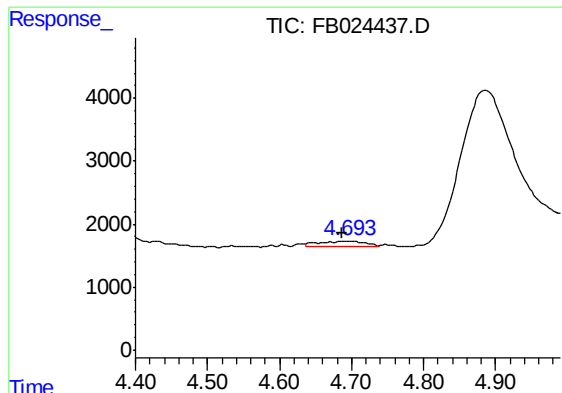


#1 2-Methylpentane

R.T.: 4.695 min
Delta R.T.: 0.008 min
Response: 3595
Conc: 0.11 ng/ml

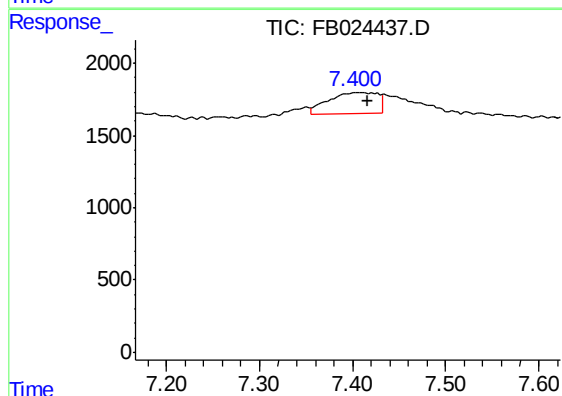


#2 2,2,4-Trimethylpentane

R.T.: 7.404 min
Delta R.T.: -0.012 min
Response: 5313
Conc: 0.16 ng/ml

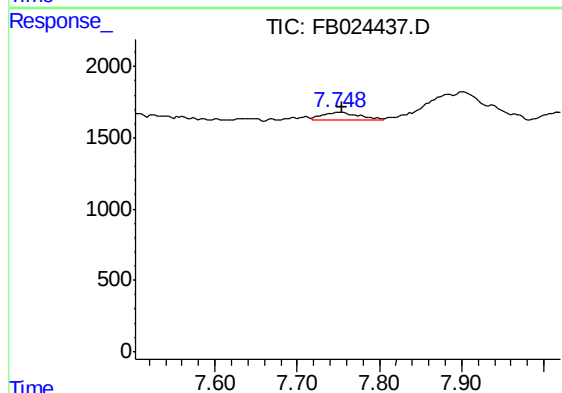


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.005 min
Response: 1550
Conc: 0.05 ng/ml

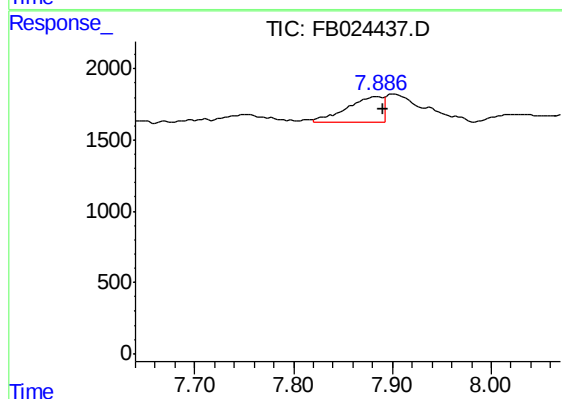


#4 Benzene

R.T.: 7.887 min
Delta R.T.: -0.003 min
Response: 4430
Conc: 0.11 ng/ml

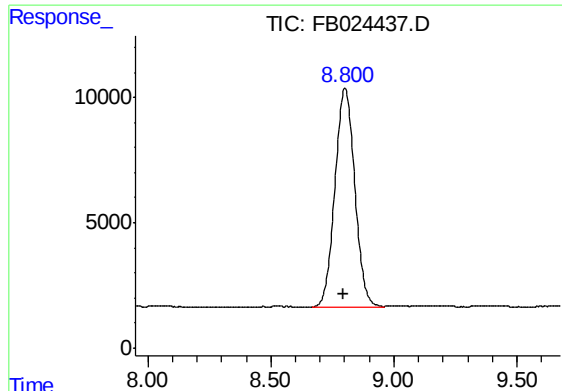


#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.005 min
Response: 488232
Conc: 20.18 ng/ml

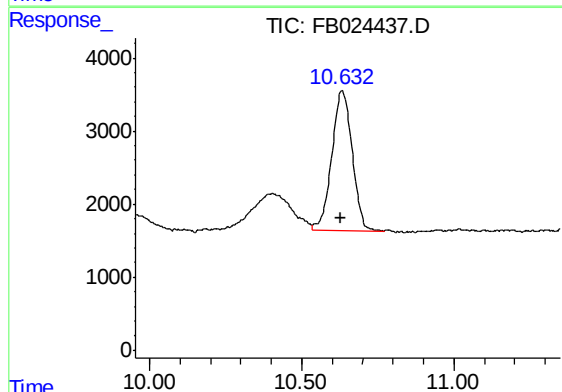


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.005 min
Response: 89897
Conc: 2.29 ng/ml

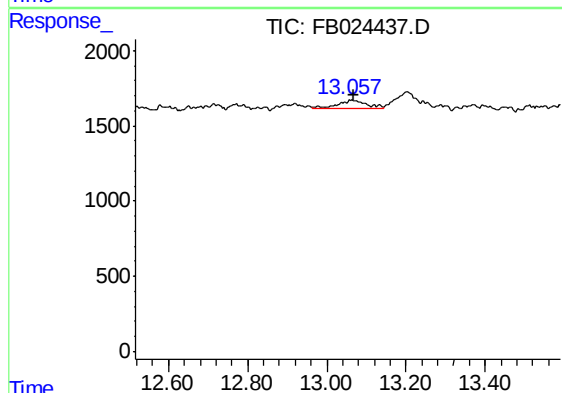


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.003 min
Response: 2812
Conc: 0.08 ng/ml

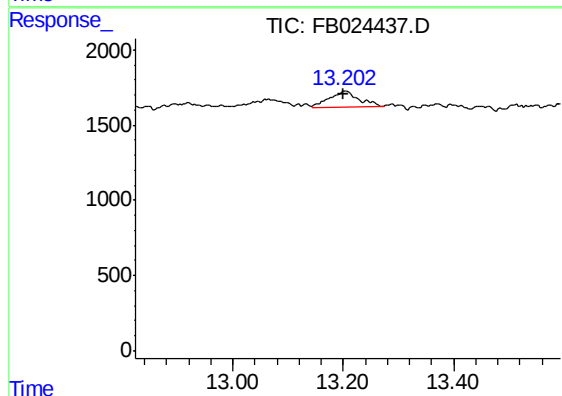


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.003 min
Response: 4106
Conc: 0.12 ng/ml

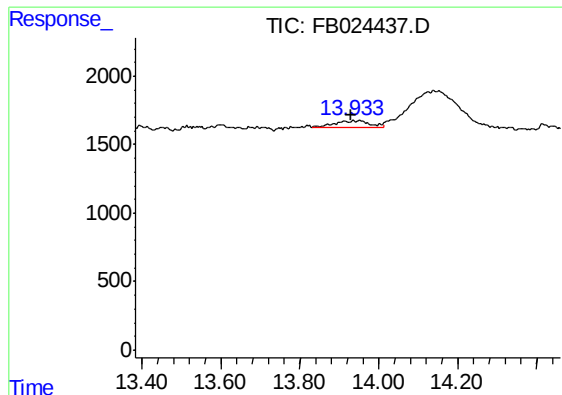

#9 O-Xylene

R.T.: 13.935 min
Delta R.T.: 0.007 min
Response: 3421
Conc: 0.10 ng/ml

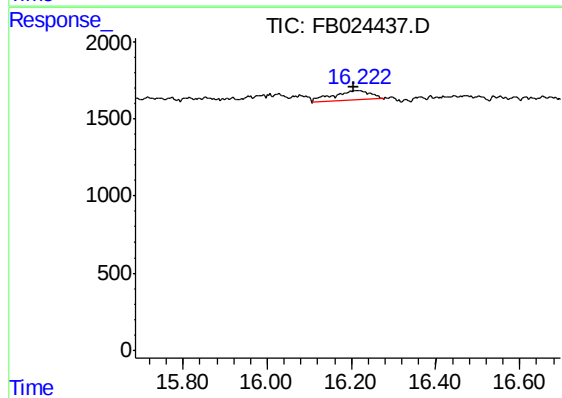

#10 1,2,4-Trimethylbenzene

R.T.: 16.222 min
Delta R.T.: 0.015 min
Response: 3582
Conc: 0.13 ng/ml