

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060921\
Data File : FB025852.D
Signal(s) : FID2B.CH
Acq On : 9 Jun 2021 11:37
Operator : DD/AJ
Sample : 20 GRO STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 09 13:03:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:02:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.221	462558	20.000 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.177	773236	30.000 ng/ml
2) t 2,2,4-Trimethylpentane	7.878	583673	30.000 ng/ml
3) t n-Heptane	8.196	344461	10.000 ng/ml
4) t Benzene	8.347	411306	10.000 ng/ml
6) t Toluene	11.041	1174678	30.000 ng/ml
7) t Ethylbenzene	13.448	357392	10.000 ng/ml
8) t m-Xylene	13.579	706913	20.000 ng/ml
9) t O-Xylene	14.301	614867	20.000 ng/ml
10) t 1,2,4-Trimethylbenzene	16.554	372883	20.000 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060921\
Data File : FB025852.D
Signal(s) : FID2B.CH
Acq On : 9 Jun 2021 11:37
Operator : DD/AJ
Sample : 20 GRO STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 09 13:03:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:02:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

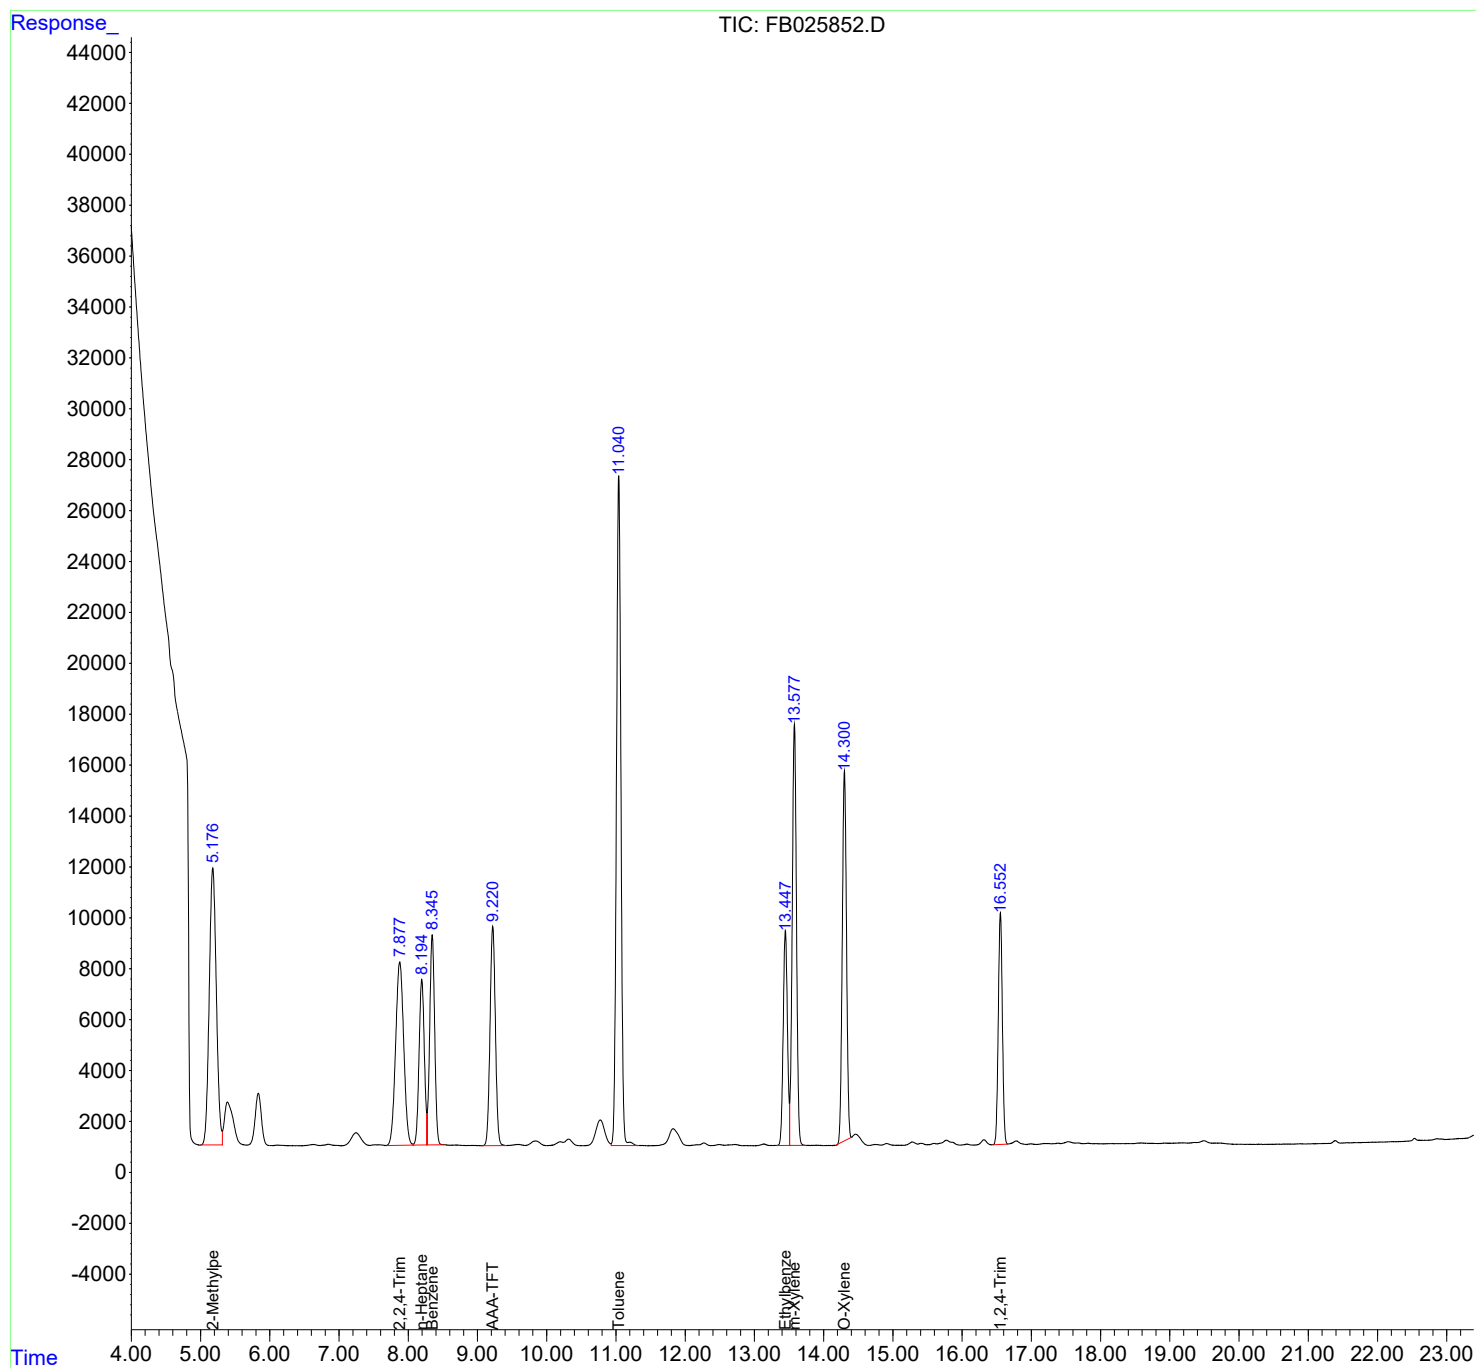


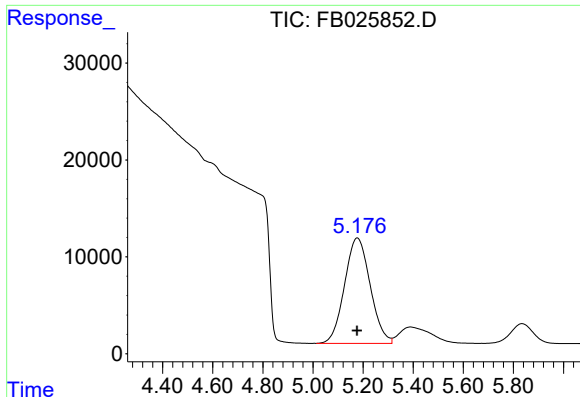

#1 2-Methylpentane


R.T.: 5.177 min
Delta R.T.: 0.000 min
Response: 773236
Conc: 30.00 ng/ml

Instrument :
FID_B
ClientSampleId :

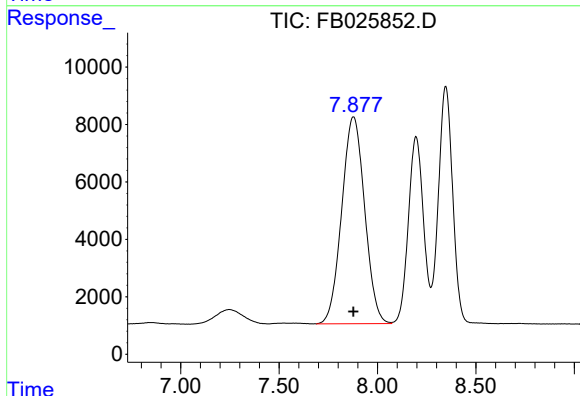


#2 2,2,4-Trimethylpentane

R.T.: 7.878 min
Delta R.T.: 0.000 min
Response: 583673
Conc: 30.00 ng/ml

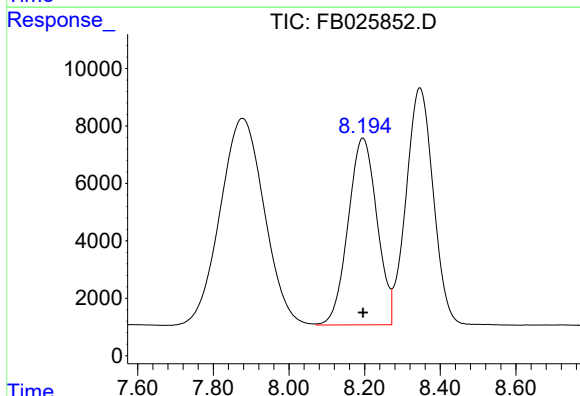


#3 n-Heptane

R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 344461
Conc: 10.00 ng/ml

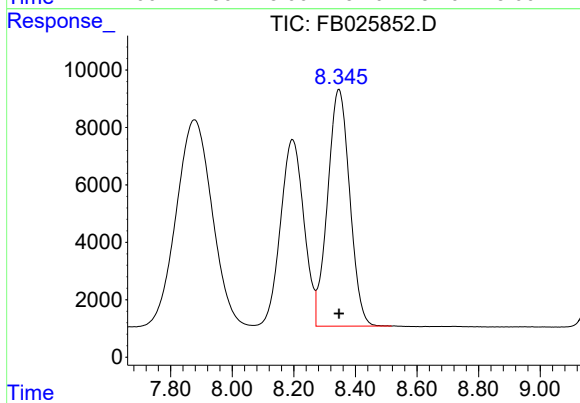

#4 Benzene


R.T.: 8.347 min
Delta R.T.: 0.000 min
Response: 411306
Conc: 10.00 ng/ml

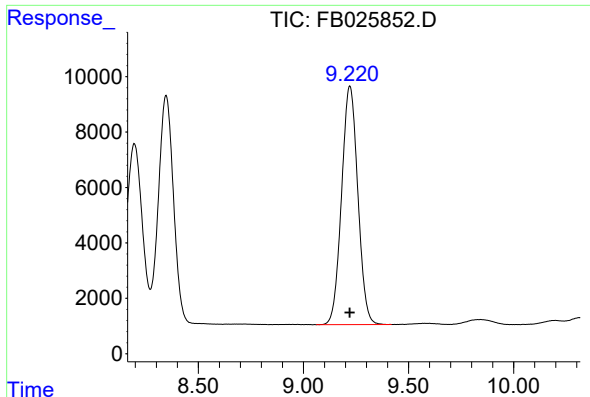

#5 AAA-TFT


R.T.: 9.221 min
Delta R.T.: 0.000 min
Response: 462558
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :

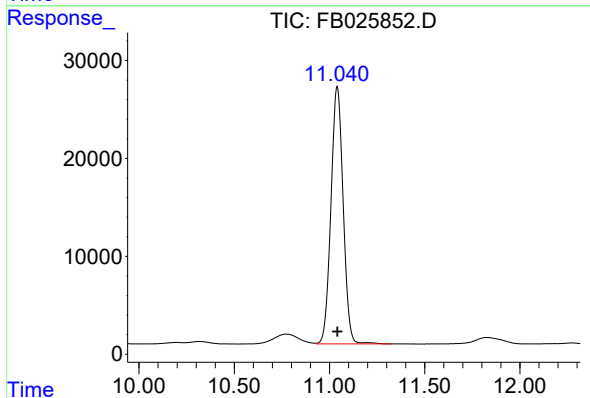


#6 Toluene

R.T.: 11.041 min
Delta R.T.: 0.000 min
Response: 1174678
Conc: 30.00 ng/ml

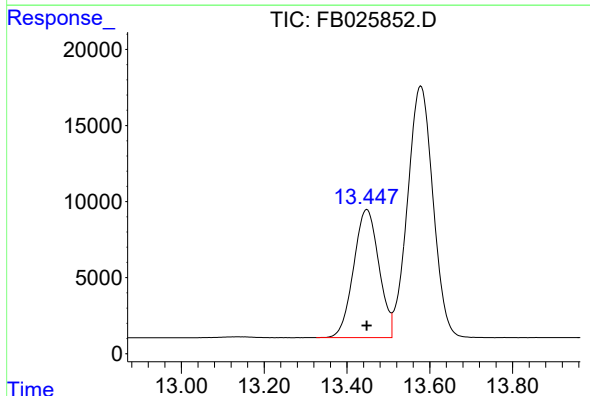


#7 Ethylbenzene

R.T.: 13.448 min
Delta R.T.: 0.000 min
Response: 357392
Conc: 10.00 ng/ml

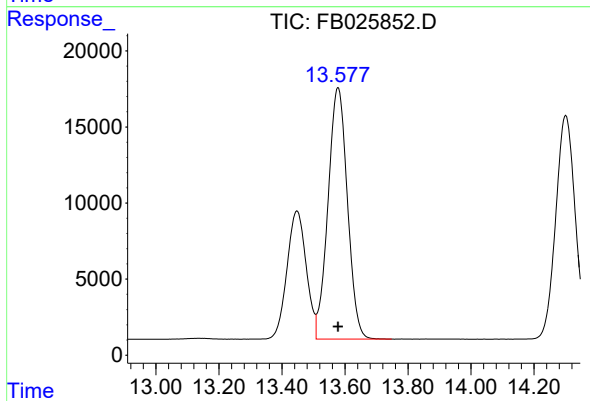

#8 m-Xylene


R.T.: 13.579 min
Delta R.T.: 0.000 min
Response: 706913
Conc: 20.00 ng/ml

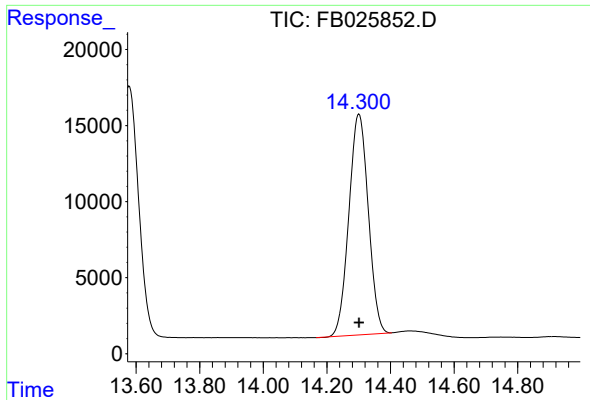

#9 O-Xylene

R.T.: 14.301 min
Delta R.T.: 0.000 min
Response: 614867
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :

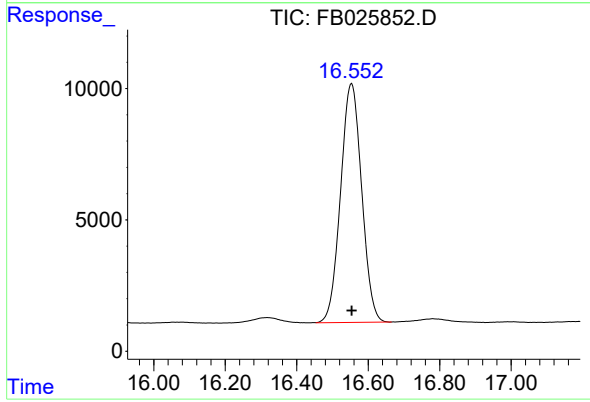

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min
Delta R.T.: 0.000 min
Response: 372883
Conc: 20.00 ng/ml