

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060921\
Data File : FB025859.D
Signal(s) : FID2B.CH
Acq On : 9 Jun 2021 16:19
Operator : DD/AJ
Sample : M2648-01
Misc : 4.03g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 09 16:39:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.228	235740	9.755 ng/ml
Target Compounds			
8) t m-Xylene	13.583	19751	0.502 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060921\
Data File : FB025859.D
Signal(s) : FID2B.CH
Acq On : 9 Jun 2021 16:19
Operator : DD/AJ
Sample : M2648-01
Misc : 4.03g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 09 16:39:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

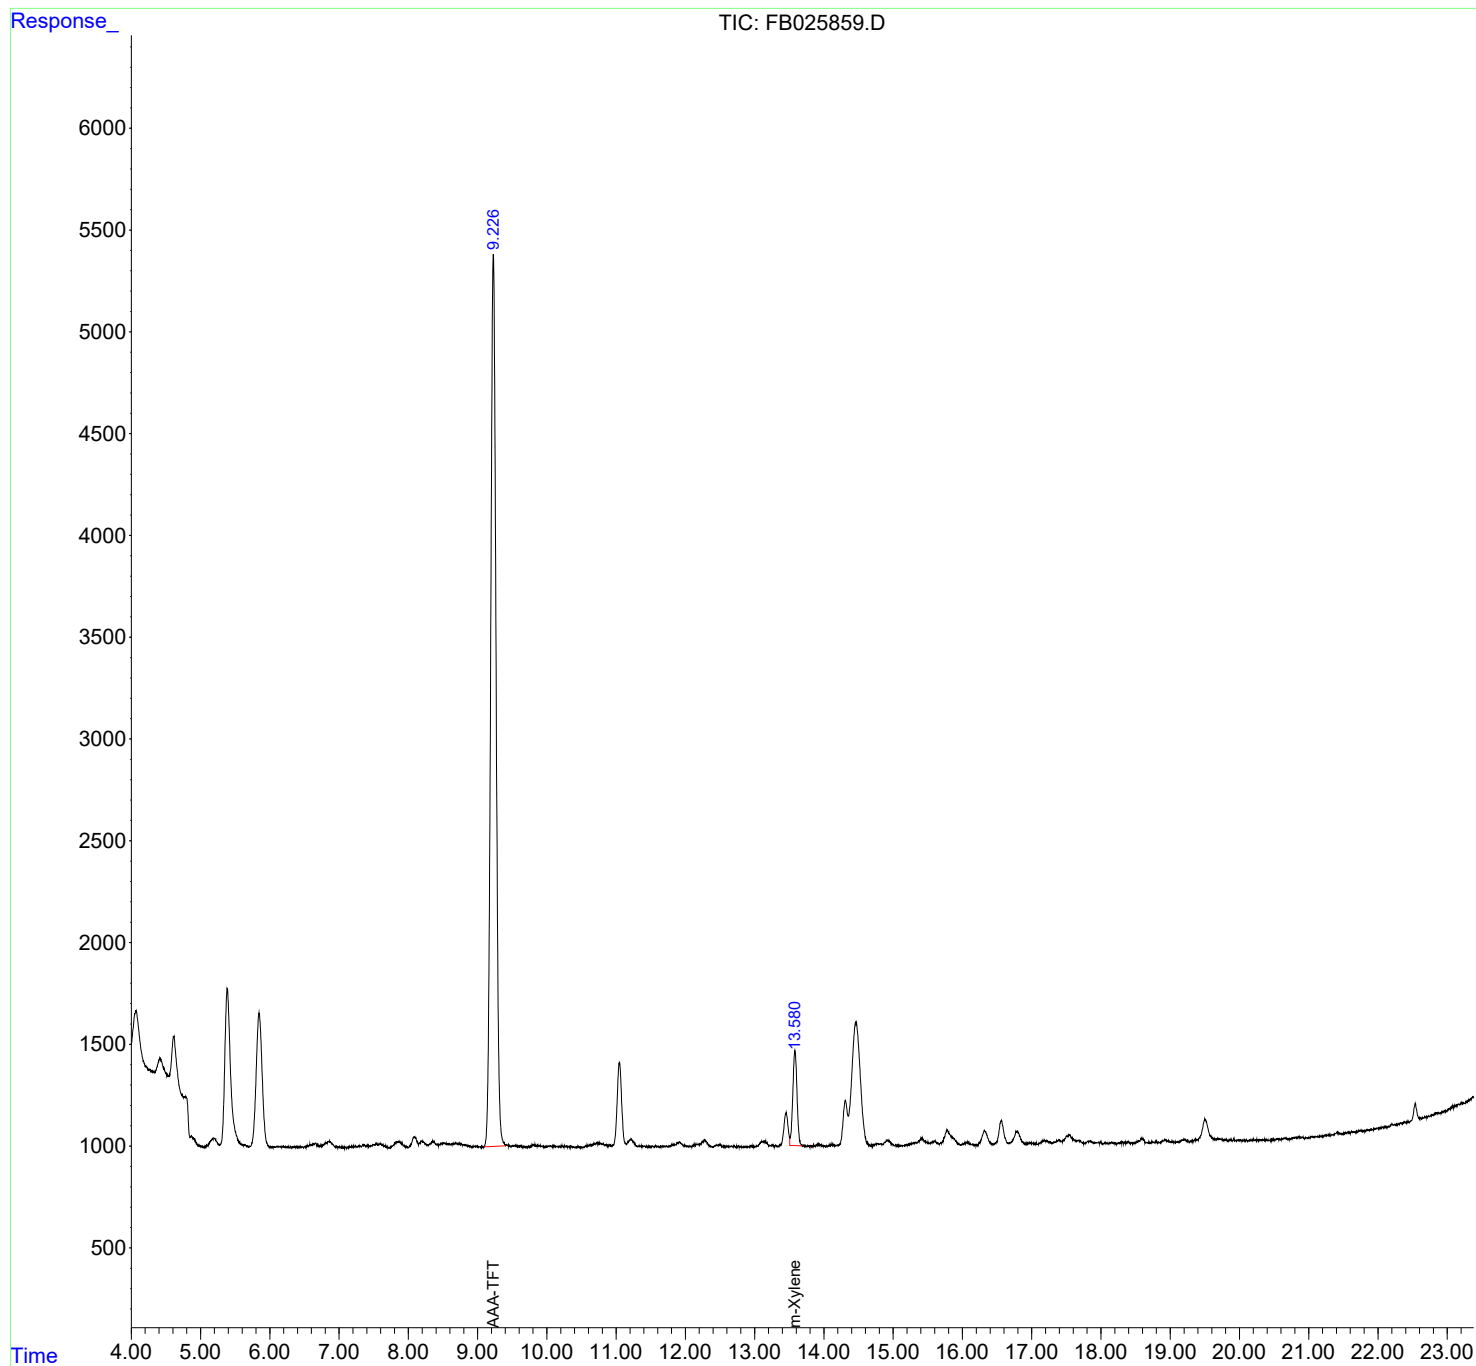


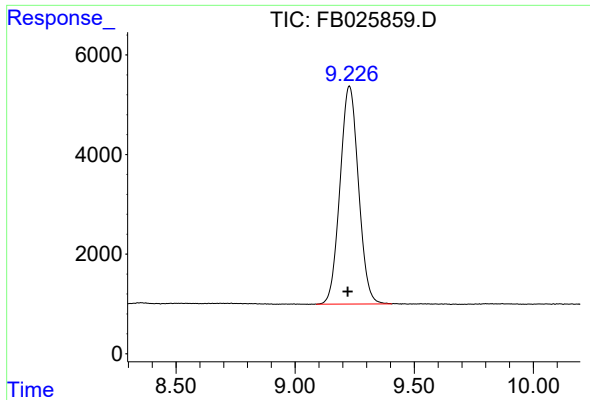

#5 AAA-TFT

R.T.: 9.228 min
Delta R.T.: 0.007 min
Response: 235740
Conc: 9.75 ng/ml

Instrument :
FID_B
ClientSampleId :

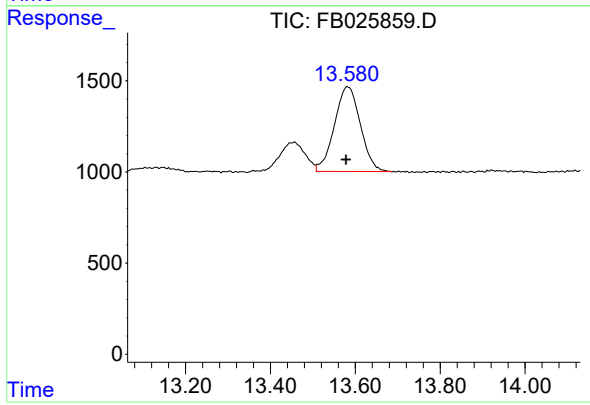

#8 m-Xylene

R.T.: 13.583 min
Delta R.T.: 0.004 min
Response: 19751
Conc: 0.50 ng/ml