

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060921\
 Data File : FB025858.D
 Signal(s) : FID2B.CH
 Acq On : 9 Jun 2021 15:44
 Operator : DD/AJ
 Sample : BSF0609S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0609S1

Integration File: Calibration.e
 Quant Time: Jun 09 16:34:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
 Quant Title :
 QLast Update : Wed Jun 09 13:39:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.223	428624	17.736 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.170	767265	29.155 ng/ml
2) t 2,2,4-Trimethylpentane	7.878	601056	29.837 ng/ml
3) t n-Heptane	8.196	370315	10.302 ng/ml
4) t Benzene	8.347	402838	9.650 ng/ml
6) t Toluene	11.044	1145610	27.839 ng/ml
7) t Ethylbenzene	13.451	343447	9.012 ng/ml
8) t m-Xylene	13.582	671694	17.086 ng/ml
9) t O-Xylene	14.305	576134	18.069 ng/ml
10) t 1,2,4-Trimethylbenzene	16.557	337985	17.172 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060921\
Data File : FB025858.D
Signal(s) : FID2B.CH
Acq On : 9 Jun 2021 15:44
Operator : DD/AJ
Sample : BSF0609S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0609S1

Integration File: Calibration.e
Quant Time: Jun 09 16:34:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

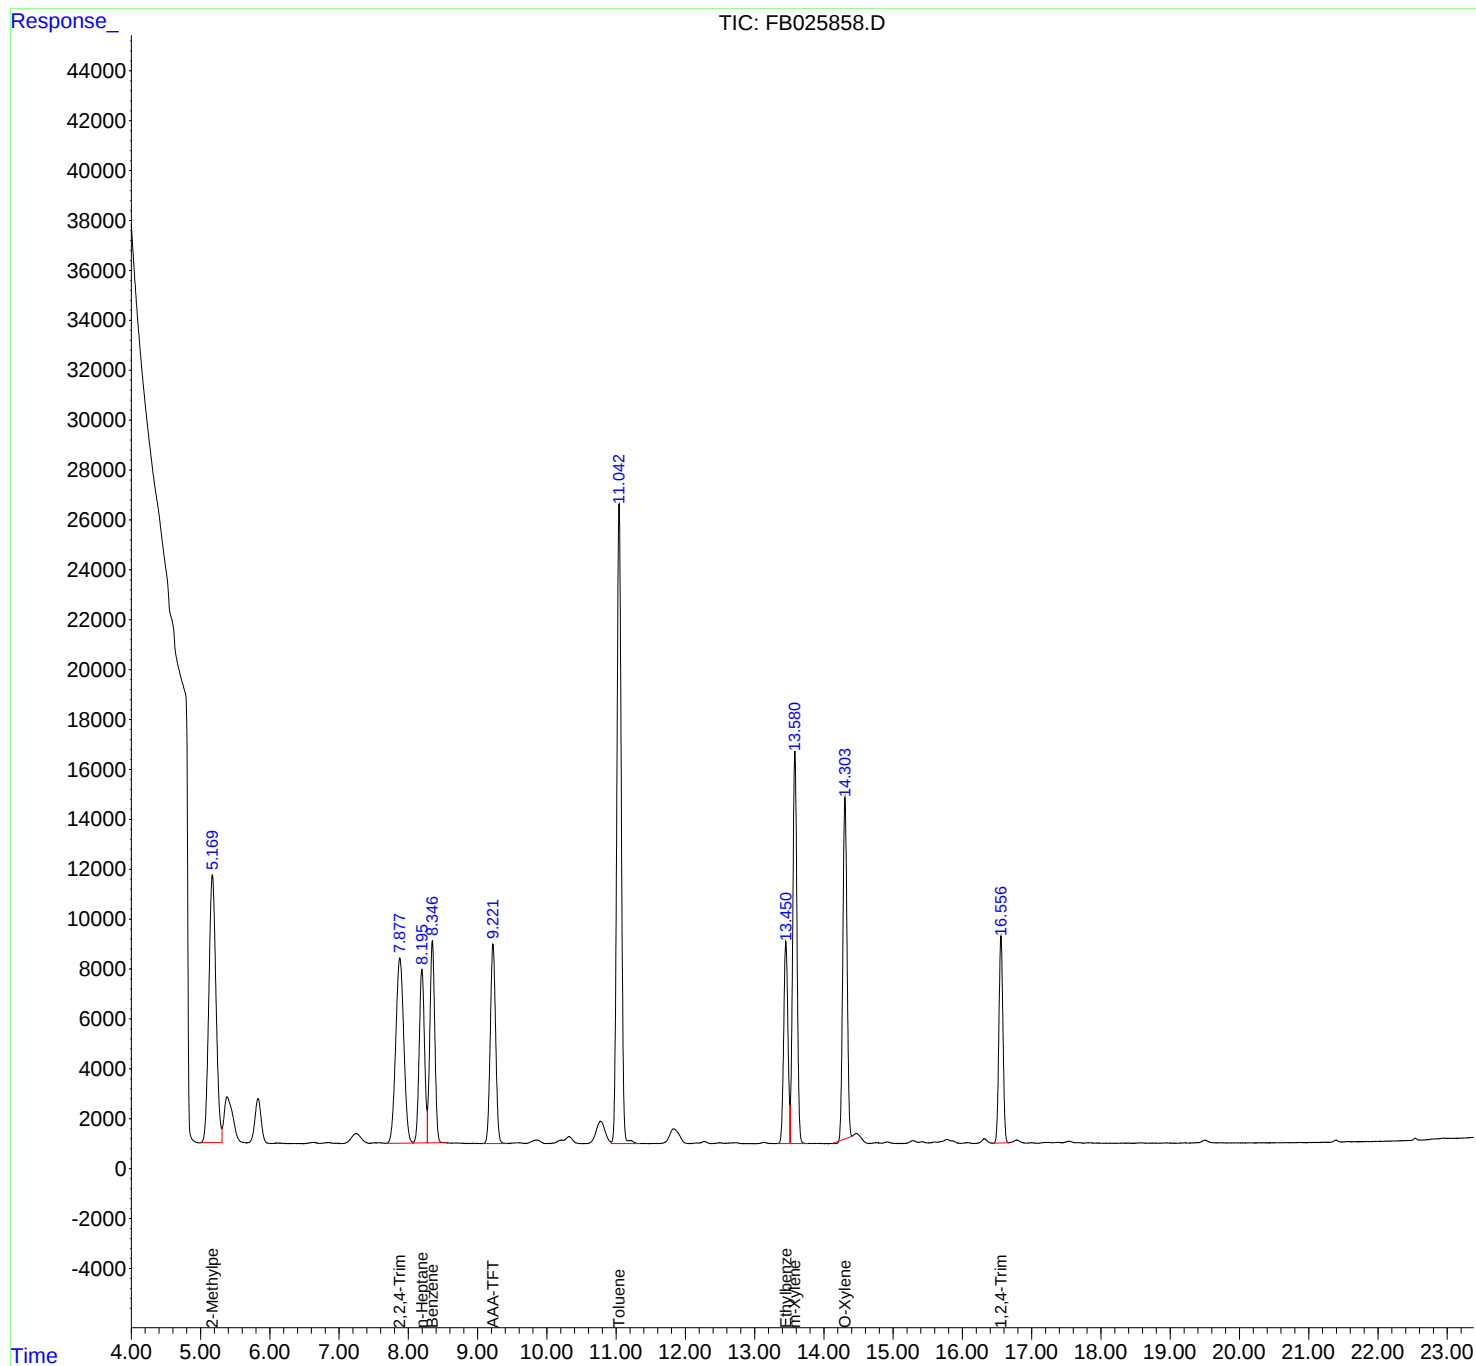


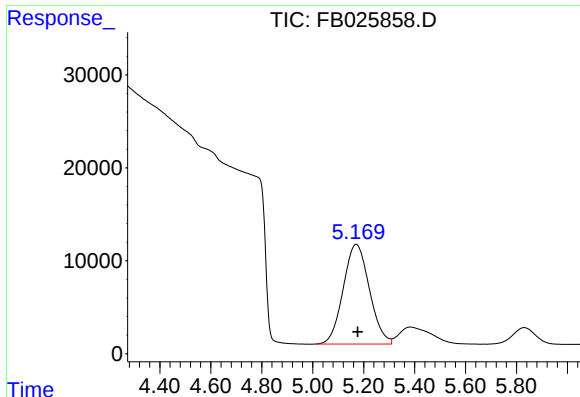

#1 2-Methylpentane


R.T.: 5.170 min
Delta R.T.: -0.007 min
Response: 767265
Conc: 29.15 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0609S1

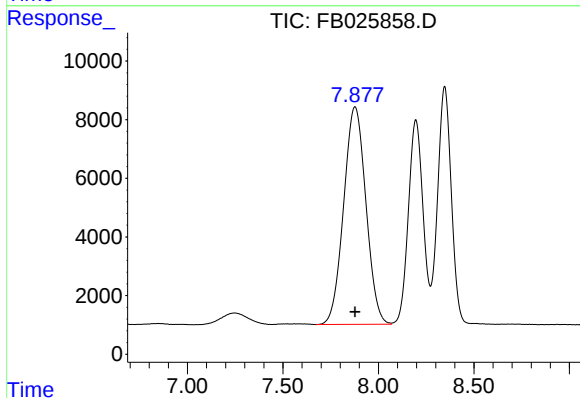


#2 2,2,4-Trimethylpentane

R.T.: 7.878 min
Delta R.T.: 0.000 min
Response: 601056
Conc: 29.84 ng/ml

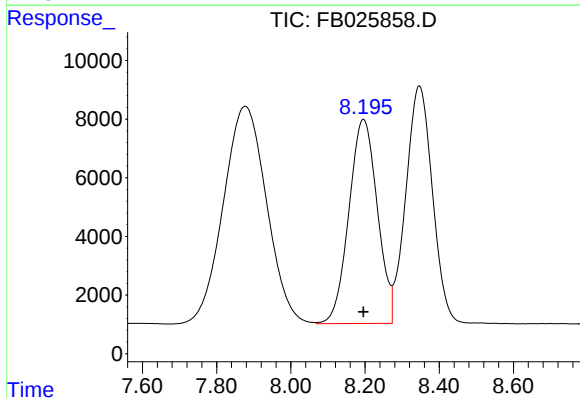


#3 n-Heptane

R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 370315
Conc: 10.30 ng/ml

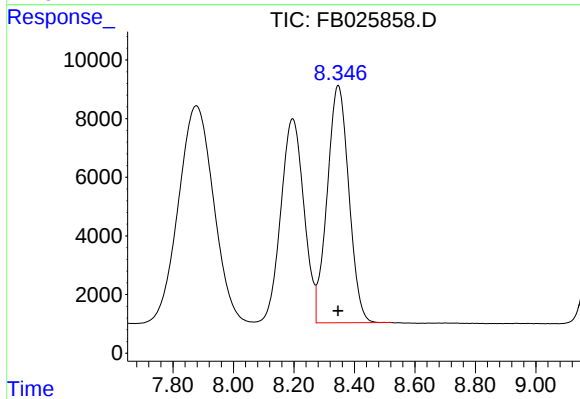

#4 Benzene


R.T.: 8.347 min
Delta R.T.: 0.000 min
Response: 402838
Conc: 9.65 ng/ml

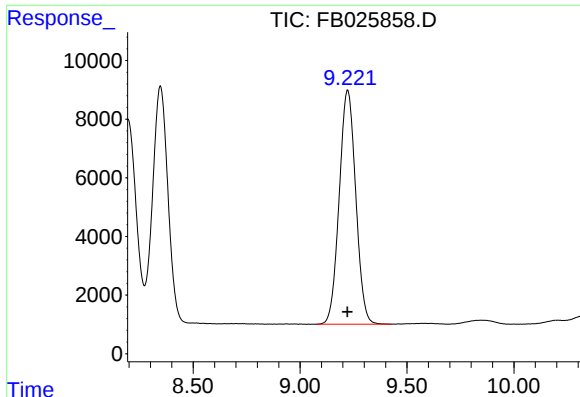

#5 AAA-TFT


R.T.: 9.223 min
Delta R.T.: 0.002 min
Response: 428624
Conc: 17.74 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0609S1

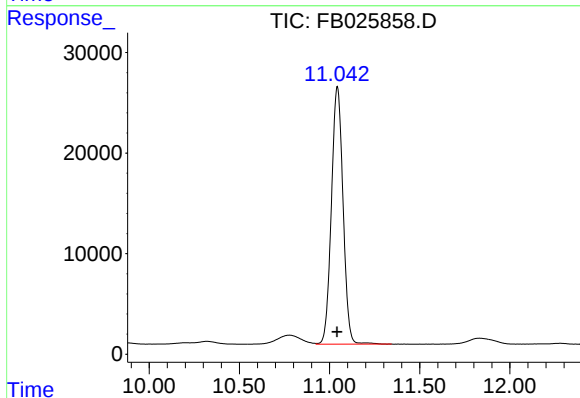


#6 Toluene

R.T.: 11.044 min
Delta R.T.: 0.002 min
Response: 1145610
Conc: 27.84 ng/ml

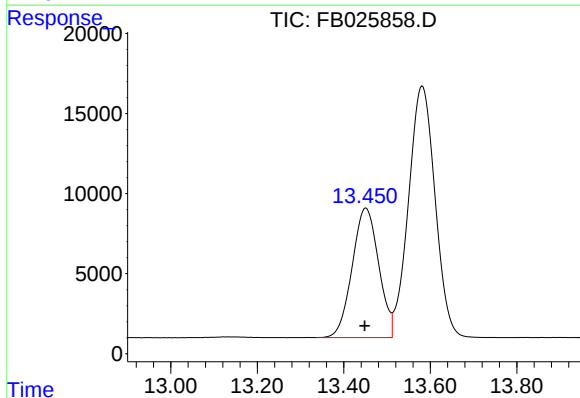


#7 Ethylbenzene

R.T.: 13.451 min
Delta R.T.: 0.003 min
Response: 343447
Conc: 9.01 ng/ml

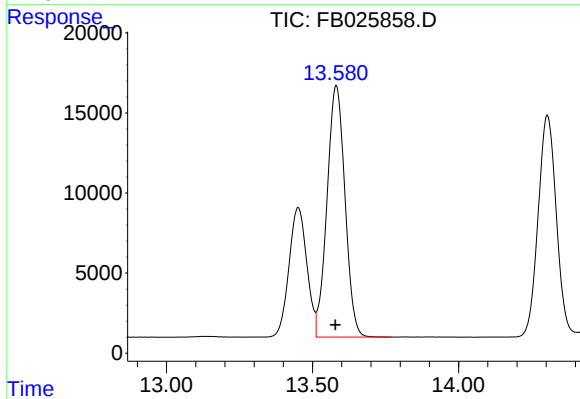

#8 m-Xylene


R.T.: 13.582 min
Delta R.T.: 0.003 min
Response: 671694
Conc: 17.09 ng/ml

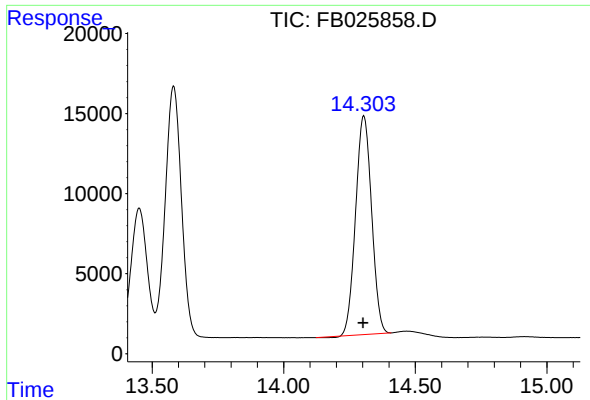

#9 O-Xylene

R.T.: 14.305 min
Delta R.T.: 0.004 min
Response: 576134
Conc: 18.07 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0609S1

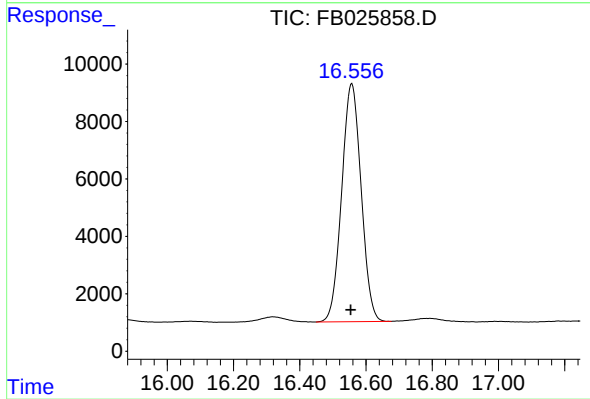

#10 1,2,4-Trimethylbenzene

R.T.: 16.557 min
Delta R.T.: 0.004 min
Response: 337985
Conc: 17.17 ng/ml