

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060921\
 Data File : FB025862.D
 Signal(s) : FID2B.CH
 Acq On : 9 Jun 2021 18:05
 Operator : DD/AJ
 Sample : M2638-02MS
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 ND-1MS

Integration File: Calibration.e
 Quant Time: Jun 10 01:08:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
 Quant Title :
 QLast Update : Wed Jun 09 13:39:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.235	449668	18.607 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.208	716003	27.207 ng/ml
2) t 2,2,4-Trimethylpentane	7.898	499575	24.799 ng/ml
3) t n-Heptane	8.212	319283	8.882 ng/ml
4) t Benzene	8.364	408303	9.781 ng/ml
6) t Toluene	11.051	1116585	27.134 ng/ml
7) t Ethylbenzene	13.455	331532	8.699 ng/ml
8) t m-Xylene	13.585	650271	16.541 ng/ml
9) t O-Xylene	14.307	576005	18.065 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	317524	16.132 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060921\
Data File : FB025862.D
Signal(s) : FID2B.CH
Acq On : 9 Jun 2021 18:05
Operator : DD/AJ
Sample : M2638-02MS
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
ND-1MS

Integration File: Calibration.e
Quant Time: Jun 10 01:08:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

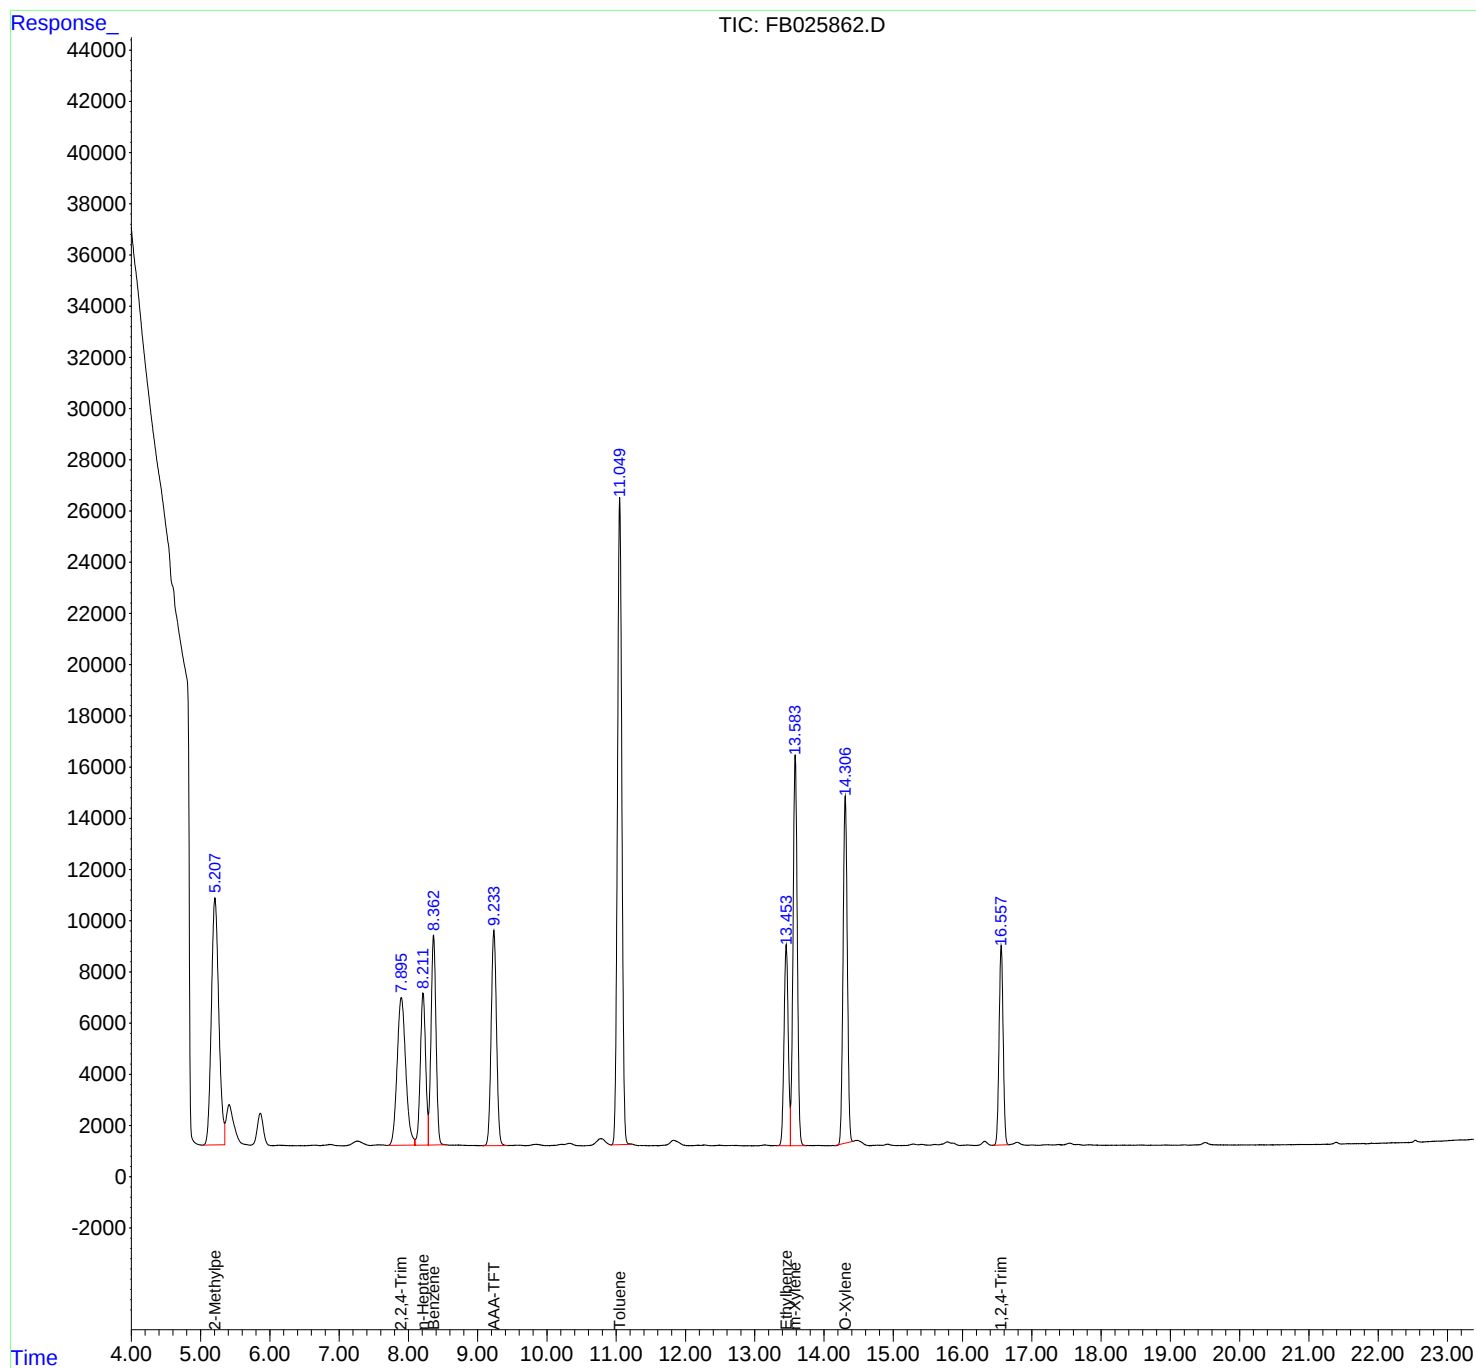


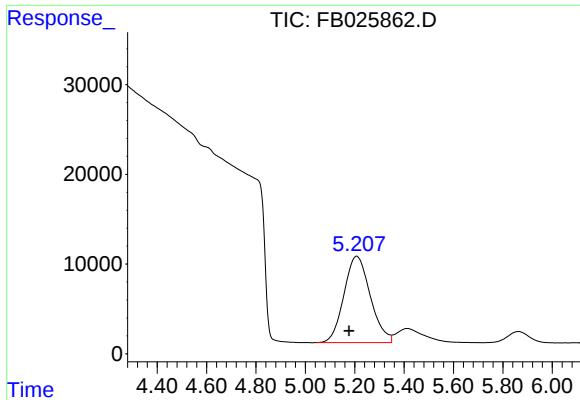

#1 2-Methylpentane


R.T.: 5.208 min
Delta R.T.: 0.032 min
Response: 716003
Conc: 27.21 ng/ml

Instrument :
FID_B
ClientSampleId :
ND-1MS

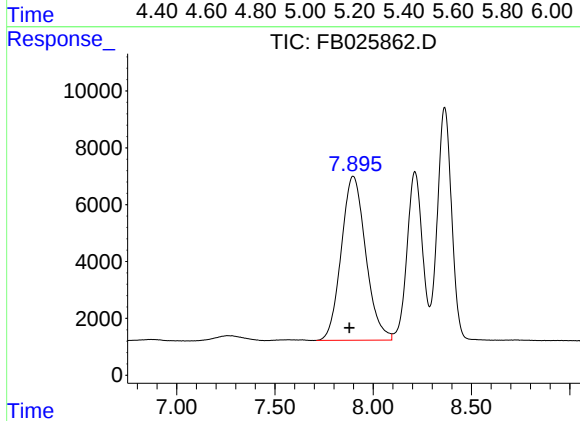


#2 2,2,4-Trimethylpentane

R.T.: 7.898 min
Delta R.T.: 0.020 min
Response: 499575
Conc: 24.80 ng/ml

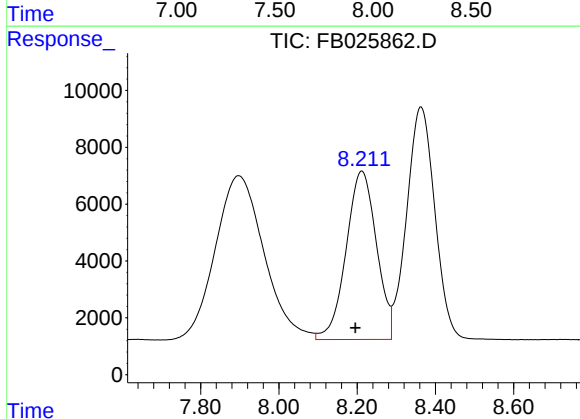


#3 n-Heptane

R.T.: 8.212 min
Delta R.T.: 0.016 min
Response: 319283
Conc: 8.88 ng/ml

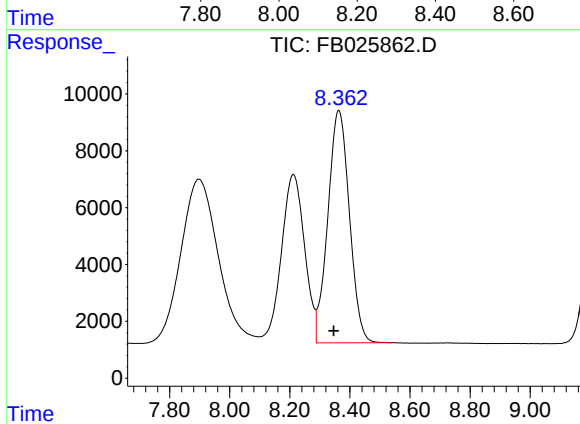

#4 Benzene


R.T.: 8.364 min
Delta R.T.: 0.017 min
Response: 408303
Conc: 9.78 ng/ml

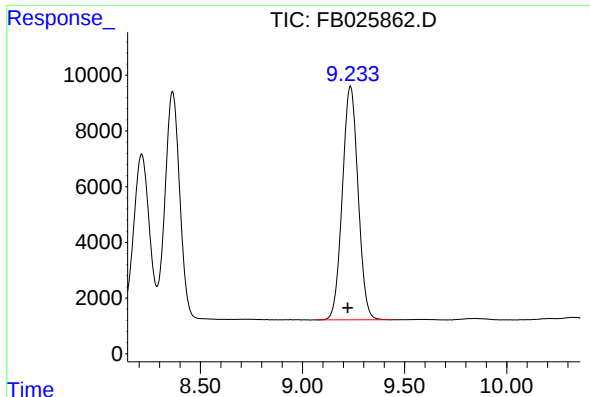

#5 AAA-TFT


R.T.: 9.235 min
Delta R.T.: 0.014 min
Response: 449668
Conc: 18.61 ng/ml

Instrument :
FID_B
ClientSampleId :
ND-1MS

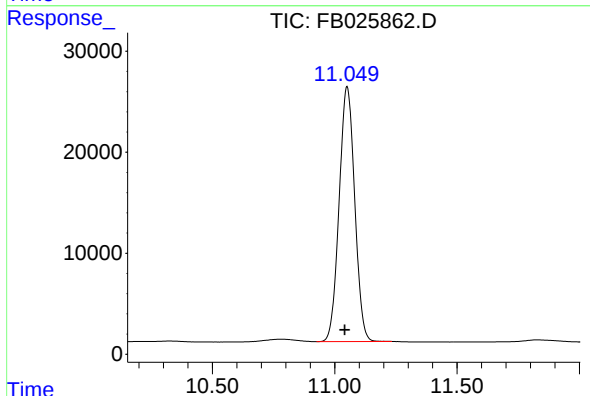


#6 Toluene

R.T.: 11.051 min
Delta R.T.: 0.010 min
Response: 1116585
Conc: 27.13 ng/ml

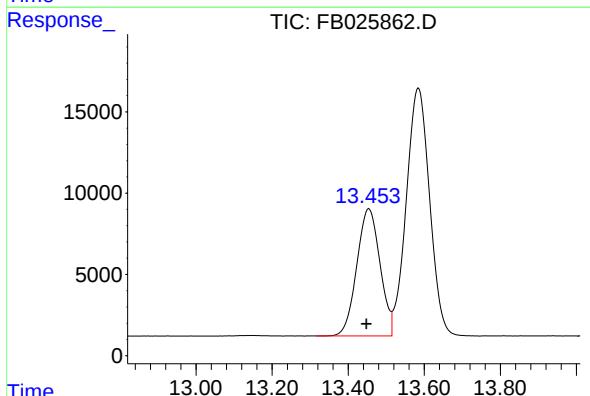


#7 Ethylbenzene

R.T.: 13.455 min
Delta R.T.: 0.006 min
Response: 331532
Conc: 8.70 ng/ml

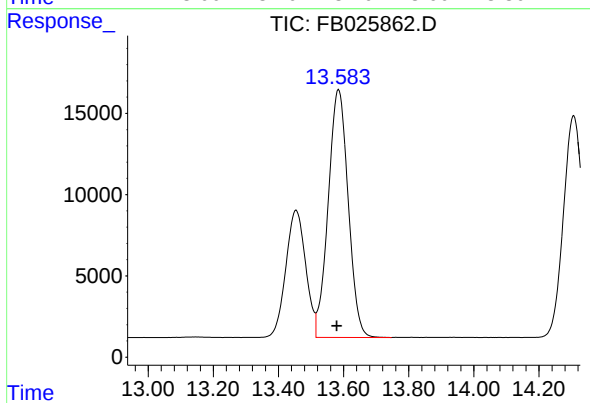

#8 m-Xylene


R.T.: 13.585 min
Delta R.T.: 0.006 min
Response: 650271
Conc: 16.54 ng/ml

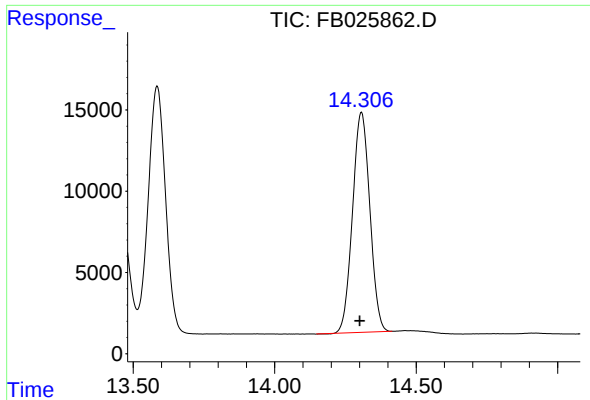

#9 O-Xylene

R.T.: 14.307 min
Delta R.T.: 0.006 min
Response: 576005
Conc: 18.07 ng/ml

Instrument :
FID_B
ClientSampleId :
ND-1MS

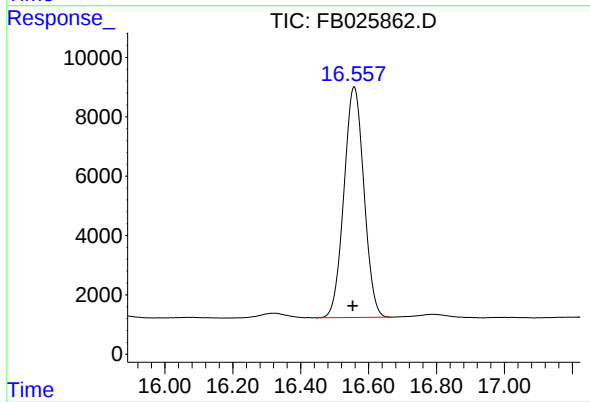

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.005 min
Response: 317524
Conc: 16.13 ng/ml