

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060921\
 Data File : FB025863.D
 Signal(s) : FID2B.CH
 Acq On : 9 Jun 2021 18:40
 Operator : DD/AJ
 Sample : M2638-02MSD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 ND-1MSD

Integration File: Calibration.e
 Quant Time: Jun 10 01:08:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
 Quant Title :
 QLast Update : Wed Jun 09 13:39:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.231	474535	19.636 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.197	689742	26.209 ng/ml
2) t 2,2,4-Trimethylpentane	7.894	470414	23.351 ng/ml
3) t n-Heptane	8.207	302248	8.408 ng/ml
4) t Benzene	8.358	403262	9.660 ng/ml
6) t Toluene	11.049	1095684	26.626 ng/ml
7) t Ethylbenzene	13.453	323392	8.485 ng/ml
8) t m-Xylene	13.583	631847	16.073 ng/ml
9) t O-Xylene	14.306	566966	17.782 ng/ml
10) t 1,2,4-Trimethylbenzene	16.557	304040	15.447 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060921\
Data File : FB025863.D
Signal(s) : FID2B.CH
Acq On : 9 Jun 2021 18:40
Operator : DD/AJ
Sample : M2638-02MSD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
ND-1MSD

Integration File: Calibration.e
Quant Time: Jun 10 01:08:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

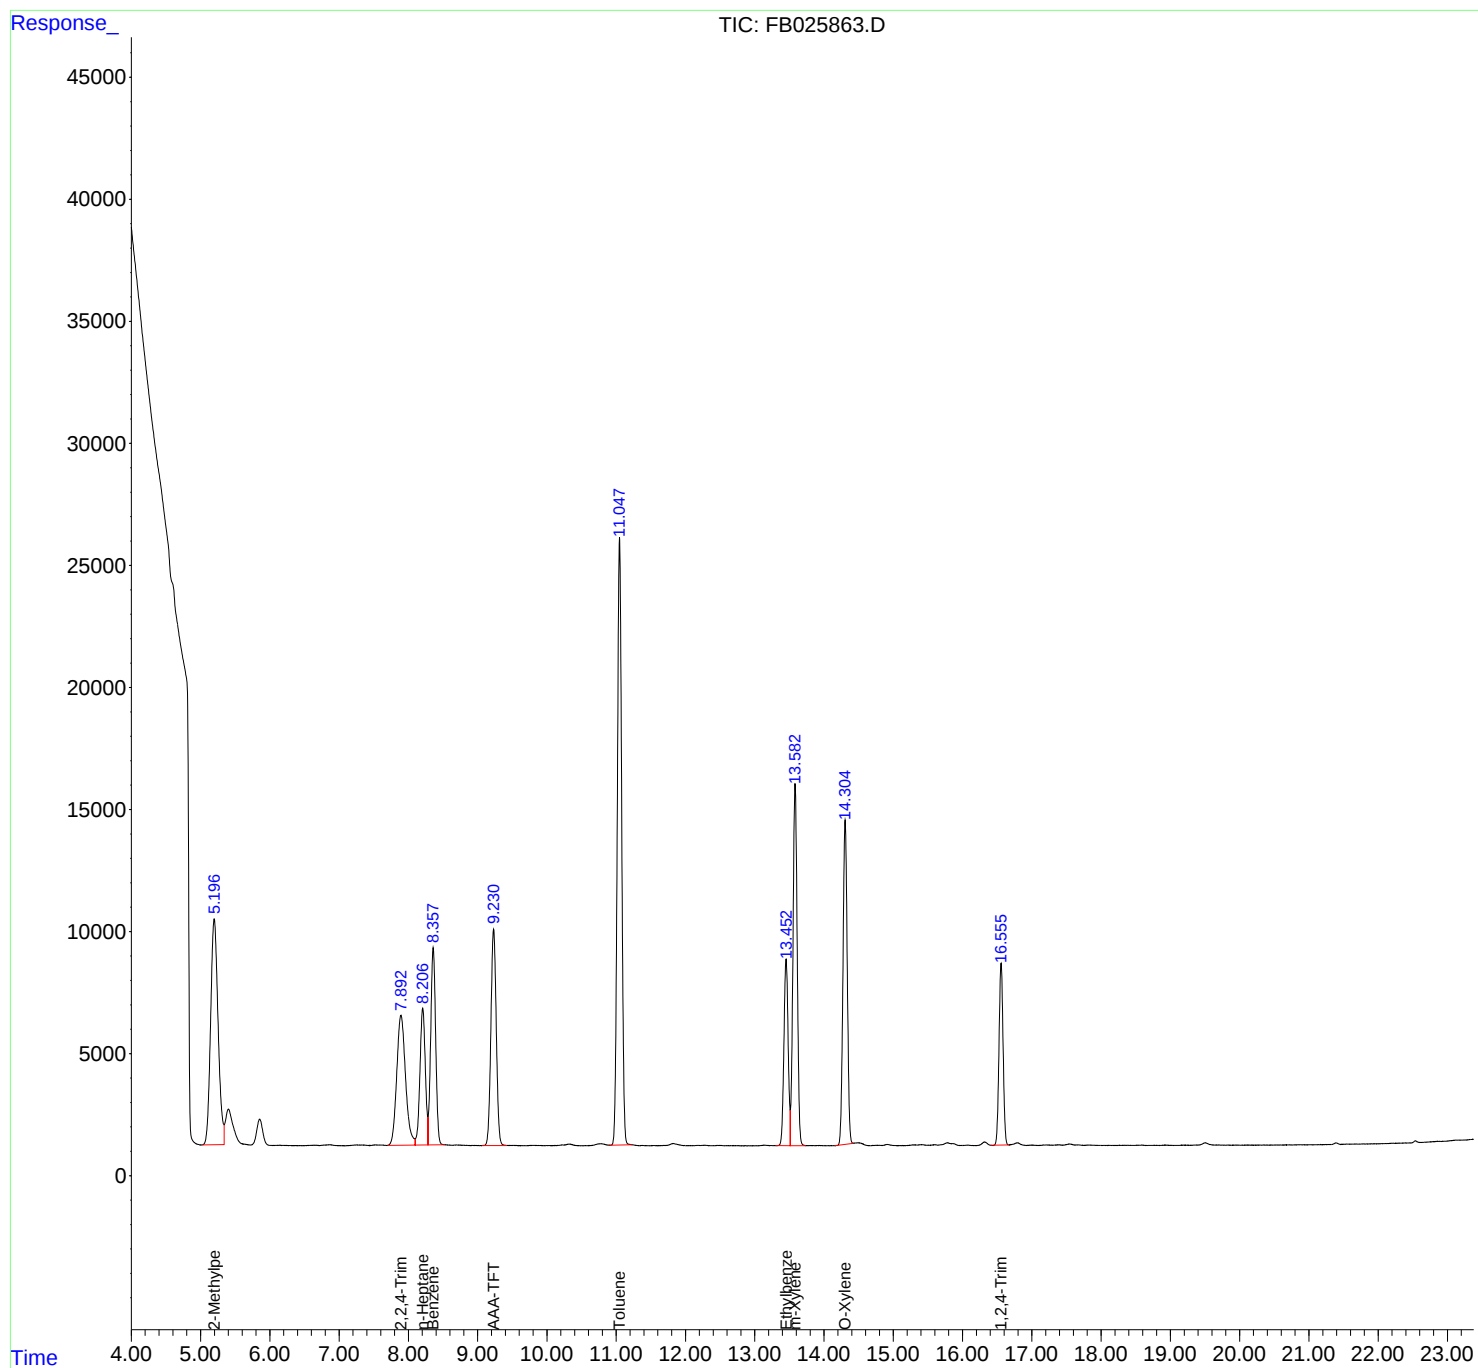


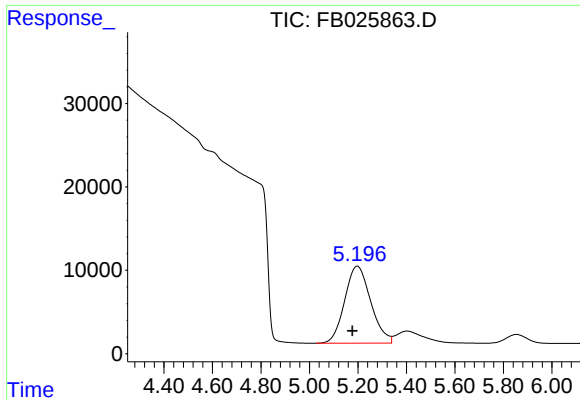

#1 2-Methylpentane


R.T.: 5.197 min
Delta R.T.: 0.020 min
Response: 689742
Conc: 26.21 ng/ml

Instrument :
FID_B
ClientSampleId :
ND-1MSD

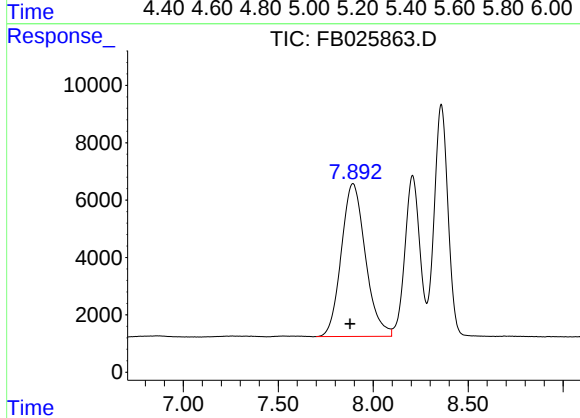


#2 2,2,4-Trimethylpentane

R.T.: 7.894 min
Delta R.T.: 0.016 min
Response: 470414
Conc: 23.35 ng/ml

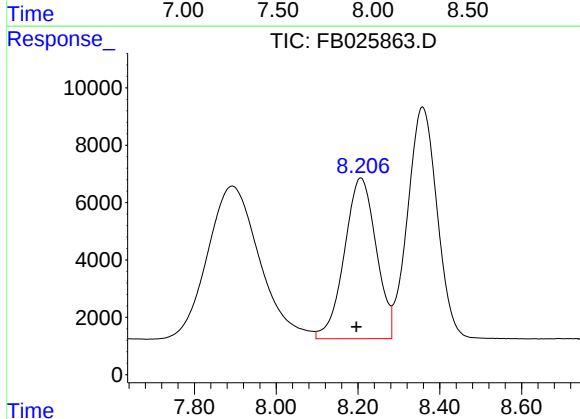


#3 n-Heptane

R.T.: 8.207 min
Delta R.T.: 0.011 min
Response: 302248
Conc: 8.41 ng/ml

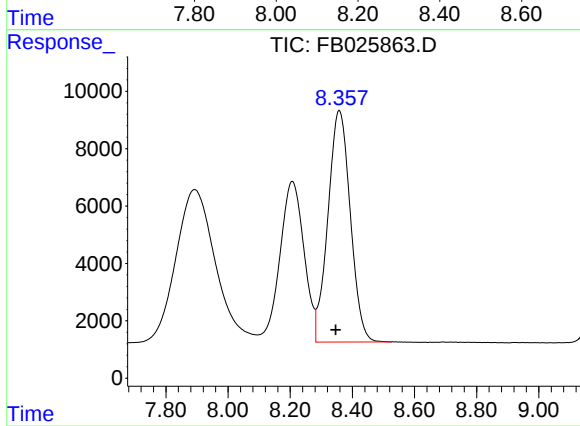

#4 Benzene


R.T.: 8.358 min
Delta R.T.: 0.012 min
Response: 403262
Conc: 9.66 ng/ml

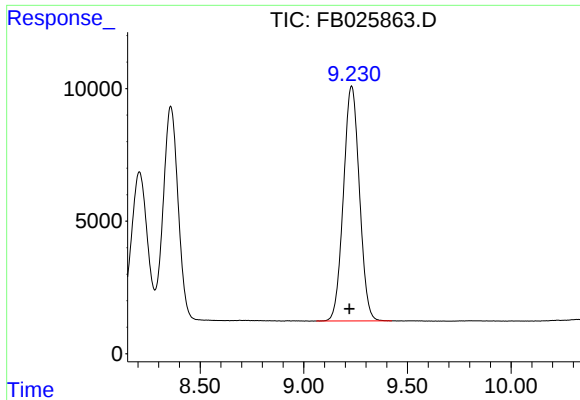

#5 AAA-TFT


R.T.: 9.231 min
Delta R.T.: 0.010 min
Response: 474535
Conc: 19.64 ng/ml

Instrument :
FID_B
ClientSampleId :
ND-1MSD

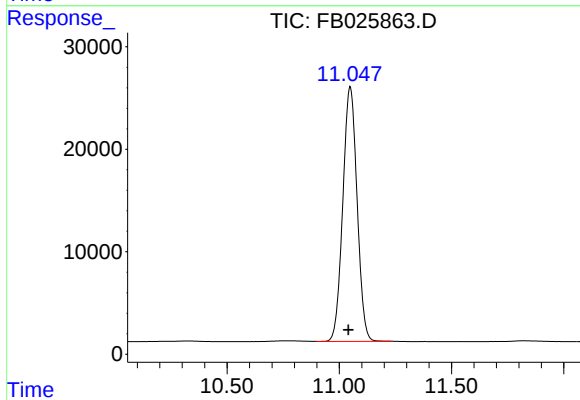


#6 Toluene

R.T.: 11.049 min
Delta R.T.: 0.008 min
Response: 1095684
Conc: 26.63 ng/ml

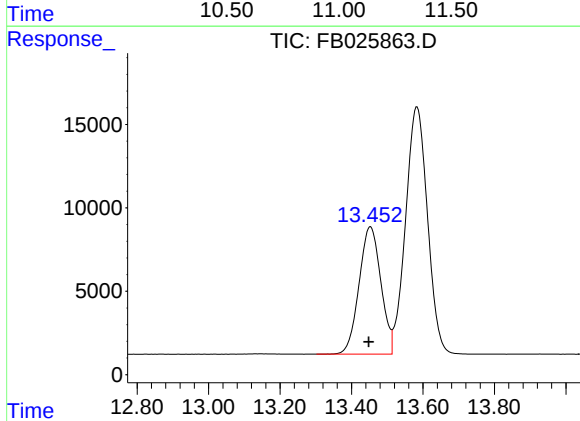


#7 Ethylbenzene

R.T.: 13.453 min
Delta R.T.: 0.005 min
Response: 323392
Conc: 8.49 ng/ml

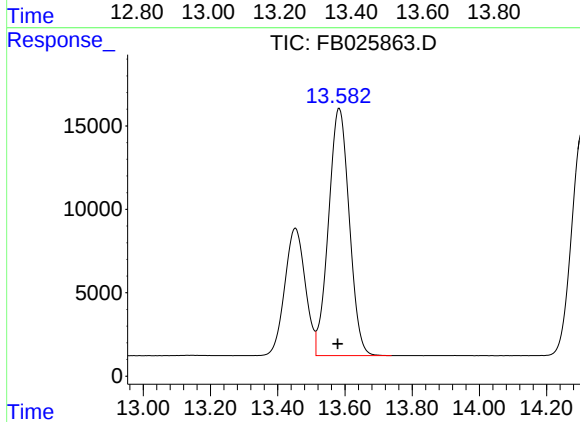

#8 m-Xylene


R.T.: 13.583 min
Delta R.T.: 0.005 min
Response: 631847
Conc: 16.07 ng/ml

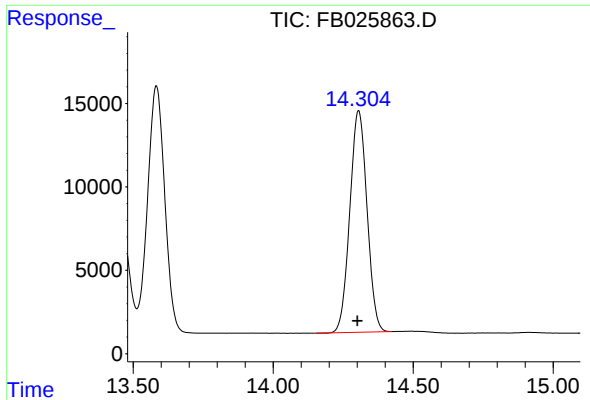

#9 O-Xylene

R.T.: 14.306 min
Delta R.T.: 0.005 min
Response: 566966
Conc: 17.78 ng/ml

Instrument :
FID_B
ClientSampleId :
ND-1MSD

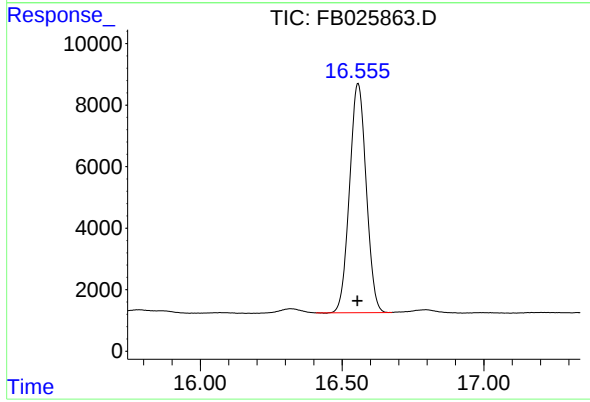

#10 1,2,4-Trimethylbenzene

R.T.: 16.557 min
Delta R.T.: 0.003 min
Response: 304040
Conc: 15.45 ng/ml