

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061019\
 Data File : FB021345.D
 Signal(s) : FID2B.CH
 Acq On : 10 Jun 2019 12:24
 Operator : MJ/SJ
 Sample : K3163-05MS
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 11 01:53:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.993	343115	23.271 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.854	989534	26.322 ng/ml
2) t 2,2,4-Trimethylpentane	7.609	852942	24.976 ng/ml
3) t n-Heptane	7.949	276172	8.471 ng/ml
4) t Benzene	8.086	341647	9.898 ng/ml
6) t Toluene	10.838	718594	30.318 ng/ml
7) t Ethylbenzene	13.288	226308	9.685 ng/ml
8) t m-Xylene	13.421	480857	19.265 ng/ml
9) t O-Xylene	14.152	499027	19.129 ng/ml
10) t 1,2,4-Trimethylbenzene	16.437	495171	18.438 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061019\
Data File : FB021345.D
Signal(s) : FID2B.CH
Acq On : 10 Jun 2019 12:24
Operator : MJ/SJ
Sample : K3163-05MS
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 11 01:53:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

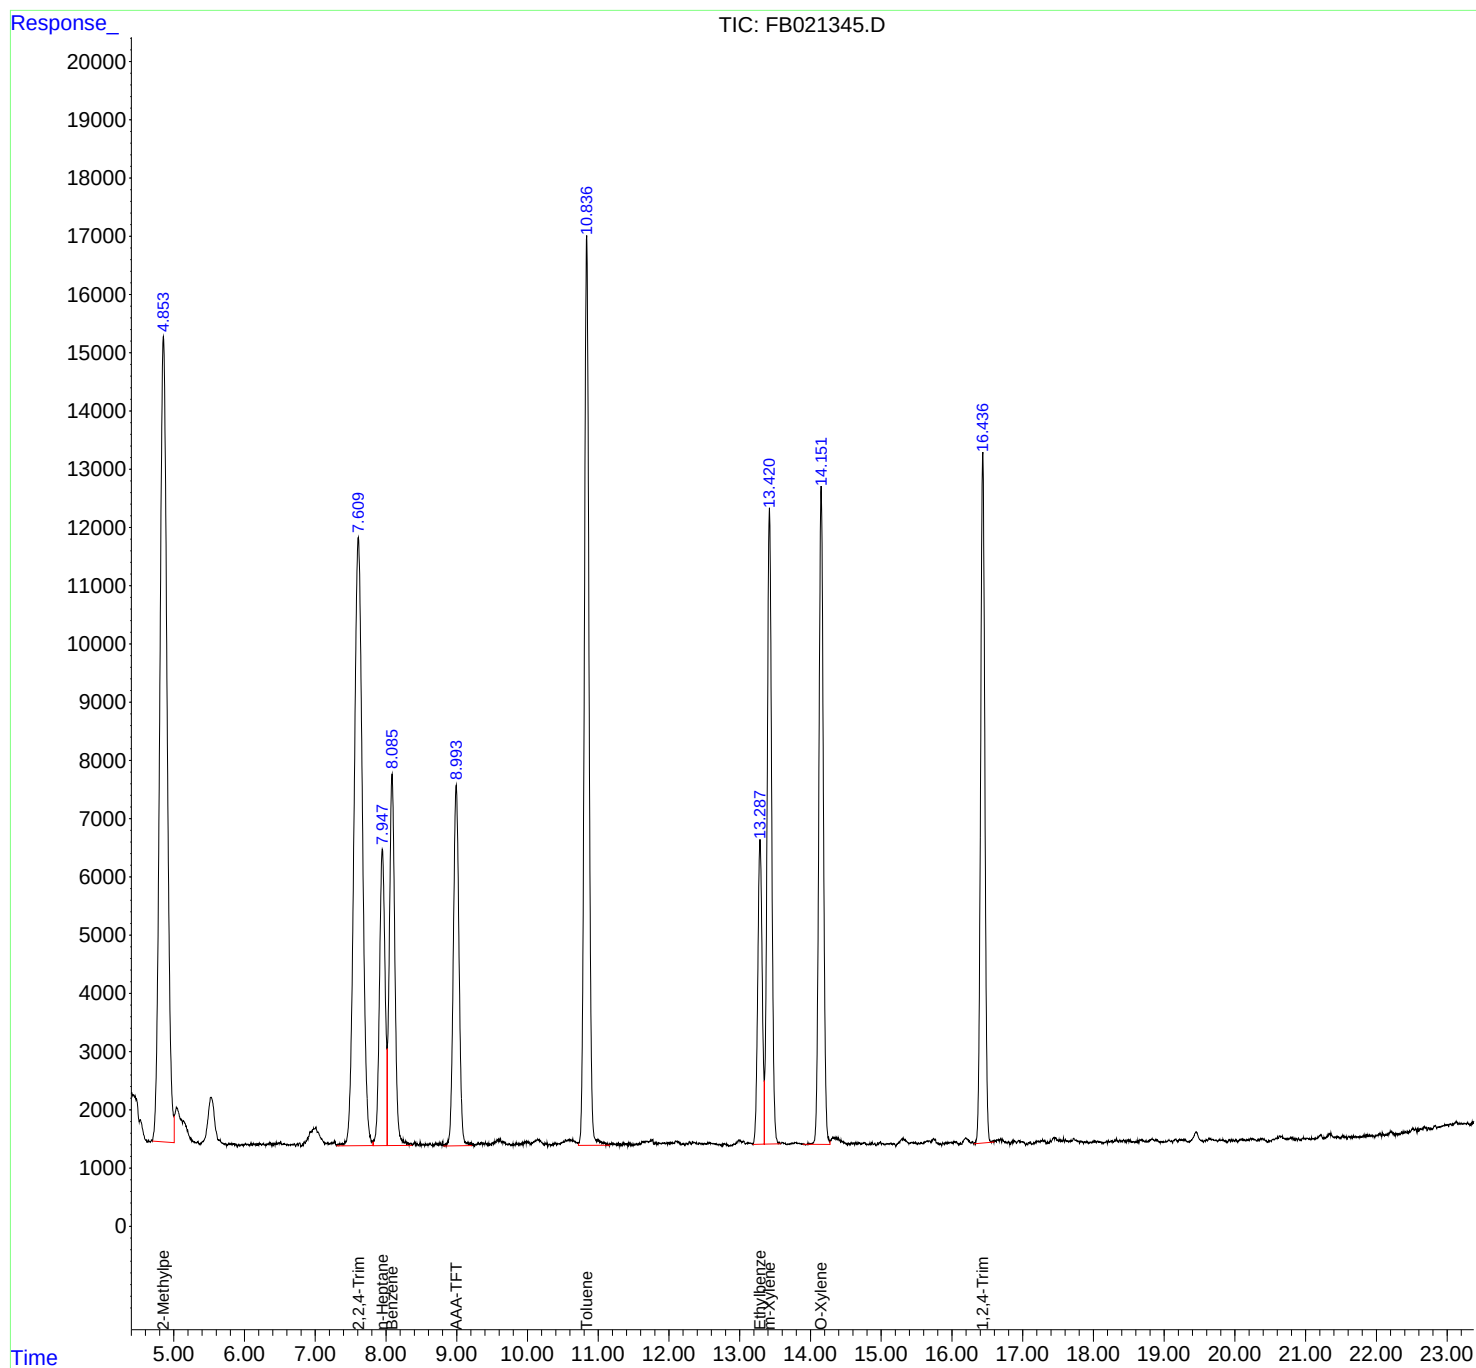

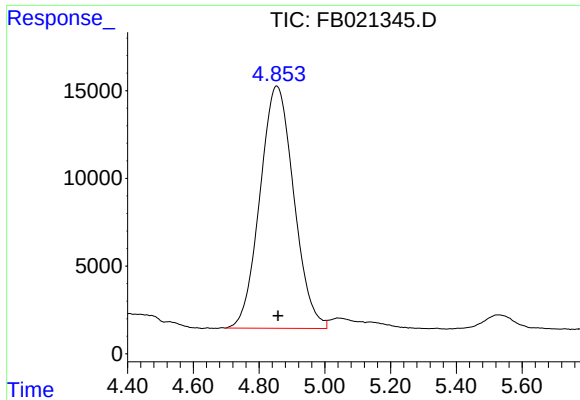


#1 2-Methylpentane

R.T.: 4.854 min
Delta R.T.: -0.004 min
Response: 989534
Conc: 26.32 ng/ml

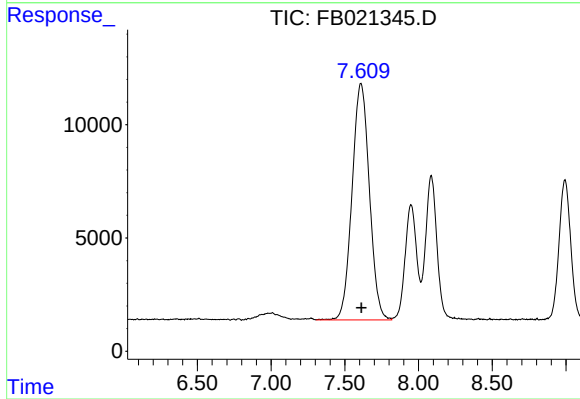


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: -0.005 min
Response: 852942
Conc: 24.98 ng/ml

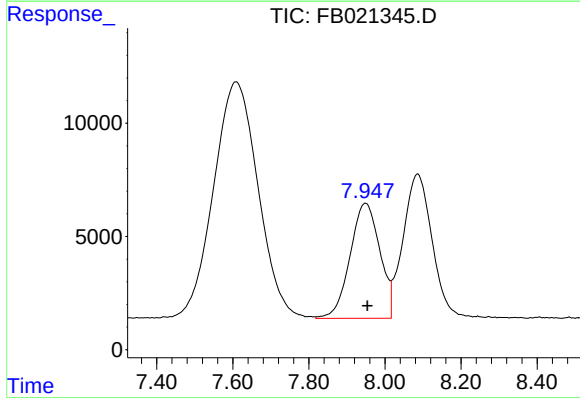


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.005 min
Response: 276172
Conc: 8.47 ng/ml

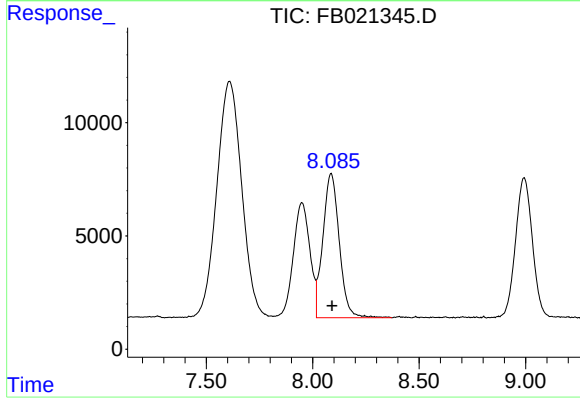


#4 Benzene

R.T.: 8.086 min
Delta R.T.: -0.004 min
Response: 341647
Conc: 9.90 ng/ml

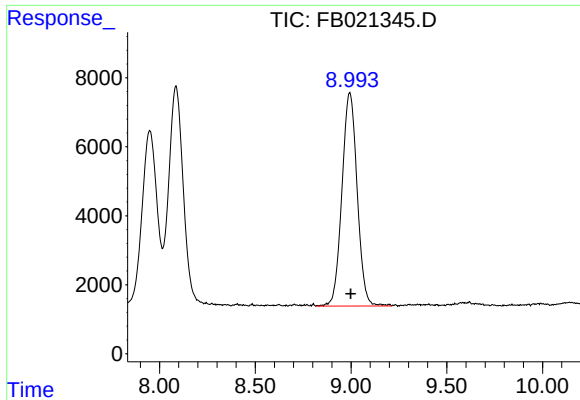


#5 AAA-TFT

R.T.: 8.993 min
Delta R.T.: -0.005 min
Response: 343115
Conc: 23.27 ng/ml

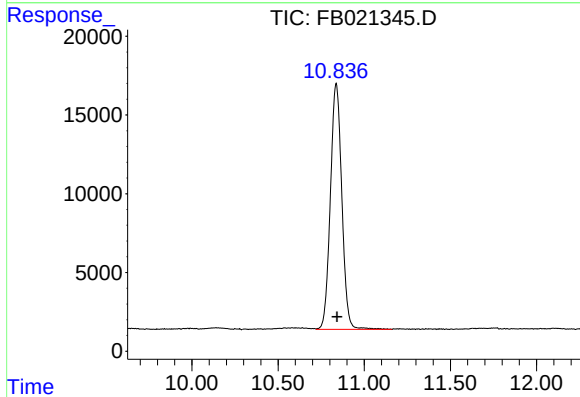


#6 Toluene

R.T.: 10.838 min
Delta R.T.: -0.005 min
Response: 718594
Conc: 30.32 ng/ml

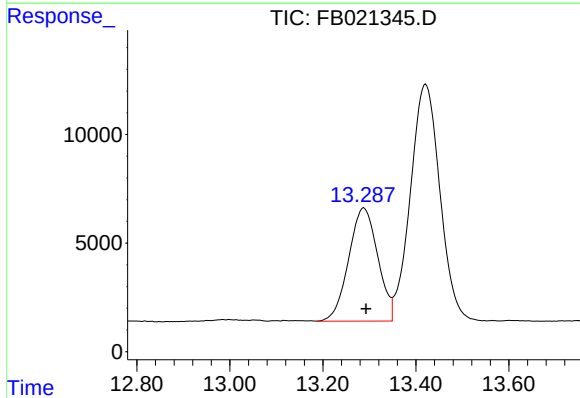


#7 Ethylbenzene

R.T.: 13.288 min
Delta R.T.: -0.005 min
Response: 226308
Conc: 9.68 ng/ml

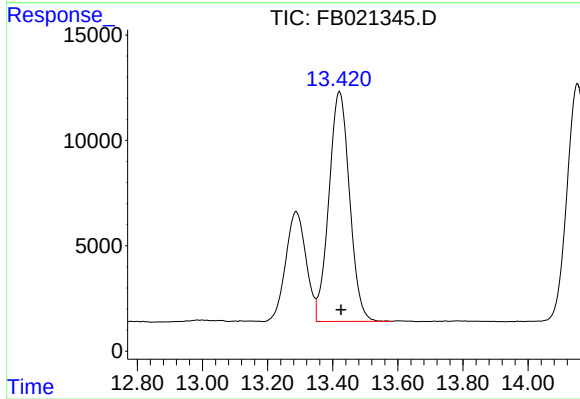


#8 m-Xylene

R.T.: 13.421 min
Delta R.T.: -0.005 min
Response: 480857
Conc: 19.27 ng/ml

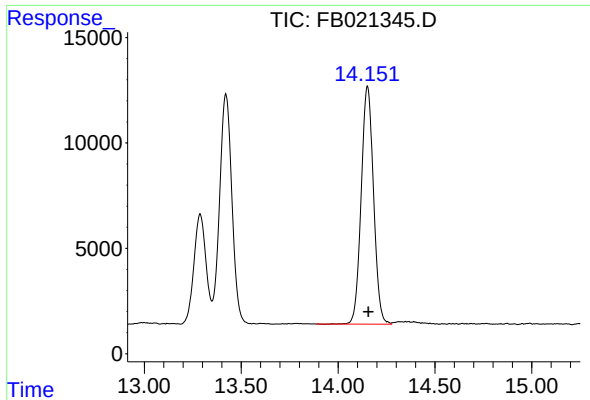

#9 O-Xylene

R.T.: 14.152 min
Delta R.T.: -0.005 min
Response: 499027
Conc: 19.13 ng/ml

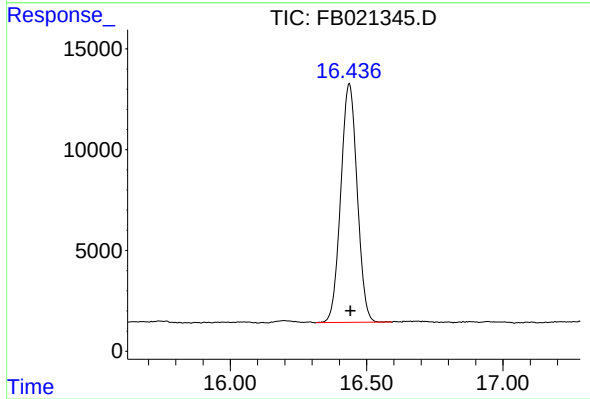

#10 1,2,4-Trimethylbenzene

R.T.: 16.437 min
Delta R.T.: -0.004 min
Response: 495171
Conc: 18.44 ng/ml