

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061019\
 Data File : FB021346.D
 Signal(s) : FID2B.CH
 Acq On : 10 Jun 2019 12:54
 Operator : MJ/SJ
 Sample : K3163-05MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 11 01:53:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.994	313255	21.246 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.858	882235	23.468 ng/ml
2) t	2,2,4-Trimethylpentane	7.609	756757	22.160 ng/ml
3) t	n-Heptane	7.951	241020	7.393 ng/ml
4) t	Benzene	8.088	302840	8.774 ng/ml
6) t	Toluene	10.839	664830	28.049 ng/ml
7) t	Ethylbenzene	13.289	225702	9.659 ng/ml
8) t	m-Xylene	13.422	476948	19.108 ng/ml
9) t	O-Xylene	14.153	492928	18.896 ng/ml
10) t	1,2,4-Trimethylbenzene	16.437	468268	17.437 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061019\
Data File : FB021346.D
Signal(s) : FID2B.CH
Acq On : 10 Jun 2019 12:54
Operator : MJ/SJ
Sample : K3163-05MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 11 01:53:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

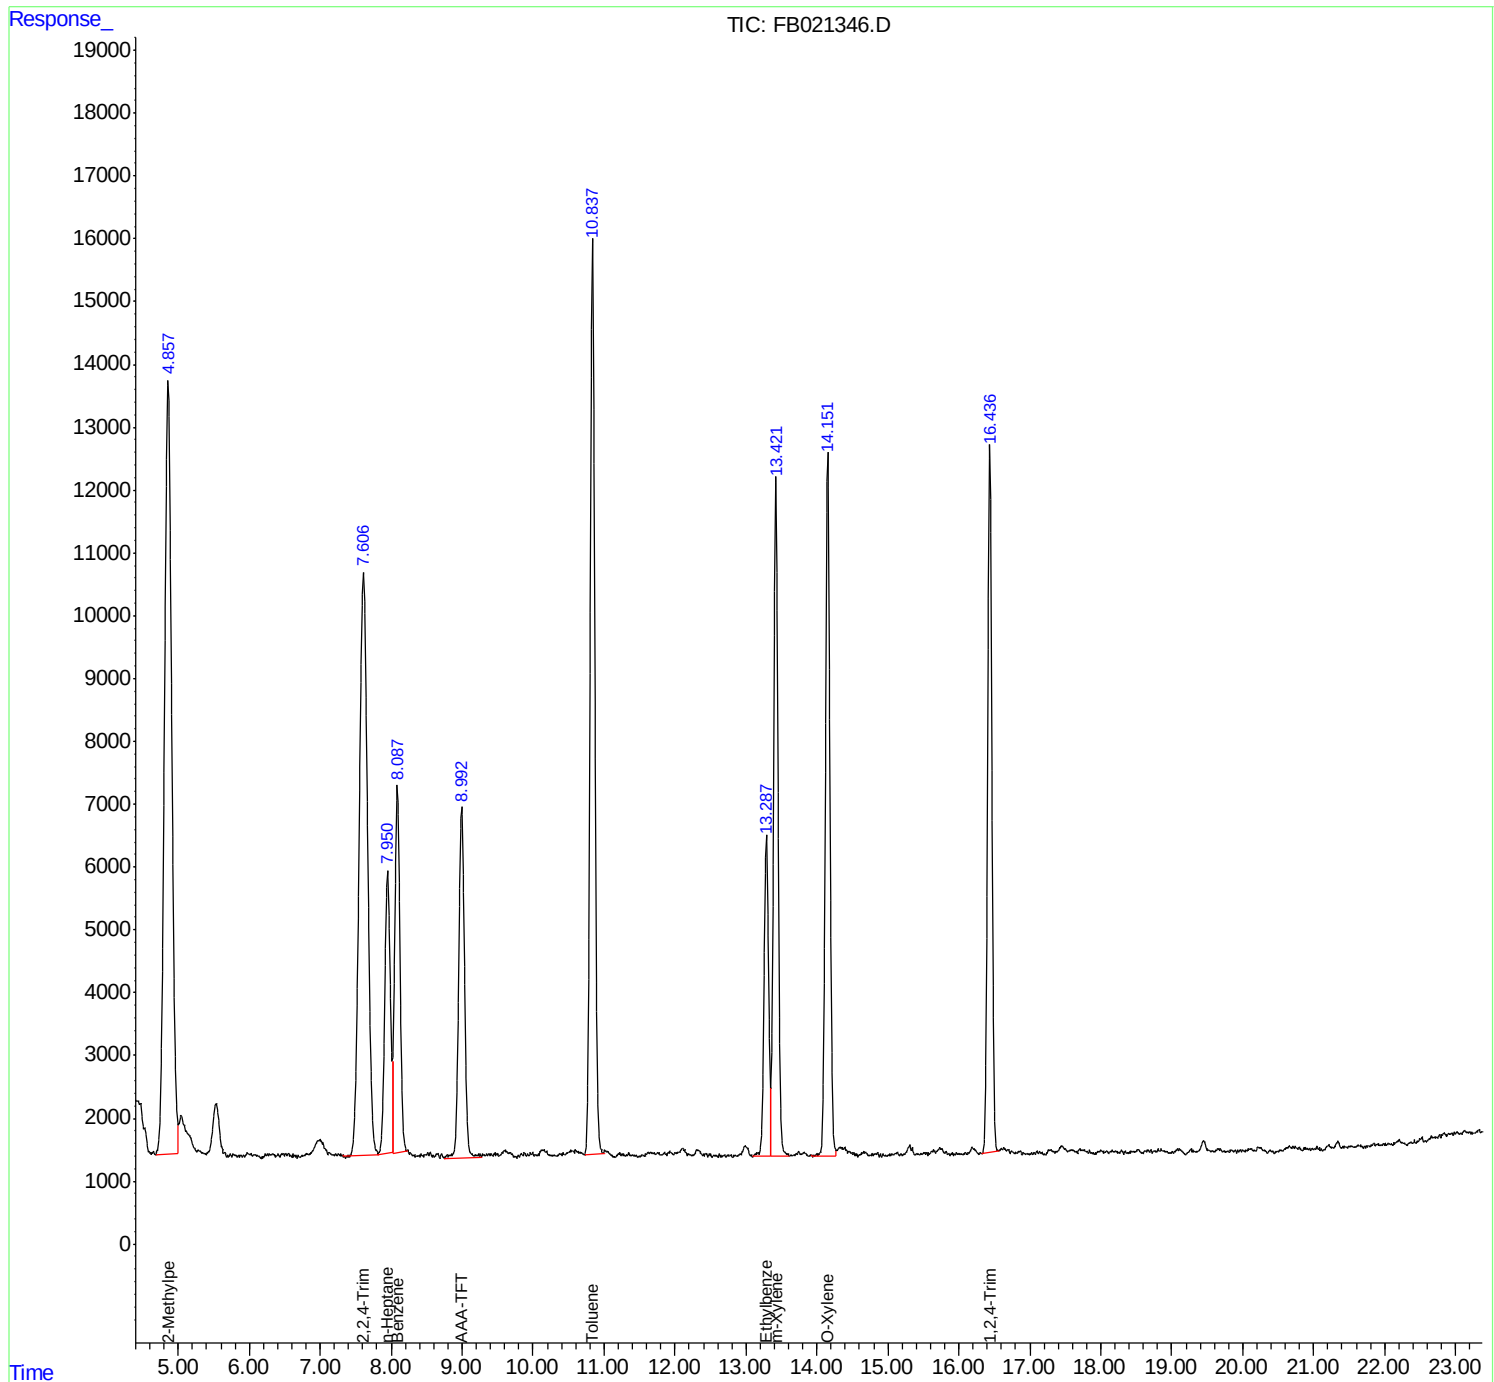

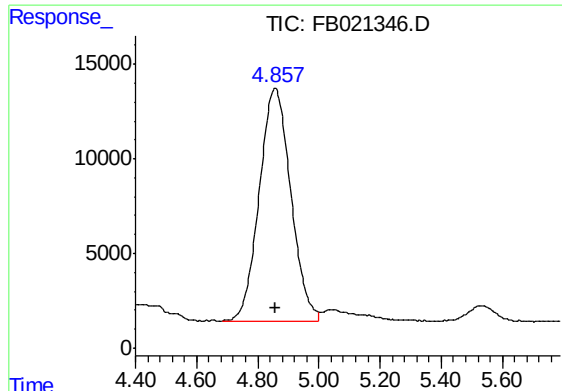


#1 2-Methylpentane

R.T.: 4.858 min
Delta R.T.: 0.000 min
Response: 882235
Conc: 23.47 ng/ml

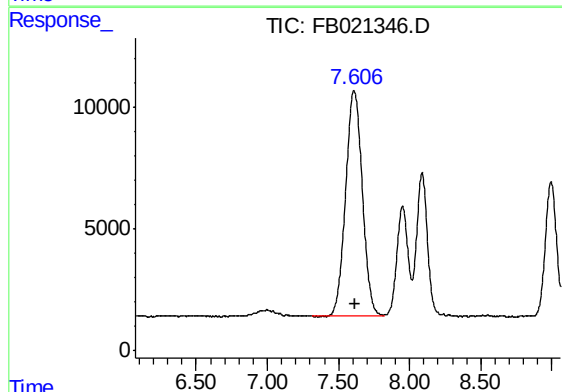


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: -0.005 min
Response: 756757
Conc: 22.16 ng/ml

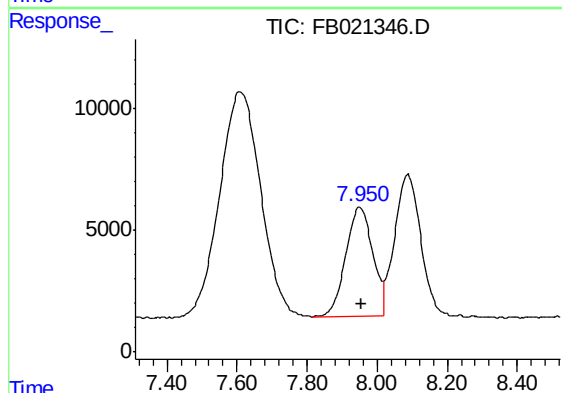


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: -0.004 min
Response: 241020
Conc: 7.39 ng/ml

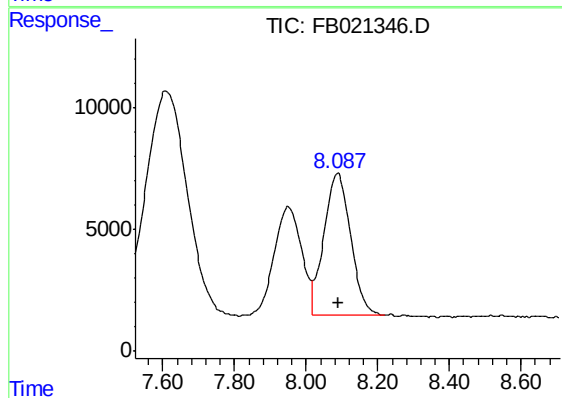


#4 Benzene

R.T.: 8.088 min
Delta R.T.: -0.002 min
Response: 302840
Conc: 8.77 ng/ml

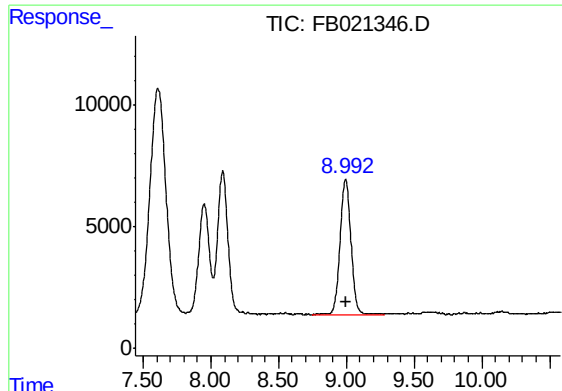


#5 AAA-TFT

R.T.: 8.994 min
Delta R.T.: -0.004 min
Response: 313255
Conc: 21.25 ng/ml

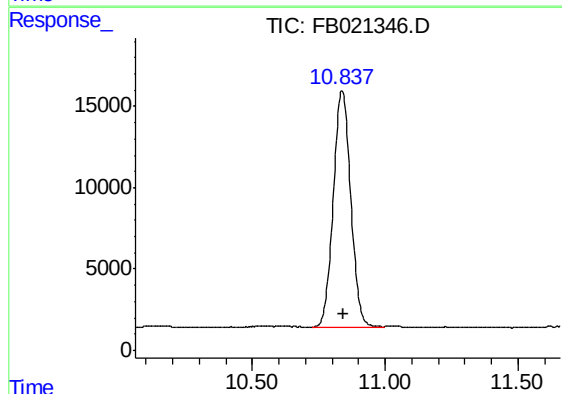


#6 Toluene

R.T.: 10.839 min
Delta R.T.: -0.004 min
Response: 664830
Conc: 28.05 ng/ml

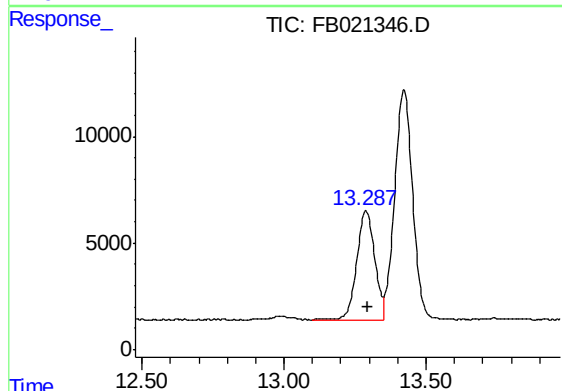


#7 Ethylbenzene

R.T.: 13.289 min
Delta R.T.: -0.004 min
Response: 225702
Conc: 9.66 ng/ml

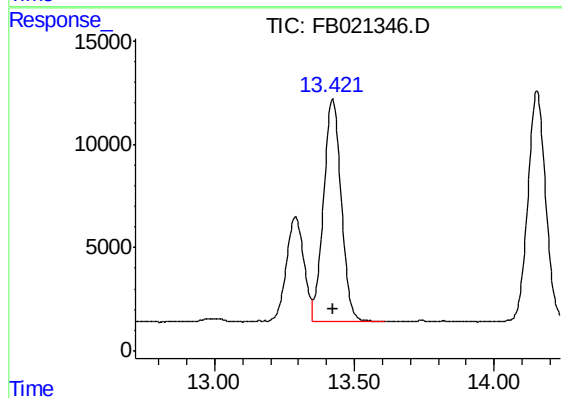


#8 m-Xylene

R.T.: 13.422 min
Delta R.T.: -0.004 min
Response: 476948
Conc: 19.11 ng/ml

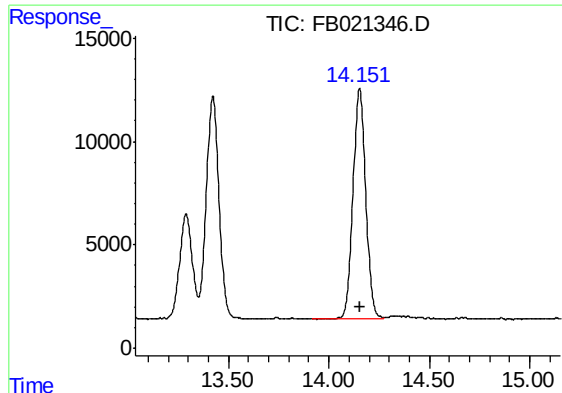

#9 O-Xylene

R.T.: 14.153 min
Delta R.T.: -0.004 min
Response: 492928
Conc: 18.90 ng/ml

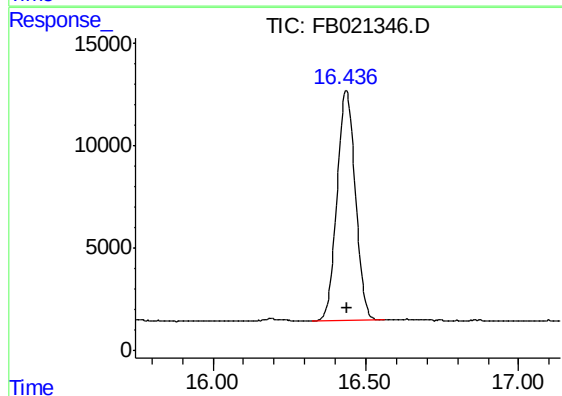

#10 1,2,4-Trimethylbenzene

R.T.: 16.437 min
Delta R.T.: -0.004 min
Response: 468268
Conc: 17.44 ng/ml