

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061119\
 Data File : FB021358.D
 Signal(s) : FID2B.CH
 Acq On : 11 Jun 2019 10:52
 Operator : MJ/SJ
 Sample : K3281-01MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 12 04:02:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.997	312821	21.217 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.858	910478	24.219 ng/ml
2) t 2,2,4-Trimethylpentane	7.612	928666	27.193 ng/ml
3) t n-Heptane	7.953	296897	9.107 ng/ml
4) t Benzene	8.091	308697	8.943 ng/ml
6) t Toluene	10.841	722430	30.479 ng/ml
7) t Ethylbenzene	13.291	228602	9.783 ng/ml
8) t m-Xylene	13.425	492912	19.748 ng/ml
9) t O-Xylene	14.155	511128	19.593 ng/ml
10) t 1,2,4-Trimethylbenzene	16.440	514201	19.147 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061119\
Data File : FB021358.D
Signal(s) : FID2B.CH
Acq On : 11 Jun 2019 10:52
Operator : MJ/SJ
Sample : K3281-01MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 12 04:02:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

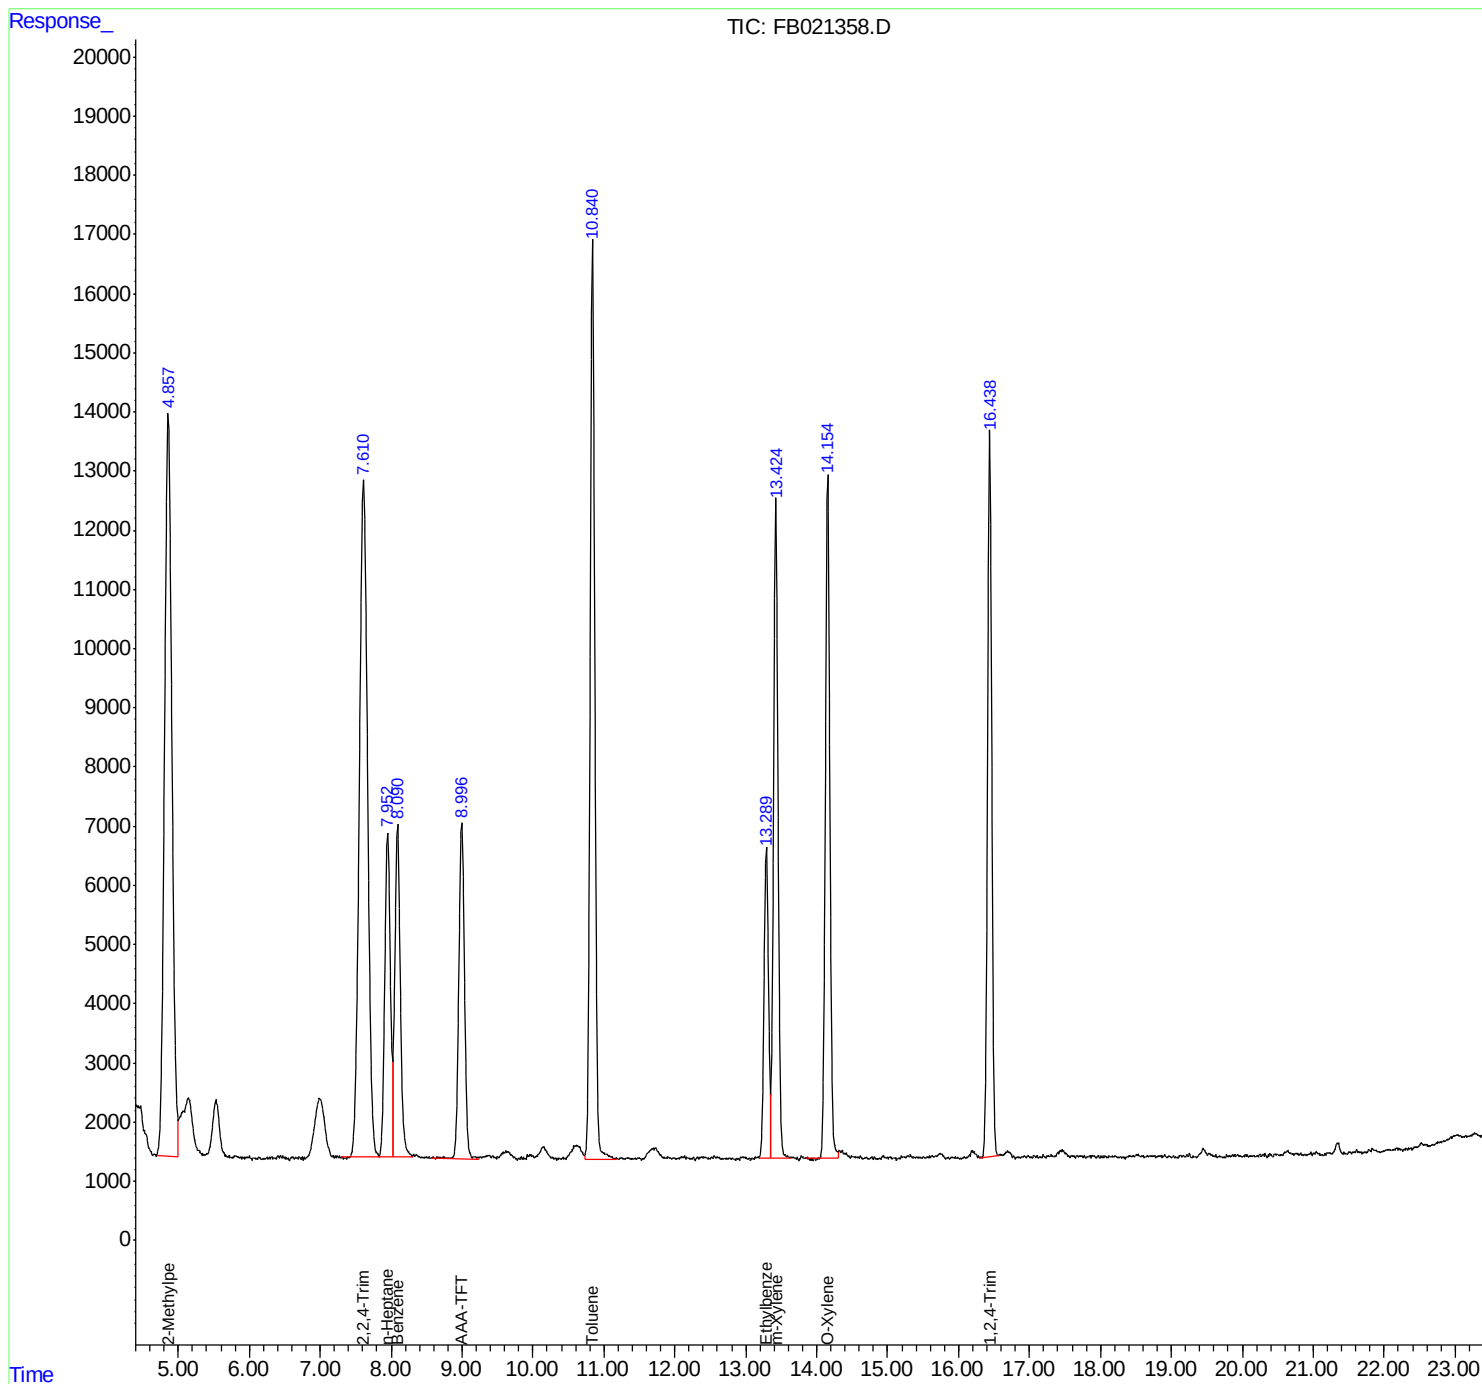

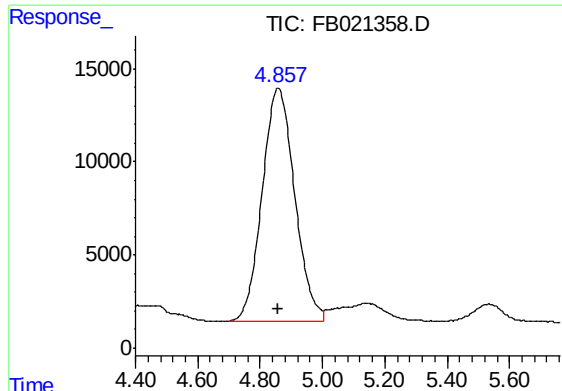


#1 2-Methylpentane

R.T.: 4.858 min
Delta R.T.: 0.000 min
Response: 910478
Conc: 24.22 ng/ml

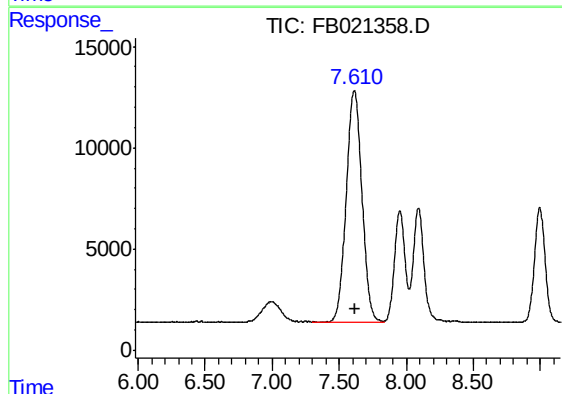


#2 2,2,4-Trimethylpentane

R.T.: 7.612 min
Delta R.T.: -0.002 min
Response: 928666
Conc: 27.19 ng/ml

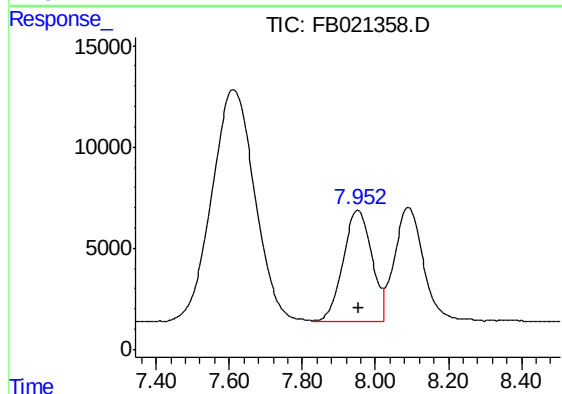


#3 n-Heptane

R.T.: 7.953 min
Delta R.T.: -0.002 min
Response: 296897
Conc: 9.11 ng/ml

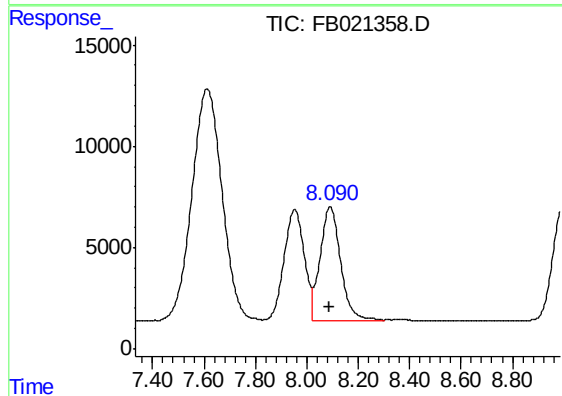


#4 Benzene

R.T.: 8.091 min
Delta R.T.: 0.000 min
Response: 308697
Conc: 8.94 ng/ml

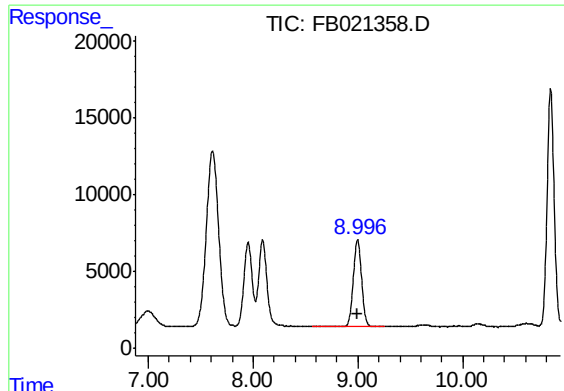


#5 AAA-TFT

R.T.: 8.997 min
Delta R.T.: -0.002 min
Response: 312821
Conc: 21.22 ng/ml

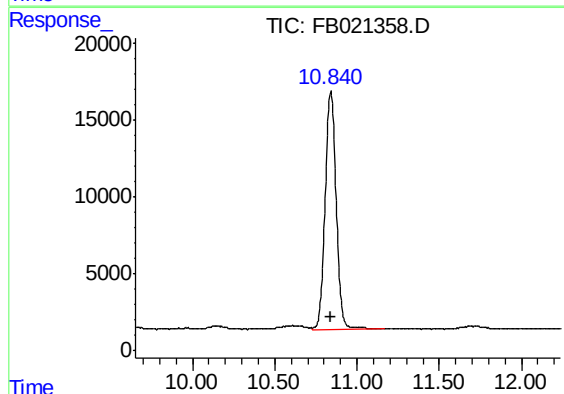


#6 Toluene

R.T.: 10.841 min
Delta R.T.: -0.002 min
Response: 722430
Conc: 30.48 ng/ml

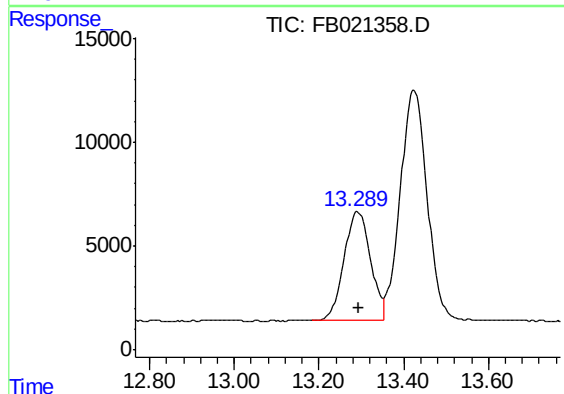


#7 Ethylbenzene

R.T.: 13.291 min
Delta R.T.: -0.002 min
Response: 228602
Conc: 9.78 ng/ml

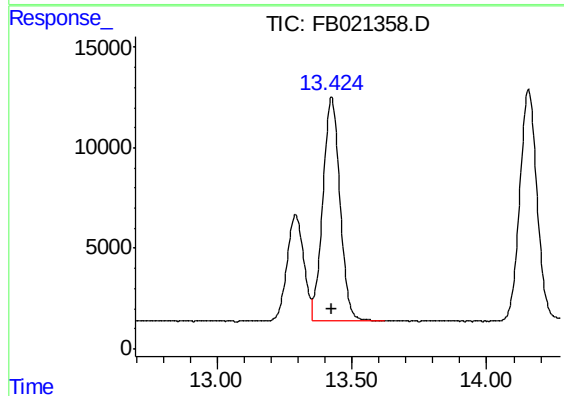


#8 m-Xylene

R.T.: 13.425 min
Delta R.T.: -0.001 min
Response: 492912
Conc: 19.75 ng/ml

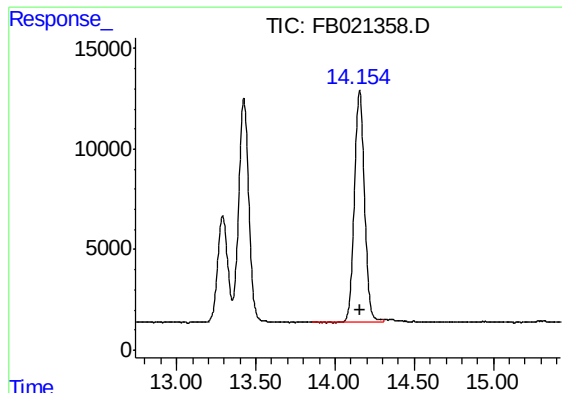

#9 O-Xylene

R.T.: 14.155 min
Delta R.T.: -0.001 min
Response: 511128
Conc: 19.59 ng/ml

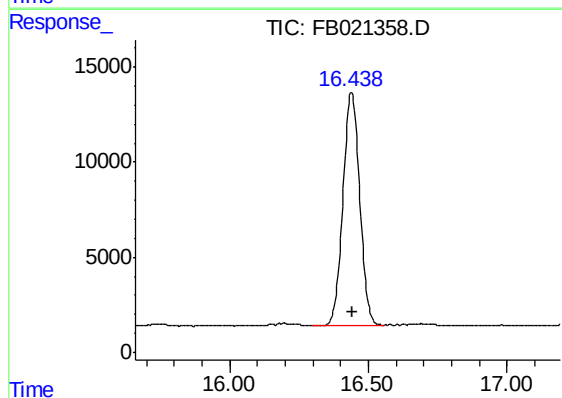

#10 1,2,4-Trimethylbenzene

R.T.: 16.440 min
Delta R.T.: -0.001 min
Response: 514201
Conc: 19.15 ng/ml