

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061119\
 Data File : FB021355.D
 Signal(s) : FID2B.CH
 Acq On : 11 Jun 2019 9:21
 Operator : MJ/SJ
 Sample : BSF0611S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 12 04:02:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.996	310857	21.083 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.857	1010946	26.891 ng/ml
2) t	2,2,4-Trimethylpentane	7.611	1021732	29.919 ng/ml
3) t	n-Heptane	7.951	325501	9.984 ng/ml
4) t	Benzene	8.090	332267	9.626 ng/ml
6) t	Toluene	10.841	743440	31.366 ng/ml
7) t	Ethylbenzene	13.291	241975	10.355 ng/ml
8) t	m-Xylene	13.424	521043	20.875 ng/ml
9) t	O-Xylene	14.156	544359	20.867 ng/ml
10) t	1,2,4-Trimethylbenzene	16.440	543765	20.248 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB061119\
Data File : FB021355.D
Signal(s) : FID2B.CH
Acq On : 11 Jun 2019 9:21
Operator : MJ/SJ
Sample : BSF0611S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 12 04:02:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

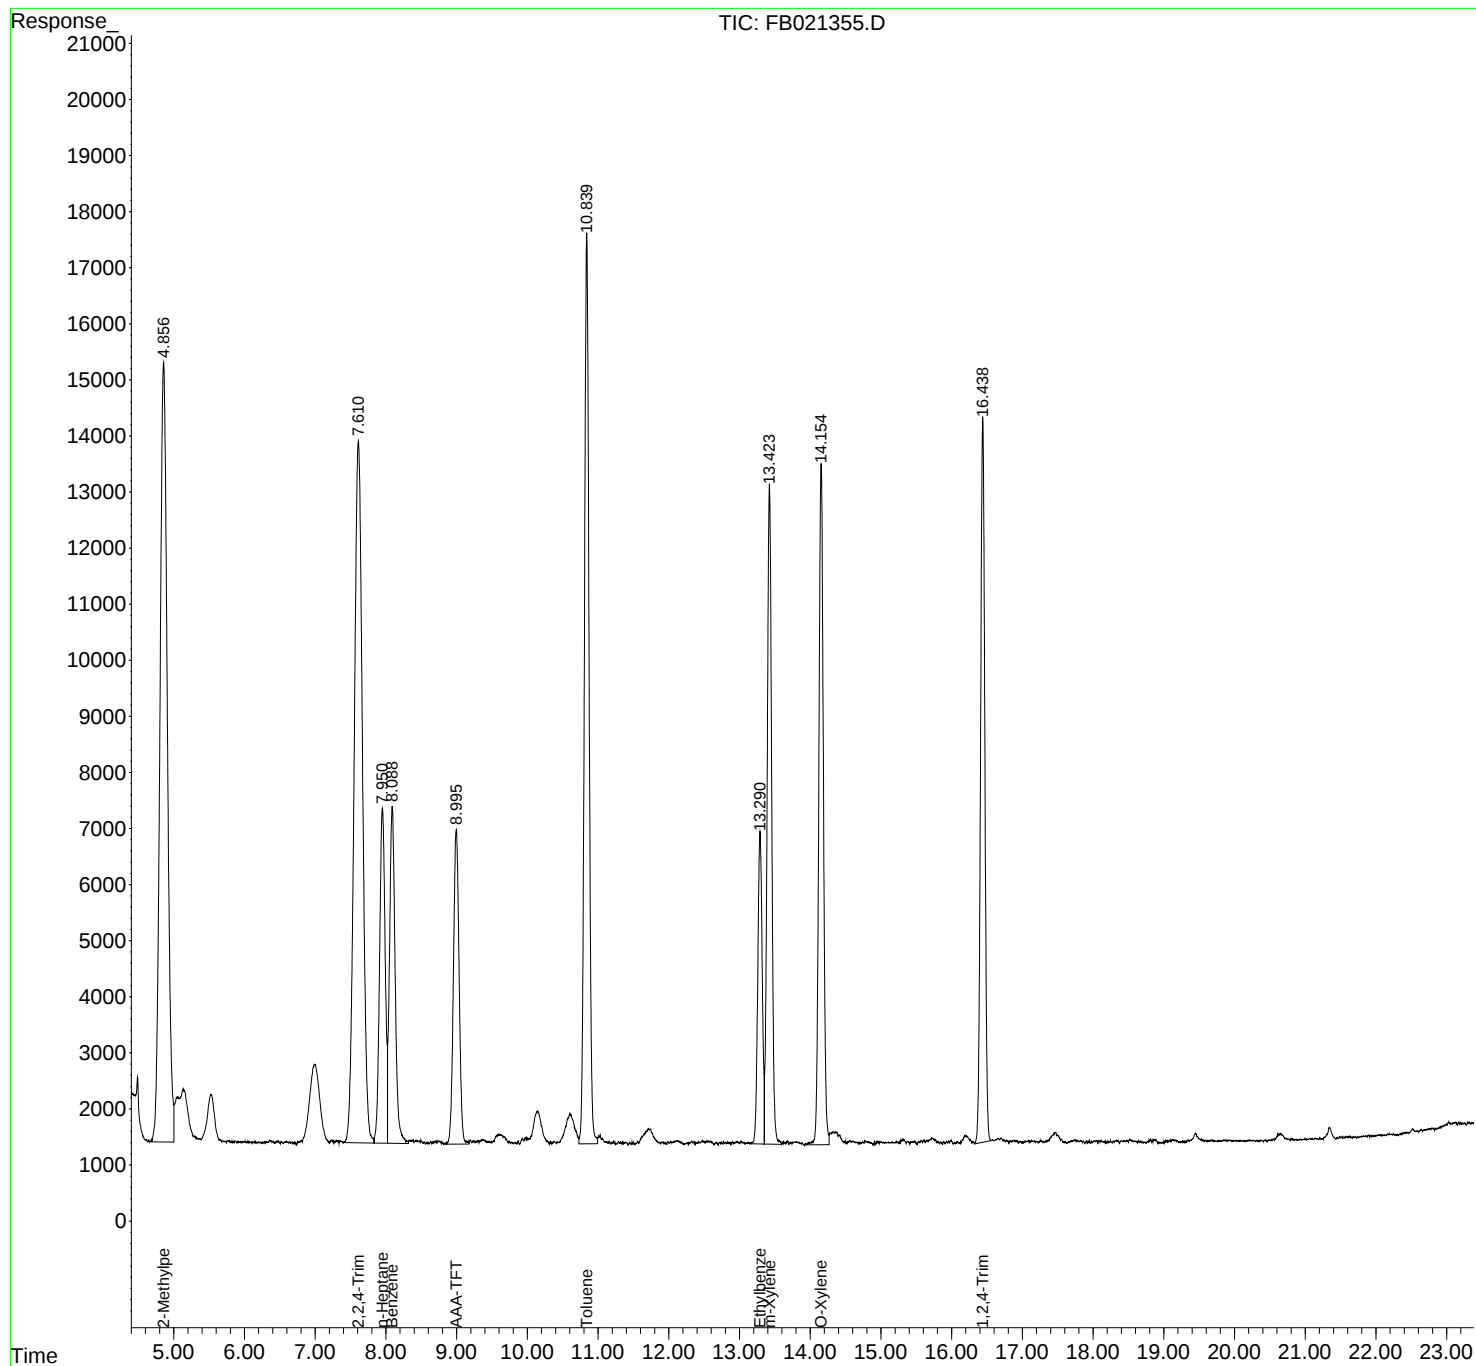

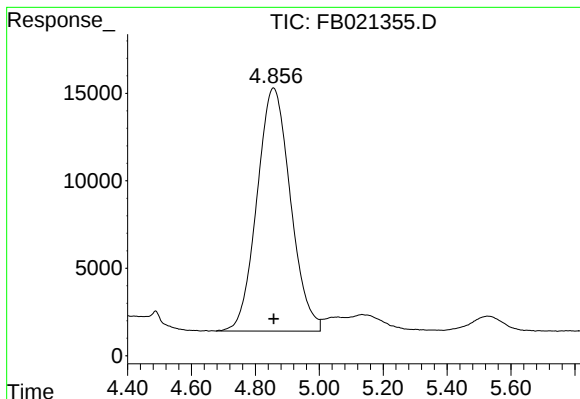


#1 2-Methylpentane

R.T.: 4.857 min
Delta R.T.: 0.000 min
Response: 1010946
Conc: 26.89 ng/ml

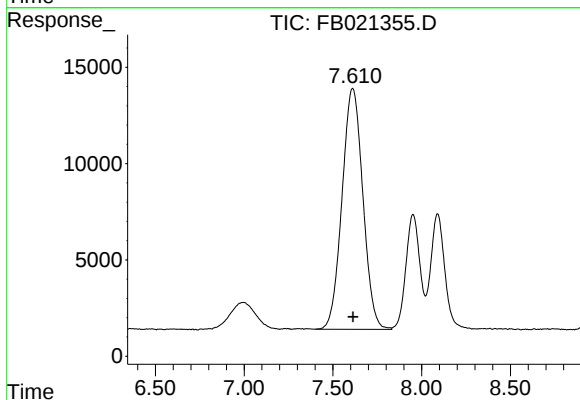


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: -0.003 min
Response: 1021732
Conc: 29.92 ng/ml

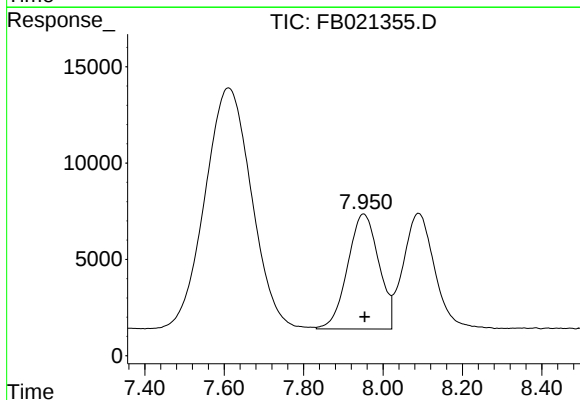


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: -0.003 min
Response: 325501
Conc: 9.98 ng/ml

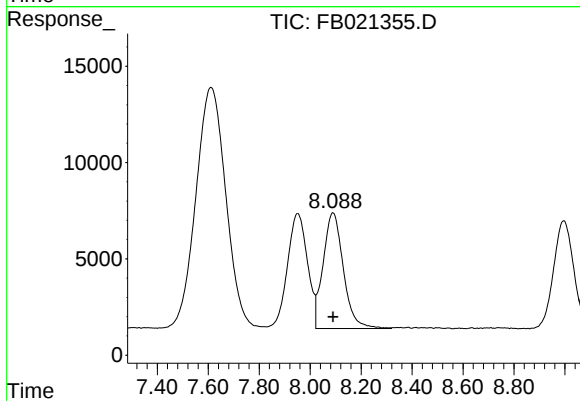


#4 Benzene

R.T.: 8.090 min
Delta R.T.: 0.000 min
Response: 332267
Conc: 9.63 ng/ml

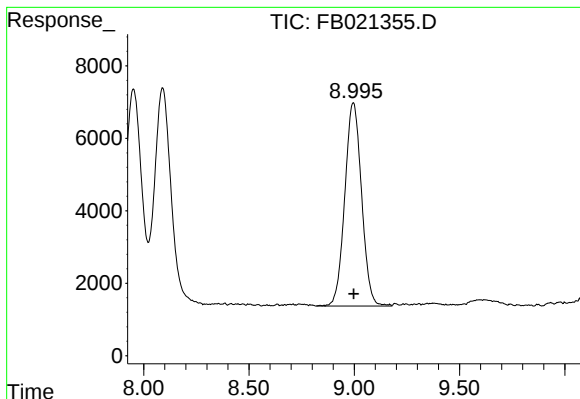


#5 AAA-TFT

R.T.: 8.996 min
Delta R.T.: -0.003 min
Response: 310857
Conc: 21.08 ng/ml

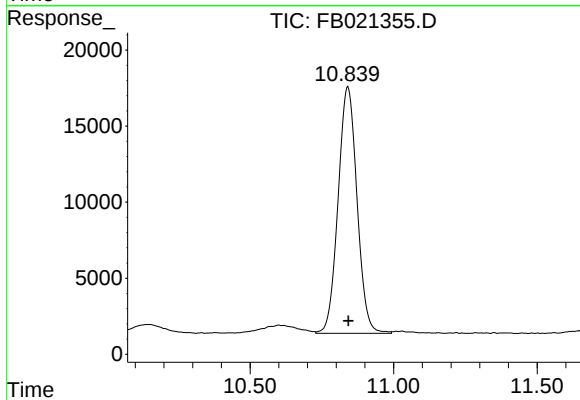


#6 Toluene

R.T.: 10.841 min
Delta R.T.: -0.002 min
Response: 743440
Conc: 31.37 ng/ml

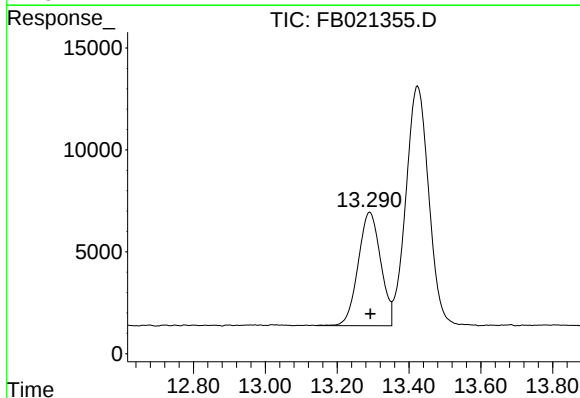


#7 Ethylbenzene

R.T.: 13.291 min
Delta R.T.: -0.002 min
Response: 241975
Conc: 10.36 ng/ml

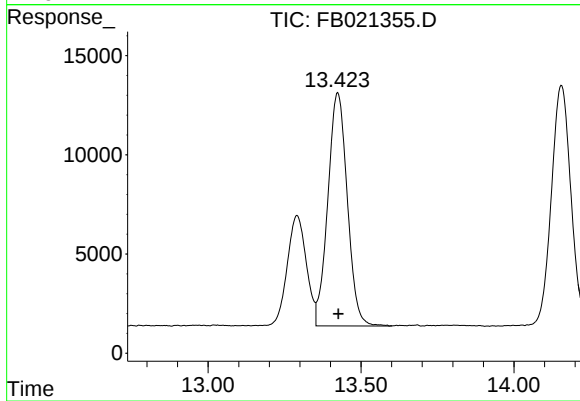


#8 m-Xylene

R.T.: 13.424 min
Delta R.T.: -0.002 min
Response: 521043
Conc: 20.88 ng/ml

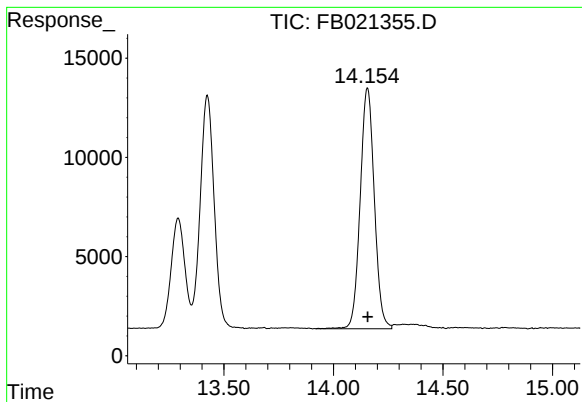

#9 O-Xylene

R.T.: 14.156 min
Delta R.T.: -0.001 min
Response: 544359
Conc: 20.87 ng/ml

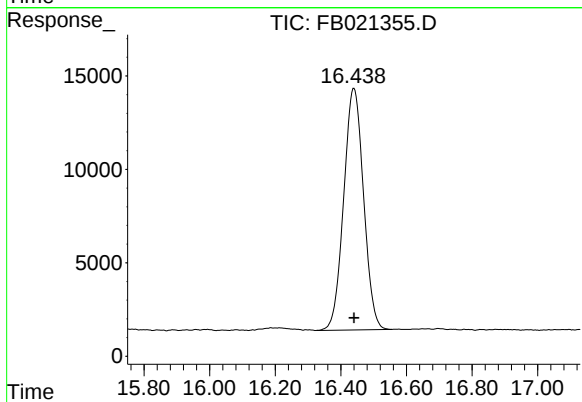

#10 1,2,4-Trimethylbenzene

R.T.: 16.440 min
Delta R.T.: 0.000 min
Response: 543765
Conc: 20.25 ng/ml